

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083023\
 Data File : VW026961.D
 Acq On : 30 Aug 2023 13:25
 Operator : SY/MD
 Sample : 04235-02
 Misc : 4.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYD9

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 09/01/2023

Quant Time: Aug 31 01:30:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Aug 31 01:29:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	515418	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	473426	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	229717	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	68572	8.093	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	32.360%		
7) Chloroethane-d5	2.899	69	65451	10.388	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	41.560%		
11) 1,1-Dichloroethene-d2	4.027	65	40276	9.665	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	38.640%#		
21) 2-Butanone-d5	7.081	46	70392	28.905	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	57.820%		
24) Chloroform-d	7.655	84	25031	1.447	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	5.800%#		
26) 1,2-Dichloroethane-d4	8.307	65	185716m	19.454	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	77.800%		
32) Benzene-d6	8.276	84	459362	14.079	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	56.320%		
36) 1,2-Dichloropropane-d6	9.270	67	164979	16.233	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	64.920%#		
41) Toluene-d8	10.325	98	395357	14.116	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	56.480%		
43) trans-1,3-Dichloroprop...	10.575	79	65835	15.689	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	62.760%		
47) 2-Hexanone-d5	10.922	63	27583m	25.828	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	51.660%		
56) 1,1,2,2-Tetrachloroeth...	12.684	84	1079m	0.134	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	0.520%#		
66) 1,2-Dichlorobenzene-d4	13.849	152	150065	18.251	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	73.000%#		
Target Compounds					Qvalue	
13) Acetone	4.131	43	11412	4.713	ug/L	97
14) Carbon disulfide	4.393	76	42965	1.568	ug/L	99
16) Methylene chloride	4.942	84	19066m	1.912	ug/L	
25) Chloroform	7.679	83	253291	14.985	ug/L	98
34) Trichloroethene	9.093	95	51843	5.904	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083023\
Data File : VW026961.D
Acq On : 30 Aug 2023 13:25
Operator : SY/MD
Sample : 04235-02
Misc : 4.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EZYD9

Quant Time: Aug 31 01:30:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Aug 31 01:29:13 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2023
Supervised By :Mahesh Dadoda 09/01/2023

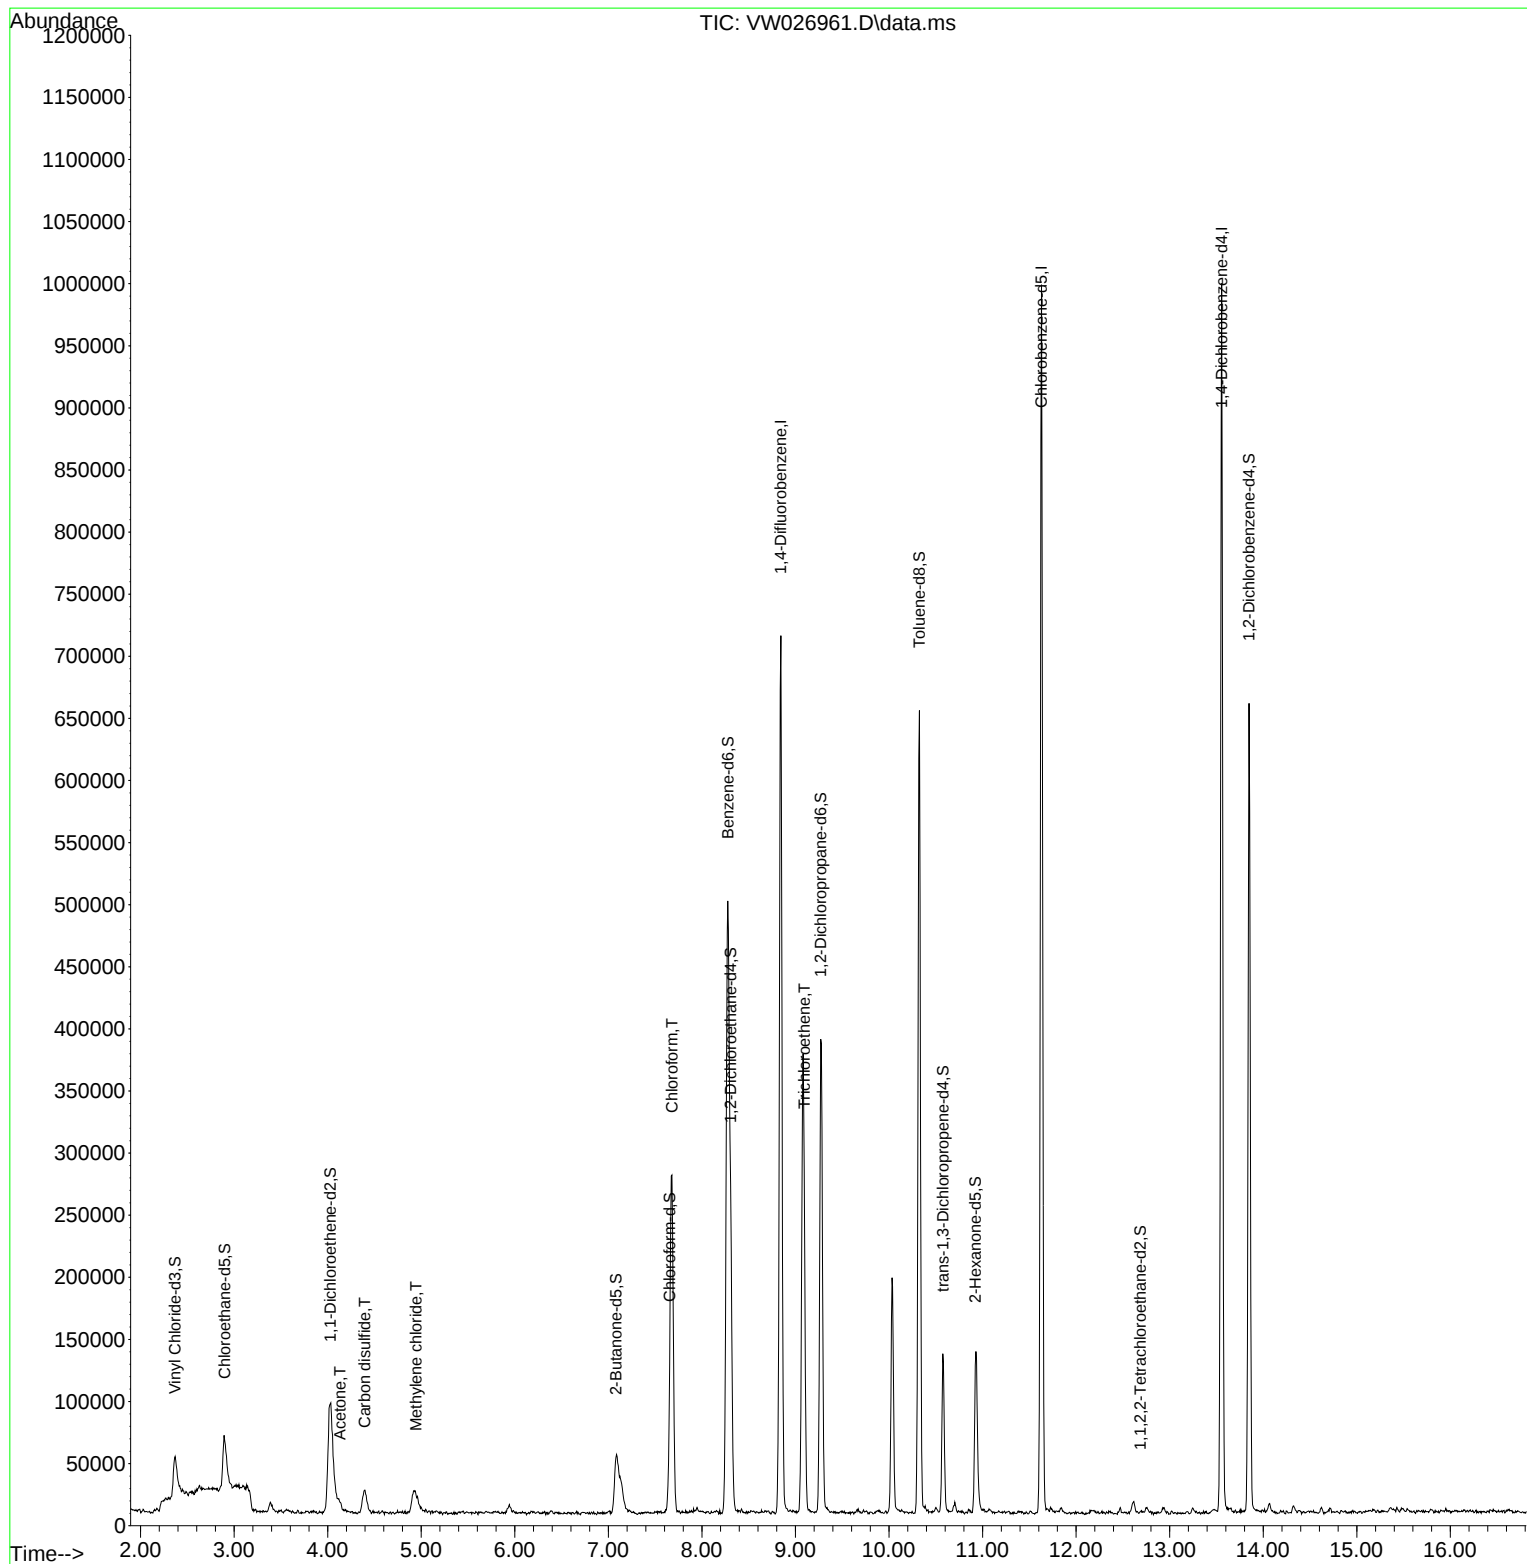

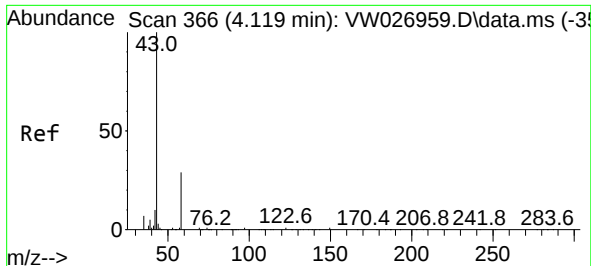





#13
Acetone
Concen: 4.713 ug/L
RT: 4.131 min Scan# 368
Delta R.T. 0.012 min
Lab File: VW026961.D
Acq: 30 Aug 2023 13:25

Instrument :
MSVOA_W
ClientSampleId :
EZYD9

Tgt Ion: 43 Resp: 1141
Ion Ratio Lower Upper
43 100
58 27.3 0.0 57.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/31/2023
Supervised By :Mahesh Dadoda 09/01/2023

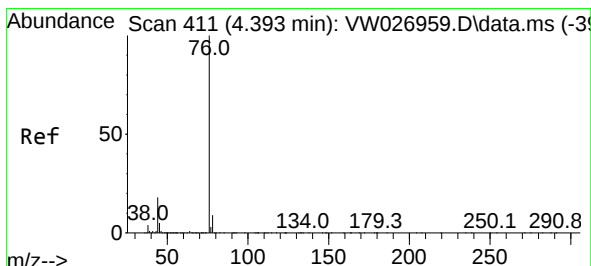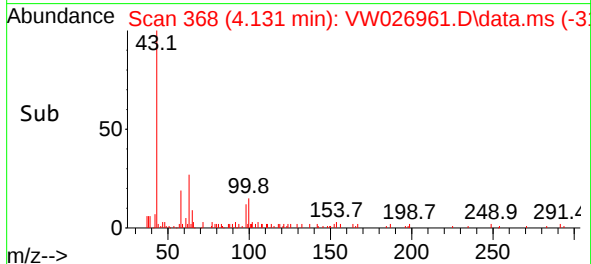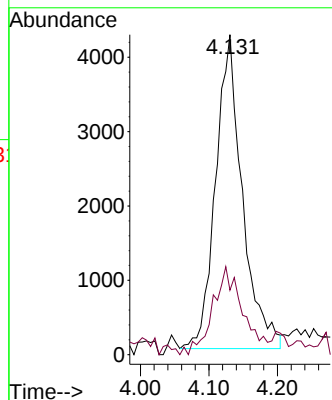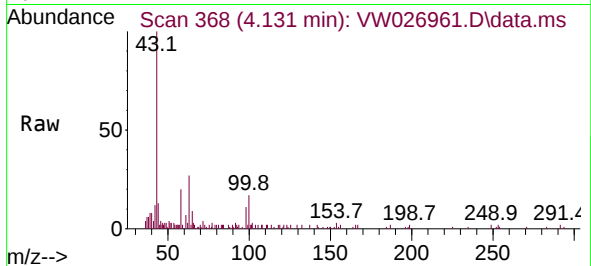

#14
Carbon disulfide
Concen: 1.568 ug/L
RT: 4.393 min Scan# 411
Delta R.T. 0.000 min
Lab File: VW026961.D
Acq: 30 Aug 2023 13:25


Tgt Ion: 76 Resp: 42965
Ion Ratio Lower Upper
76 100
78 9.2 7.1 10.7

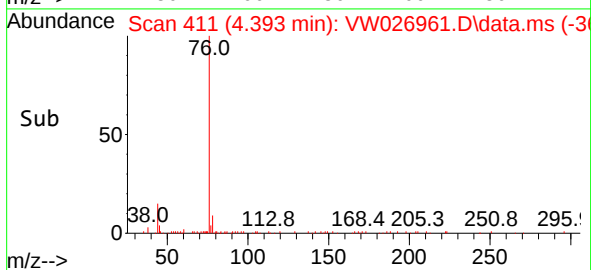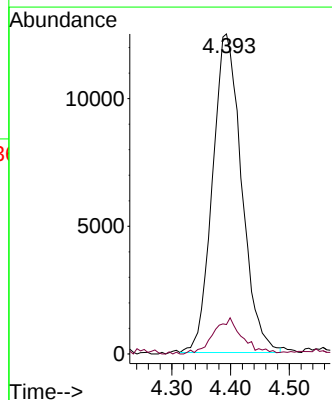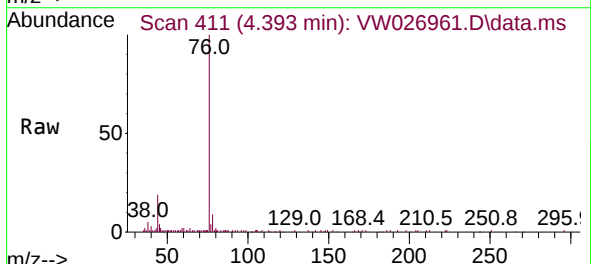

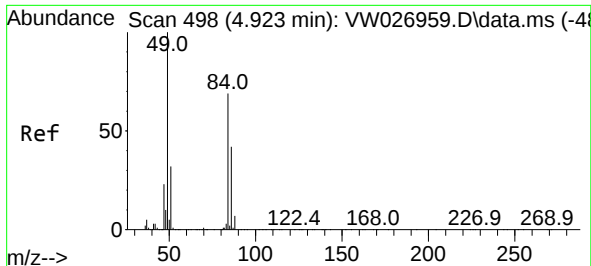

#16
Methylene chloride
Concen: 1.912 ug/L m
RT: 4.942 min Scan# 501
Delta R.T. 0.018 min
Lab File: VW026961.D
Acq: 30 Aug 2023 13:25




Instrument :
MSVOA_W
ClientSampleId :
EZYD9

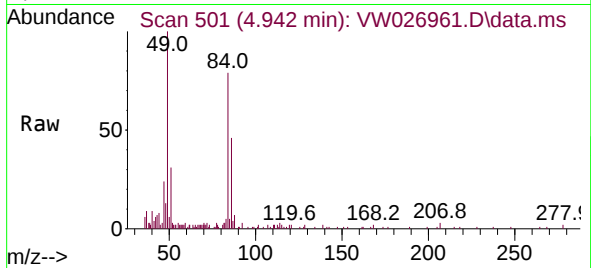

Tgt Ion: 84 Resp: 1906
Ion Ratio Lower Upper
84 100
86 57.6 43.5 80.9
49 126.0 96.0 178.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 08/31/2023
Supervised By :Mahesh Dadoda 09/01/2023

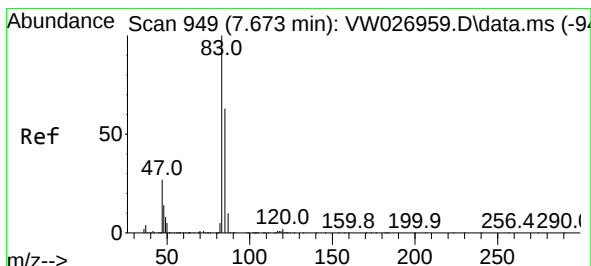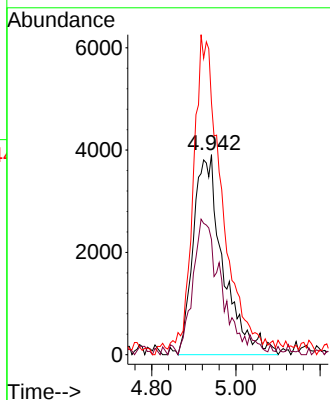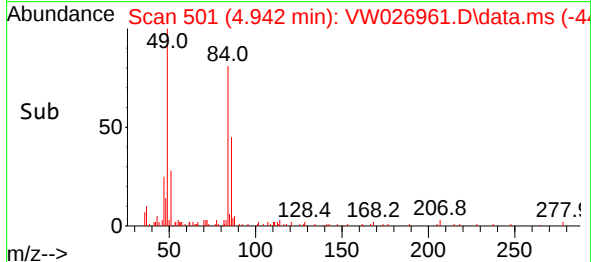

#25
Chloroform
Concen: 14.985 ug/L
RT: 7.679 min Scan# 950
Delta R.T. 0.006 min
Lab File: VW026961.D
Acq: 30 Aug 2023 13:25

Tgt Ion: 83 Resp: 253291
Ion Ratio Lower Upper
83 100
85 62.9 45.4 84.2

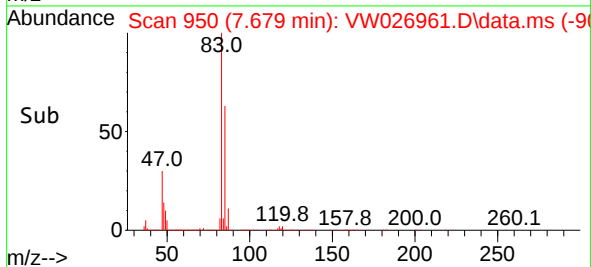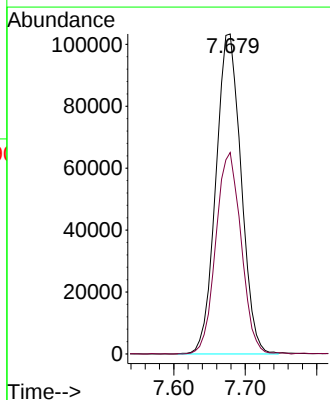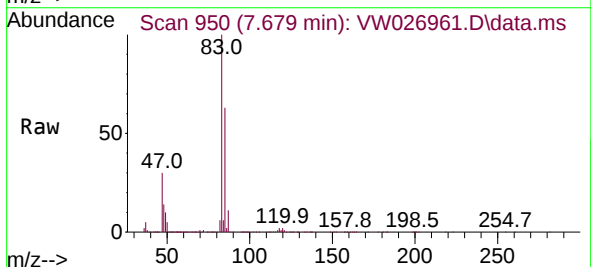

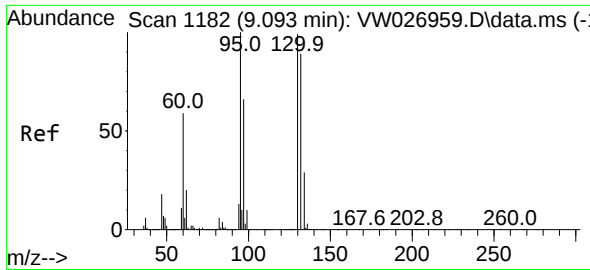

#34

Trichloroethene

Concen: 5.904 ug/L

RT: 9.093 min Scan# 1182

Delta R.T. 0.000 min

Lab File: VW026961.D


Acq: 30 Aug 2023 13:25

Instrument :

MSVOA_W

ClientSampleId :

EZYD9

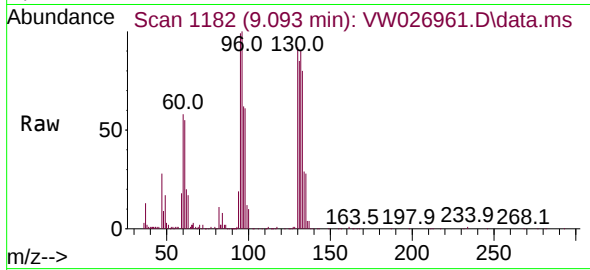

Tgt Ion: 95 Resp: 5184

Ion Ratio Lower Upper

95 100

97 62.1 44.6 82.8

132 90.8 66.4 123.2

130 92.9 67.3 125.1

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2023

Supervised By :Mahesh Dadoda 09/01/2023

