

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW083119\
 Data File : VW012424.D
 Acq On : 01 Sep 2019 02:46
 Operator : SY/VA
 Sample : K4516-01
 Misc : 6.53G/5ML/MSVOA W/SOIL
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 T1-S-B2-(0)

Quant Time: Sep 01 05:13:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 26 07:18:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	53548	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	82575	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	66025	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.55	152	20101	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	34941	54.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	109.78%	
35) Dibromofluoromethane	7.88	113	27365	55.52	ug/l	0.00
Spiked Amount 50.000			Recovery	=	111.04%	
50) Toluene-d8	10.32	98	99384	49.73	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.46%	
62) 4-Bromofluorobenzene	12.62	95	26627	37.80	ug/l	0.00
Spiked Amount 50.000			Recovery	=	75.60%	
Target Compounds						
16) Acetone	4.12	43	2156	13.250	ug/l #	86
20) Methylene Chloride	4.91	84	5669	9.216	ug/l	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW083119\
Data File : VW012424.D
Acq On : 01 Sep 2019 02:46
Operator : SY/VA
Sample : K4516-01
Misc : 6.53G/5ML/MSVOA W/SOIL
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
T1-S-B2-(0)

Quant Time: Sep 01 05:13:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 26 07:18:31 2019
Response via : Initial Calibration

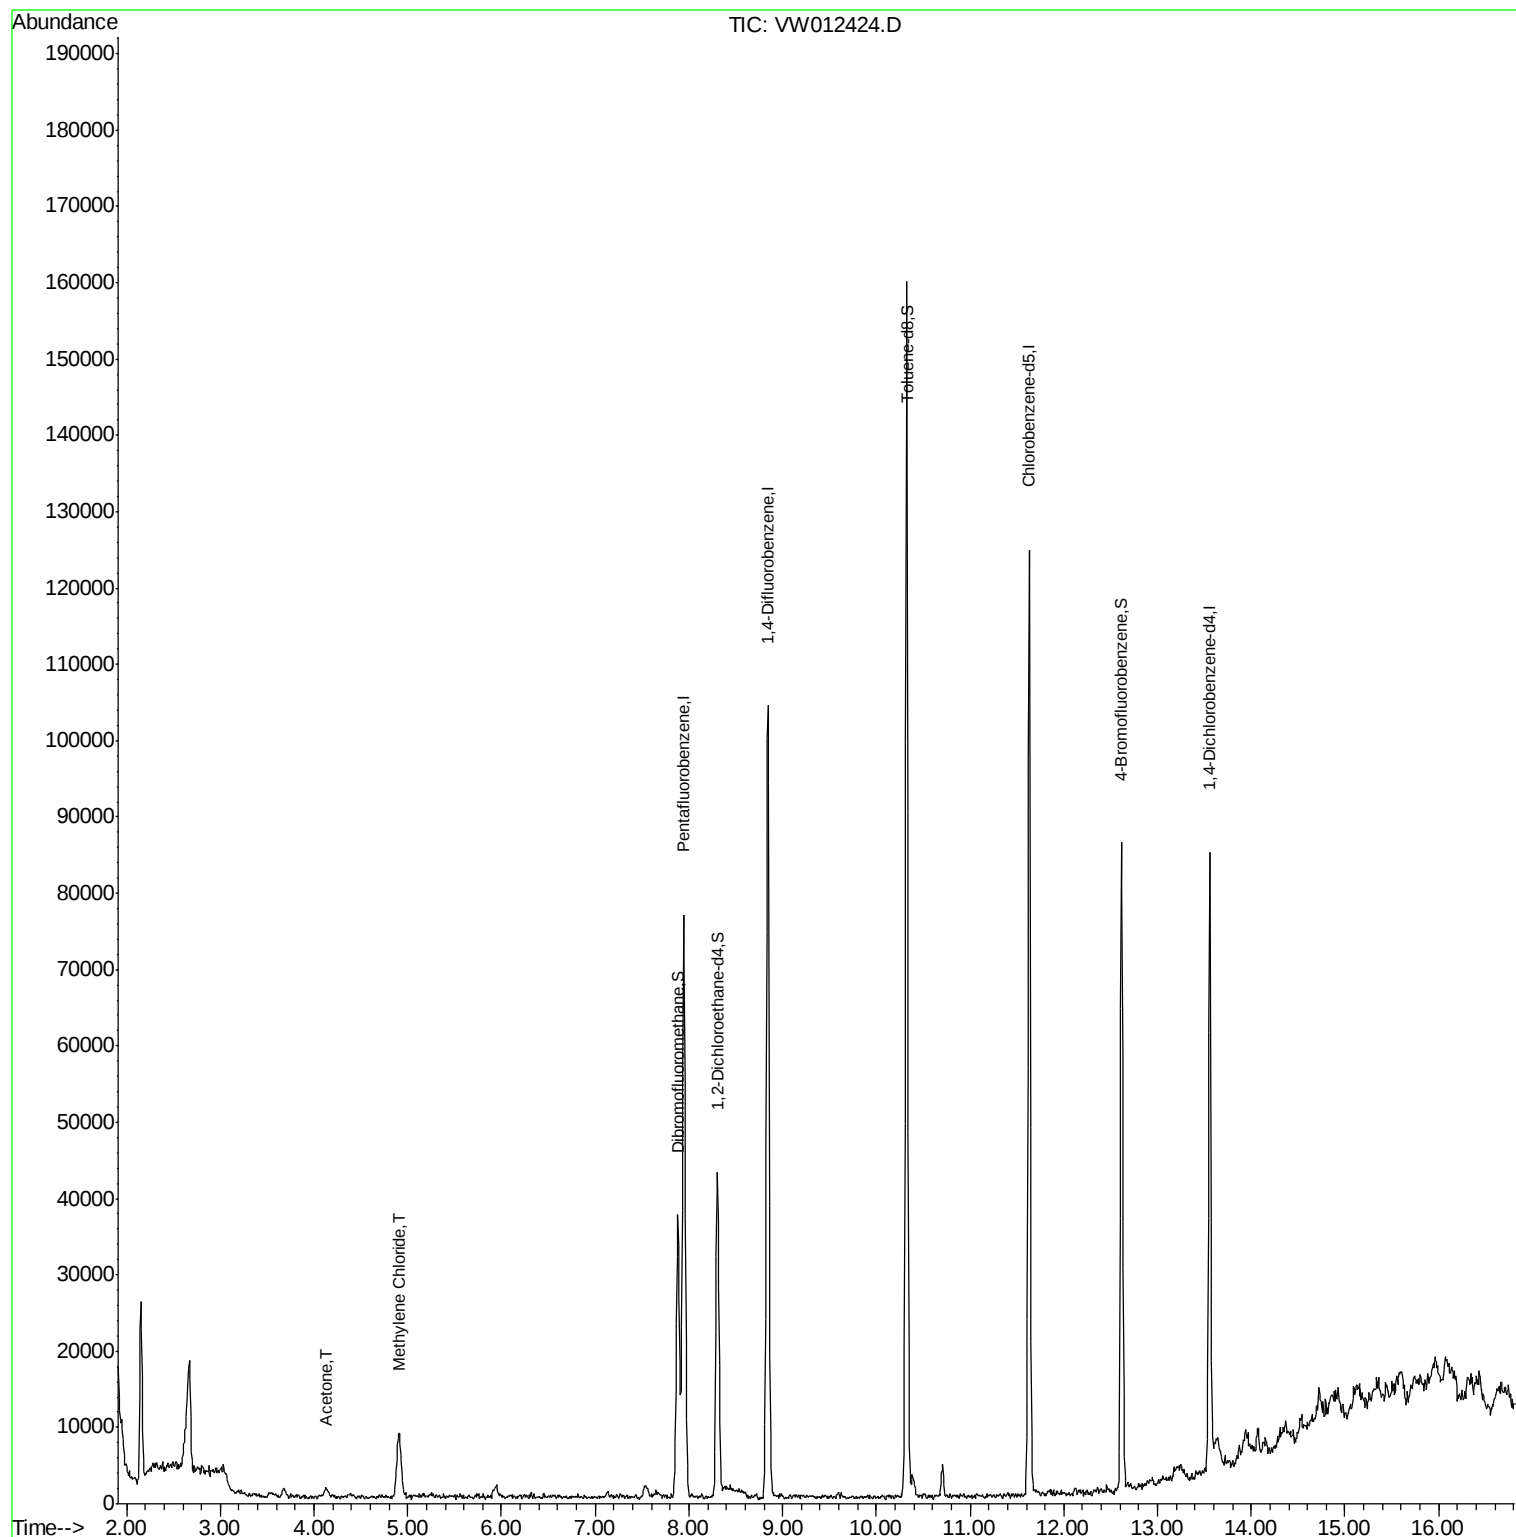



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW012424.D

Acq: 01 Sep 2019 02:46

Instrument :

MSVOA_W

ClientSampleId :


T1-S-B2-(0)

Tot Ion:168 Resp: 53548

Ion Ratio Lower Upper




168 100

99 63.5 49.2 73.8

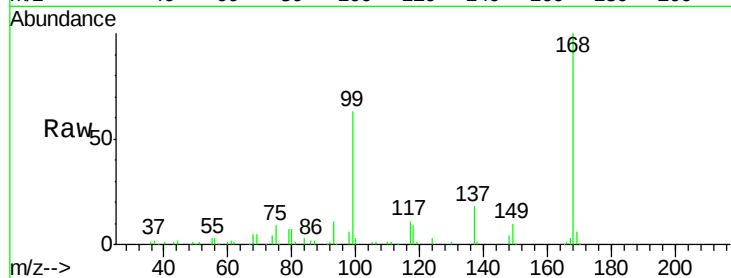

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

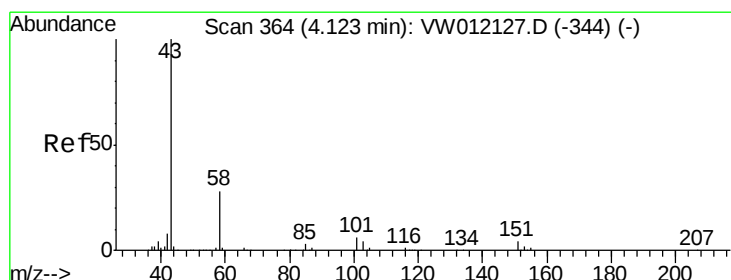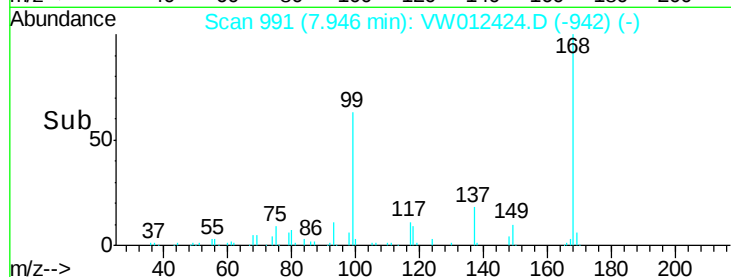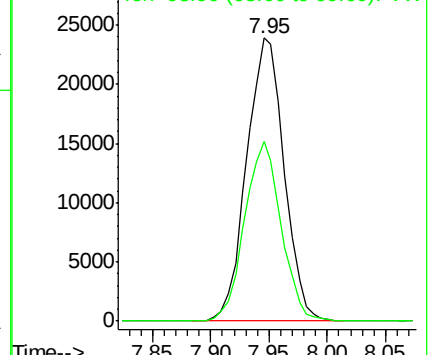

#16

Acetone

Concen: 13.250 ug/l

RT: 4.12 min Scan# 364

Delta R.T. -0.00 min

Lab File: VW012424.D


Acq: 01 Sep 2019 02:46

Tgt Ion: 43 Resp: 2156

Ion Ratio Lower Upper



43 100


58 35.6 22.4 33.6#

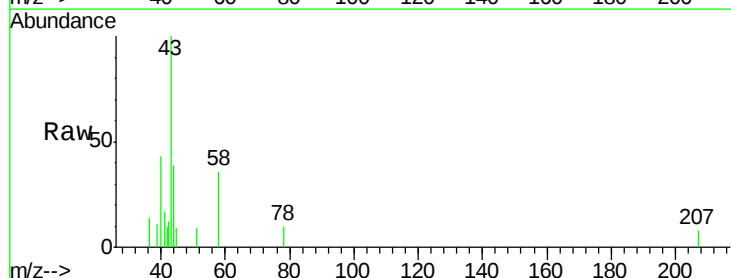

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

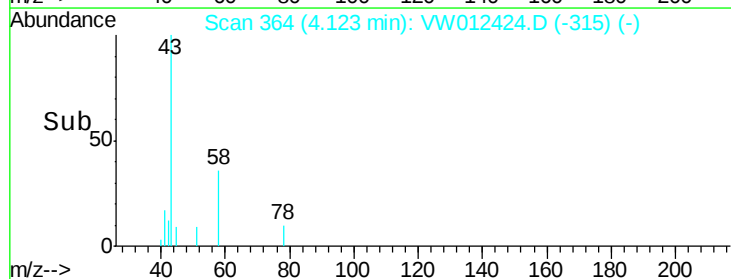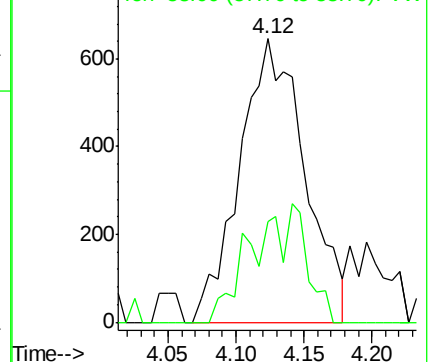


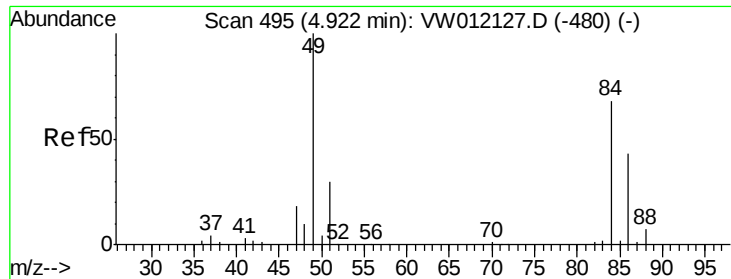




#20
Methvlene Chloride
Concen: 9.216 ug/l
RT: 4.91 min Scan# 493
Delta R.T. -0.01 min
Lab File: VW012424.D
Acq: 01 Sep 2019 02:46

Instrument :
MSVOA_W
ClientSampleId :
T1-S-B2-(0)

Tot Ion: 84 Resp: 5669
Ion Ratio Lower Upper
84 100
49 124.8 117.8 176.8
51 48.7 35.6 53.4
86 63.6 51.2 76.8

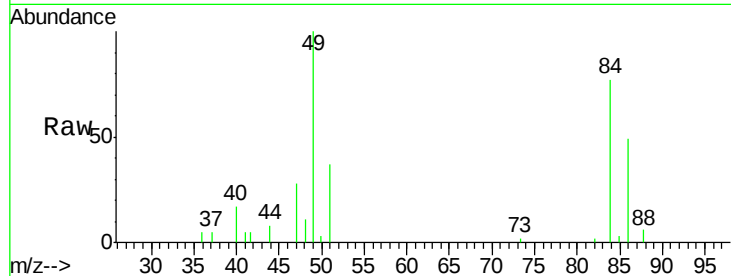


Abundance Ion 83.90 (83.60 to 84.60): VW
Ion 48.90 (48.60 to 49.60): VW
Ion 50.90 (50.60 to 51.60): VW
Ion 85.90 (85.60 to 86.60): VW

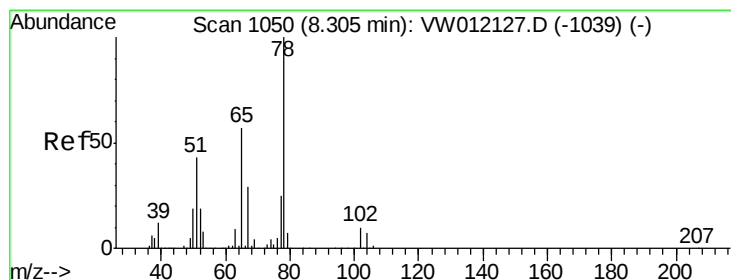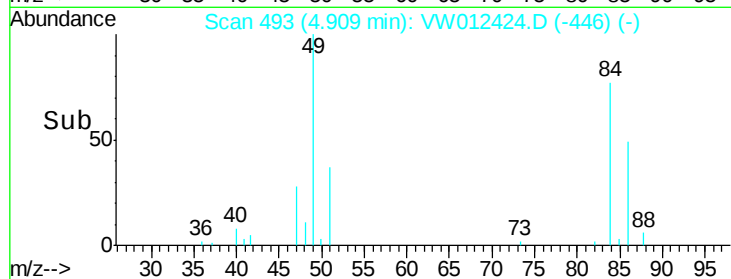
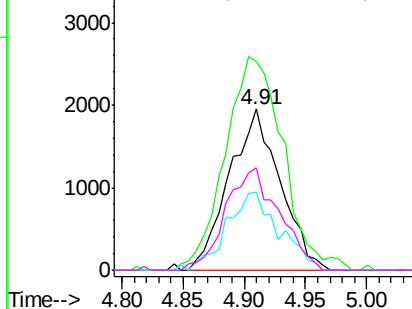



#33
1,2-Dichloroethane-d4
Concen: 54.891 ug/l
RT: 8.31 min Scan# 1050
Delta R.T. -0.00 min
Lab File: VW012424.D
Acq: 01 Sep 2019 02:46

Tgt Ion: 65 Resp: 34941
Ion Ratio Lower Upper
65 100
67 50.2 0.0 102.6

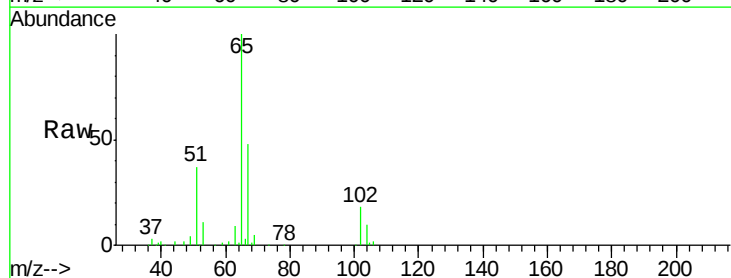

Abundance Ion 64.90 (64.60 to 65.60): VW
Ion 66.90 (66.60 to 67.60): VW

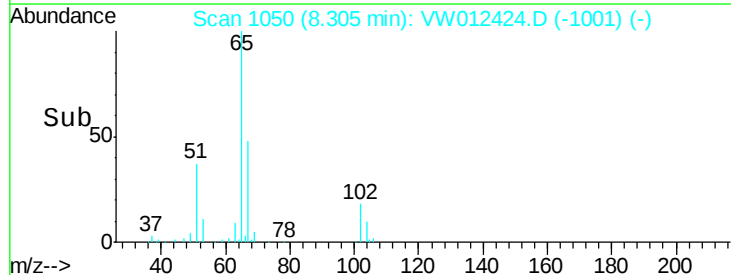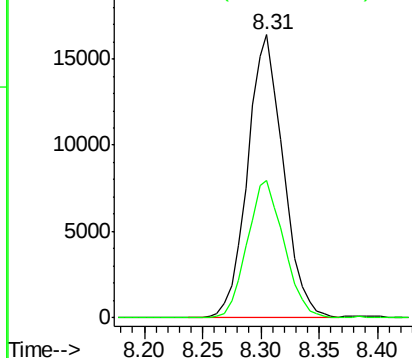


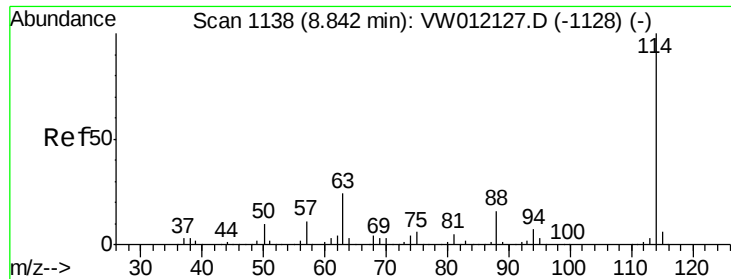




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VW012424.D
 Acq: 01 Sep 2019 02:46

Instrument :
 MSVOA_W
 ClientSampled :
 T1-S-B2-(0)

Tot Ion:114 Resp: 82575
 Ion Ratio Lower Upper
 114 100
 63 24.5 0.0 48.6
 88 16.3 0.0 32.2

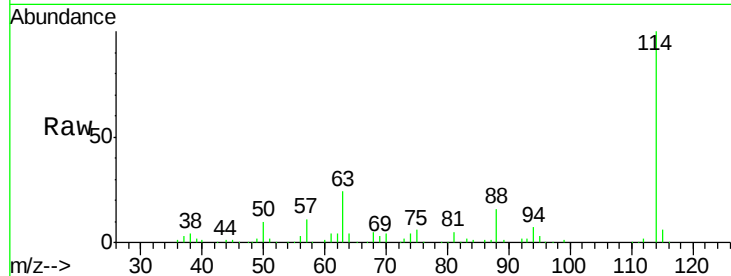


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

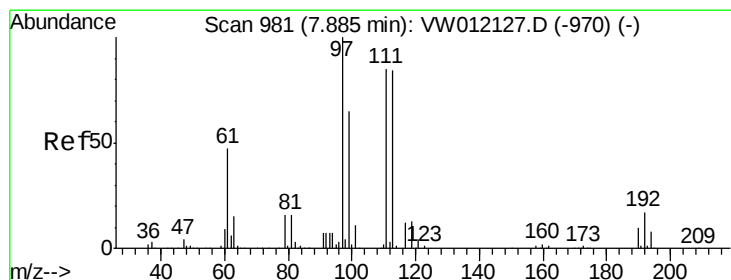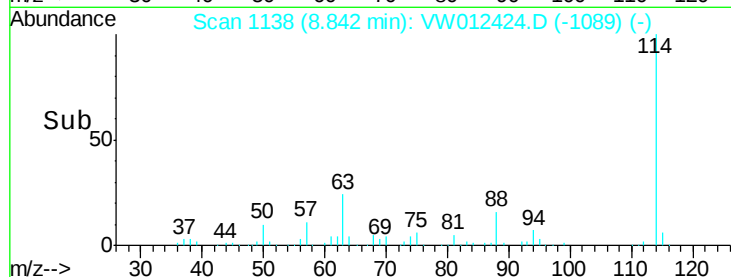
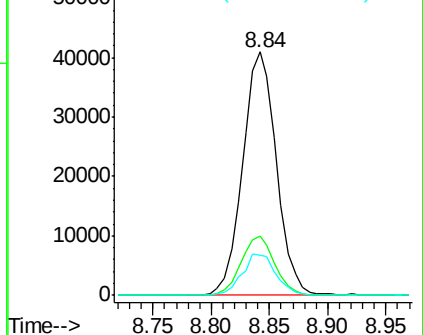



#35
 Dibromofluoromethane
 Concen: 55.519 ug/l
 RT: 7.88 min Scan# 980
 Delta R.T. -0.01 min
 Lab File: VW012424.D
 Acq: 01 Sep 2019 02:46

Tgt Ion:113 Resp: 27365
 Ion Ratio Lower Upper
 113 100
 111 100.3 82.7 124.1
 192 20.6 16.2 24.2

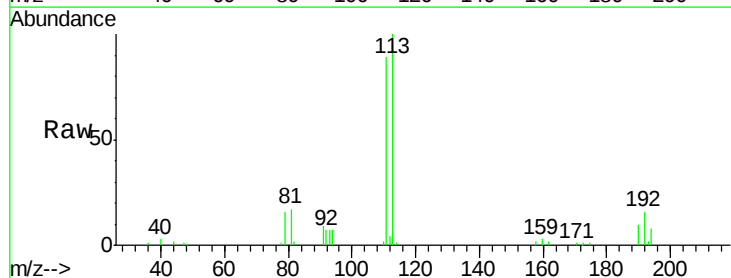

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

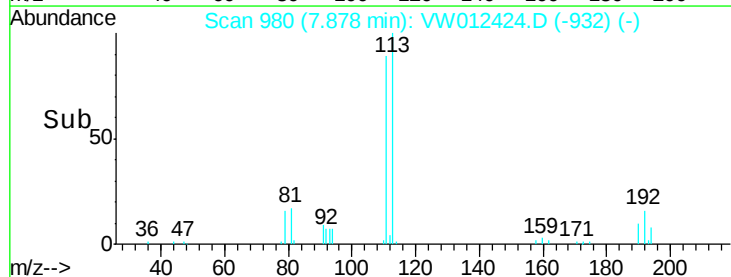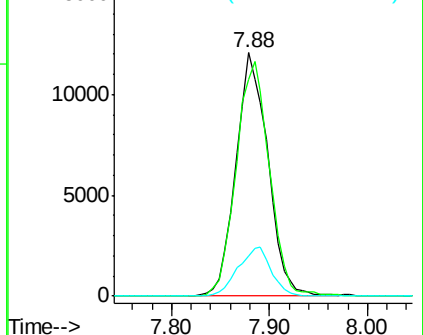

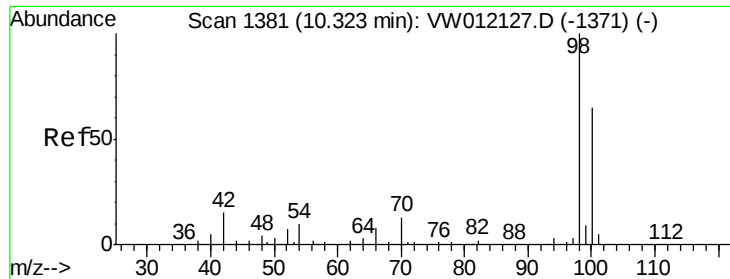

#50

Toluene-d8

Concen: 49.728 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.00 min

Lab File: VW012424.D

Acq: 01 Sep 2019 02:46

Instrument :

MSVOA_W

ClientSampleId :


T1-S-B2-(0)

Tot Ion: 98 Resp: 99384

Ion Ratio Lower Upper




98 100

100 65.9 52.4 78.6

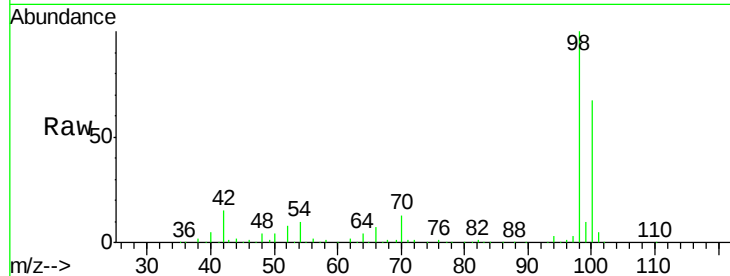

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

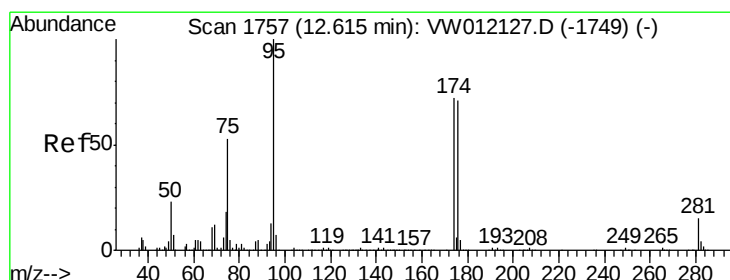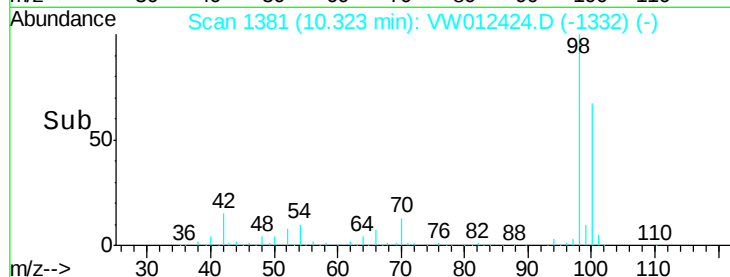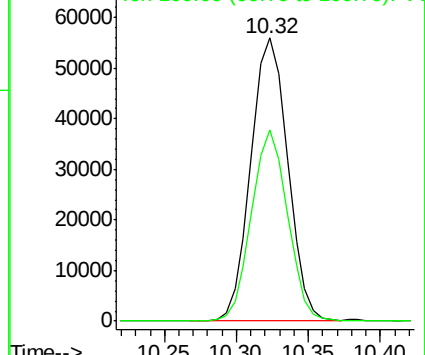

#62

4-Bromofluorobenzene

Concen: 37.797 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. -0.00 min

Lab File: VW012424.D

Acq: 01 Sep 2019 02:46


Tgt Ion: 95 Resp: 26627

Ion Ratio Lower Upper

95 100

174 77.4 0.0 150.8



176 74.0 0.0 148.6

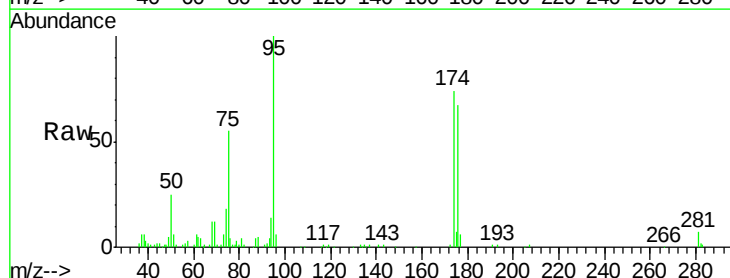


Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW



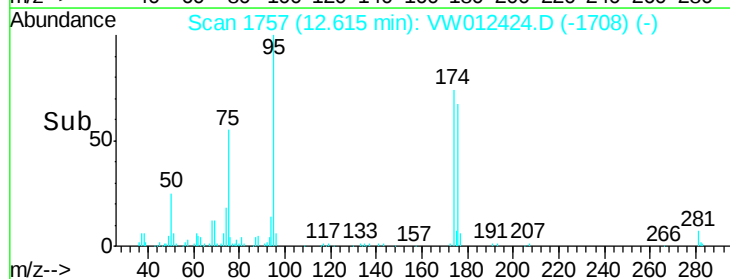
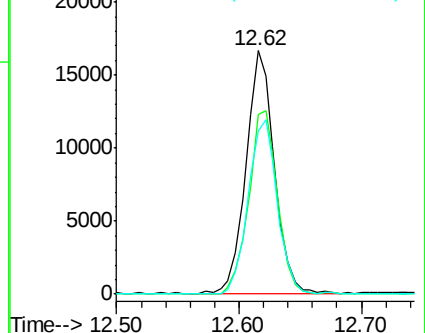


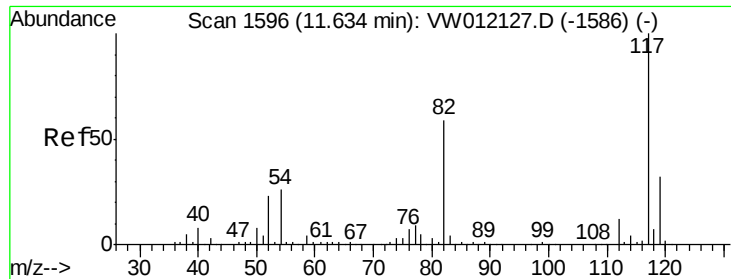

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1595
Delta R.T. -0.01 min
Lab File: VW012424.D
Acq: 01 Sep 2019 02:46

Instrument :
MSVOA_W
ClientSampleId :
T1-S-B2-(0)

Tot Ion:117 Resp: 66025
Ion Ratio Lower Upper
117 100
82 60.0 47.4 71.2
119 32.2 25.4 38.2

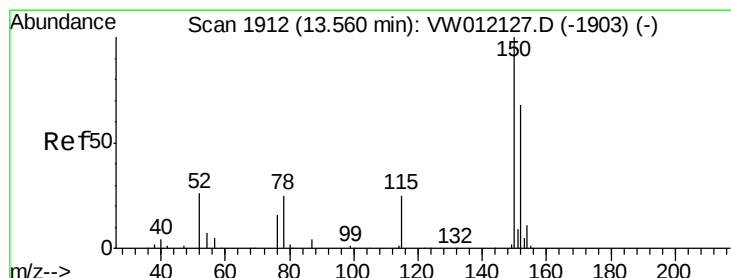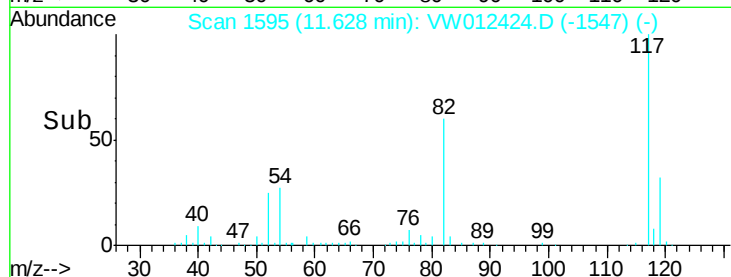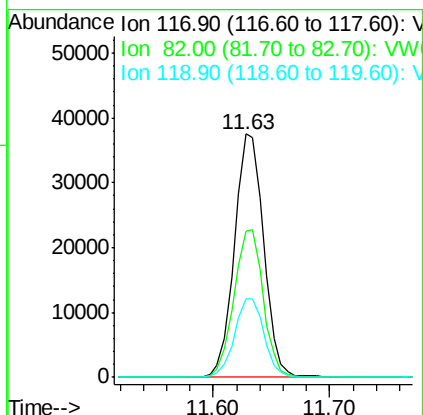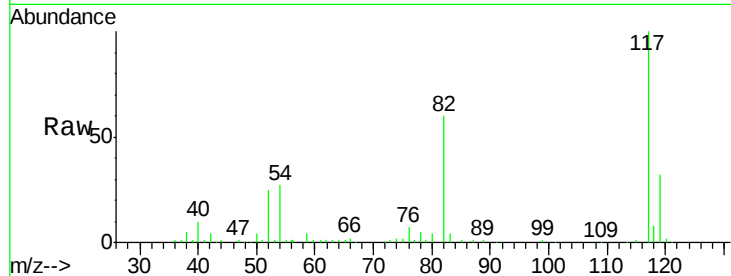

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.55 min Scan# 1911
Delta R.T. -0.01 min
Lab File: VW012424.D
Acq: 01 Sep 2019 02:46

Tgt Ion:152 Resp: 20101
Ion Ratio Lower Upper
152 100
115 61.5 30.1 90.3
150 155.2 0.0 345.8

