


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW083119\
 Data File : VW012413.D
 Acq On : 31 Aug 2019 21:09
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
 Title : SW846 8260
 Last Update : Mon Aug 26 07:18:31 2019

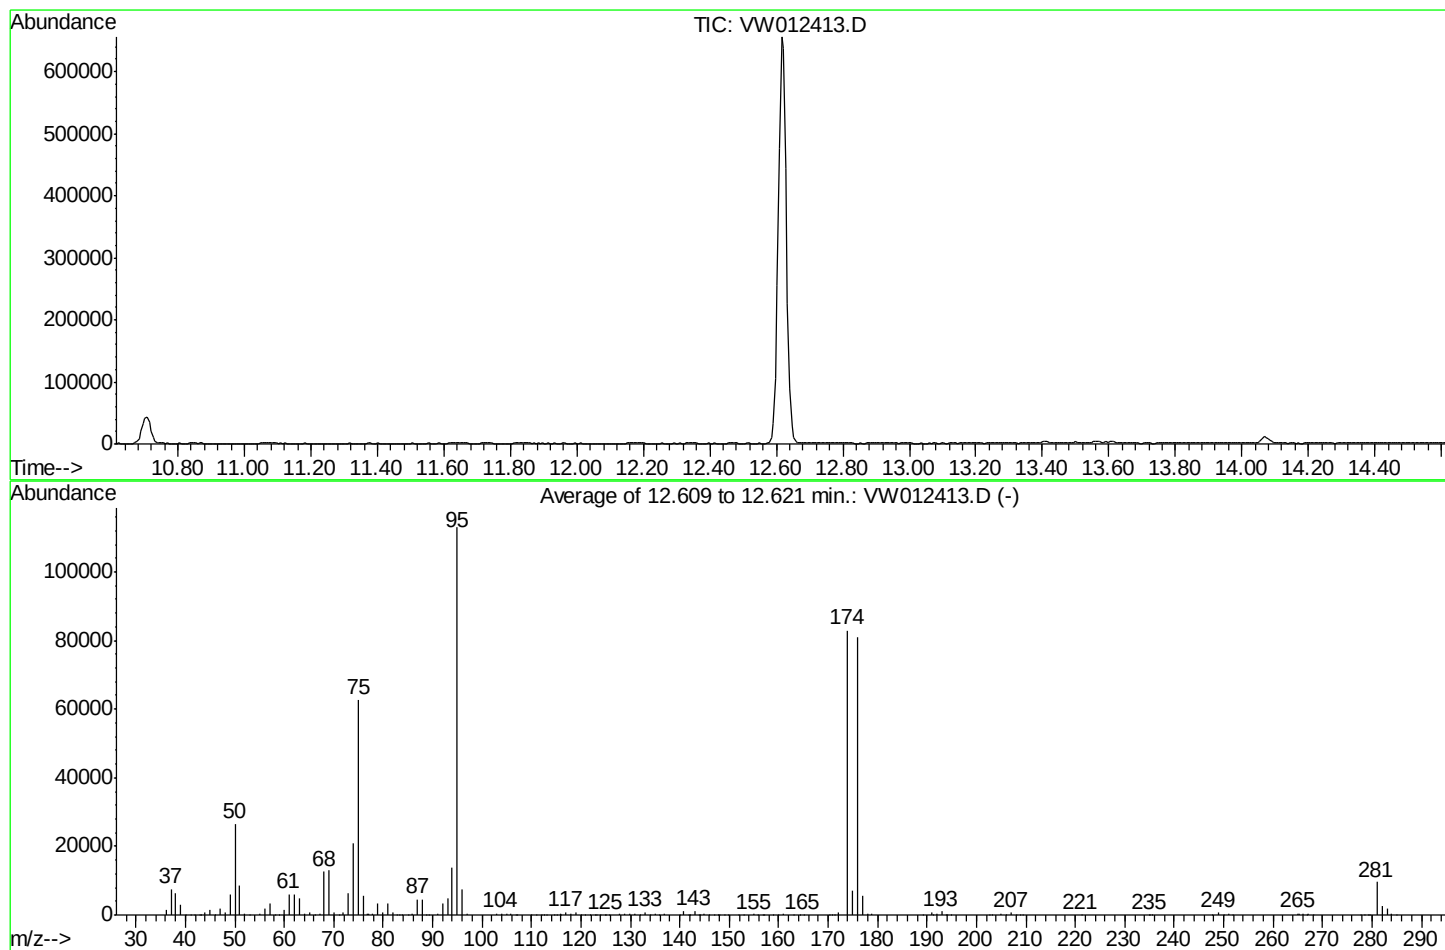

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	26608	PASS
75	95	30	60	55.5	62738	PASS
95	95	100	100	100.0	112986	PASS
96	95	5	9	6.8	7627	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.4	82965	PASS
175	174	5	9	8.4	6965	PASS
176	174	95	101	97.6	80946	PASS
177	176	5	9	7.0	5634	PASS