

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW083120\
 Data File : VW016418.D
 Acq On : 31 Aug 2020 18:05
 Operator : SY/VA
 Sample : L3848-04
 Misc : 4.53G/5ML/MSVOA W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 LINDEN-BH-02-A

Quant Time: Sep 01 04:04:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082820S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 28 15:01:43 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	140274	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	236139	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	218731	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	103053	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	77448	55.15	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.30%	
35) Dibromofluoromethane	7.89	113	76591	51.24	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.48%	
50) Toluene-d8	10.33	98	279394	49.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.84%	
62) 4-Bromofluorobenzene	12.62	95	105555	50.29	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.58%	
Target Compounds						
16) Acetone	4.12	43	3340	14.007	ug/l	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW083120\
Data File : VW016418.D
Acq On : 31 Aug 2020 18:05
Operator : SY/VA
Sample : L3848-04
Misc : 4.53G/5ML/MSVOA W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
LINDEN-BH-02-A

Quant Time: Sep 01 04:04:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W082820S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 28 15:01:43 2020
Response via : Initial Calibration

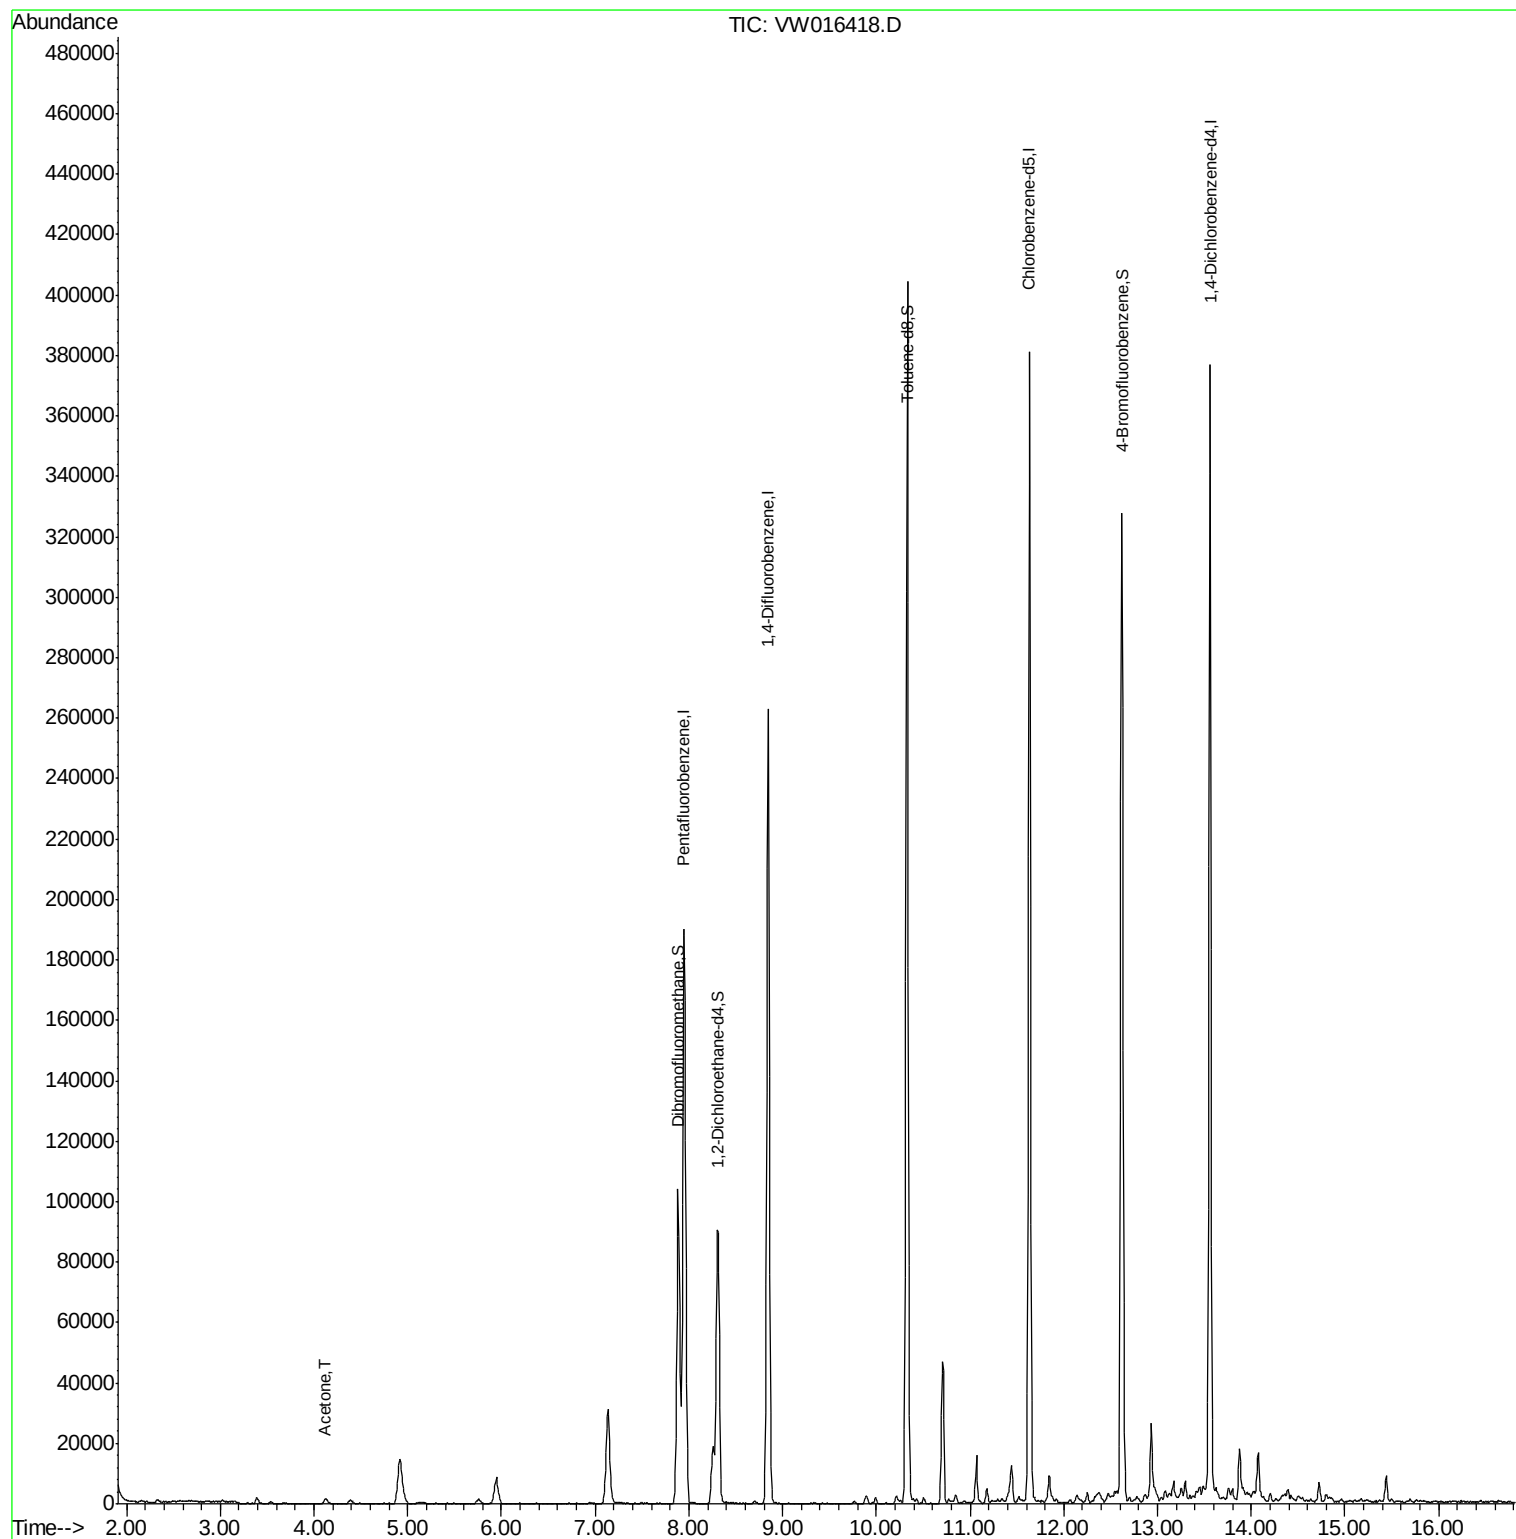

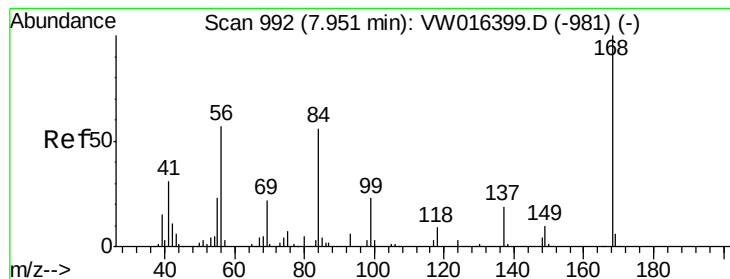

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.01 min

Lab File: VW016418.D

Acq: 31 Aug 2020 18:05

Instrument :

MSVOA_W

ClientSampleId :


LINDEN-BH-02-A

Tot Ion:168 Resp: 140274

Ion Ratio Lower Upper




168 100

99 62.3 49.0 73.4

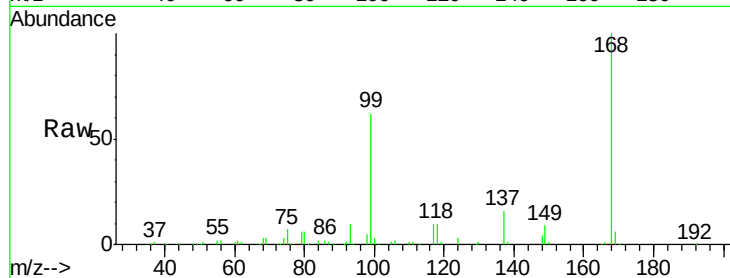

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

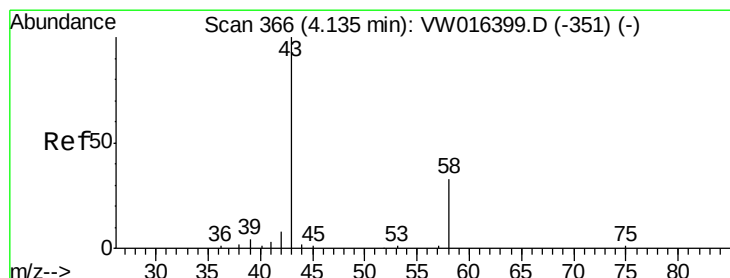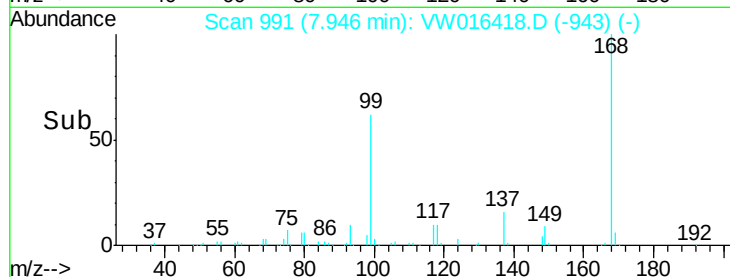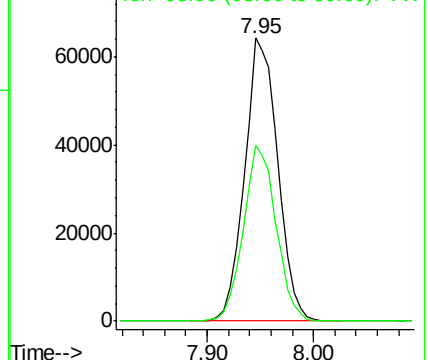

#16

Acetone

Concen: 14.007 ug/l

RT: 4.12 min Scan# 363

Delta R.T. -0.02 min

Lab File: VW016418.D


Acq: 31 Aug 2020 18:05

Tgt Ion: 43 Resp: 3340

Ion Ratio Lower Upper



43 100


58 27.0 26.6 39.8

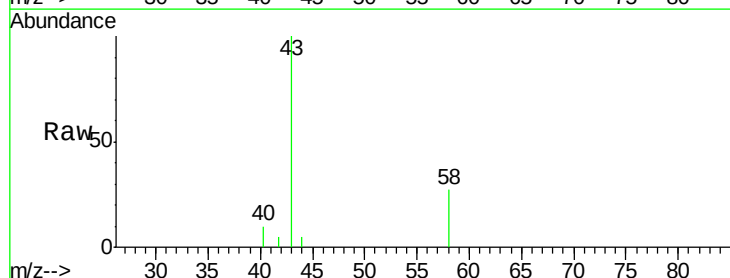

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW



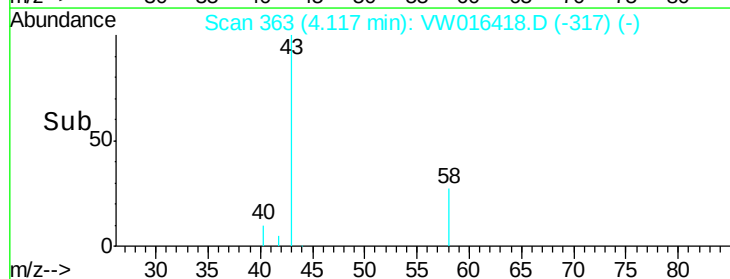
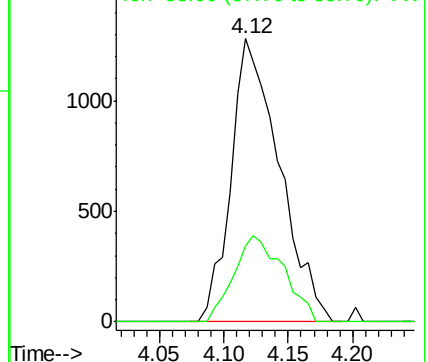


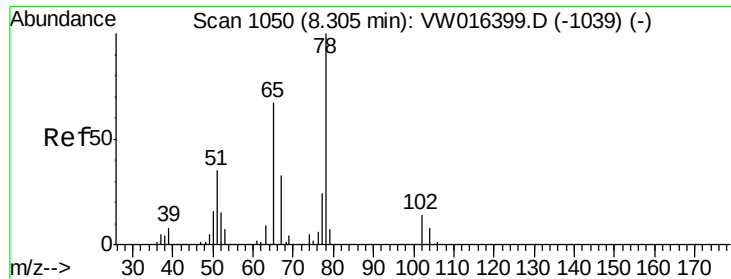

#33
 1,2-Dichloroethane-d4
 Concen: 55.154 ug/l
 RT: 8.31 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: VW016418.D
 Acq: 31 Aug 2020 18:05




Instrument :
 MSVOA_W
 ClientSampleId :
 LINDEN-BH-02-A


Tot Ion: 65 Resp: 77448
 Ion Ratio Lower Upper
 65 100
 67 50.6 0.0 100.2

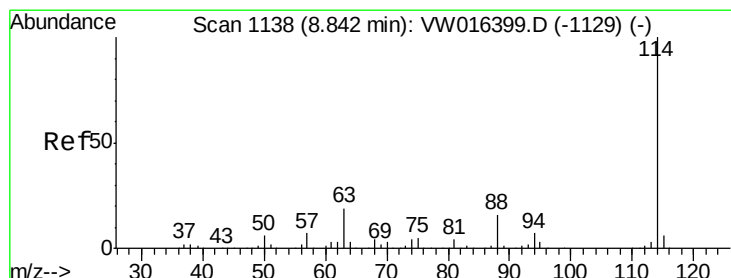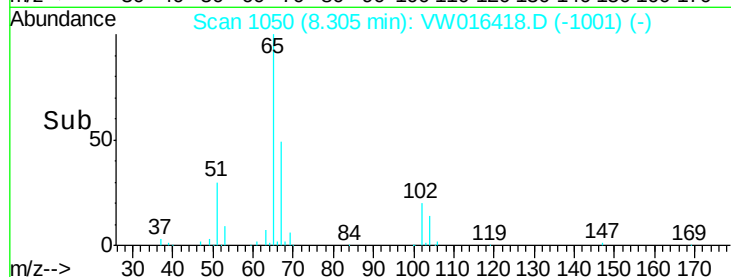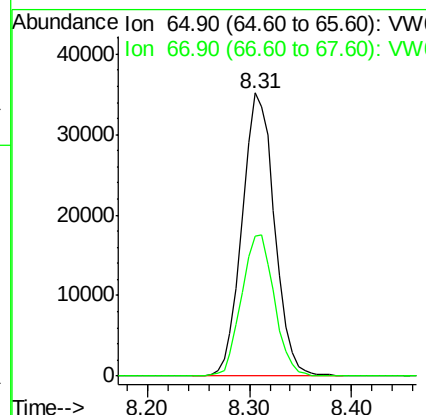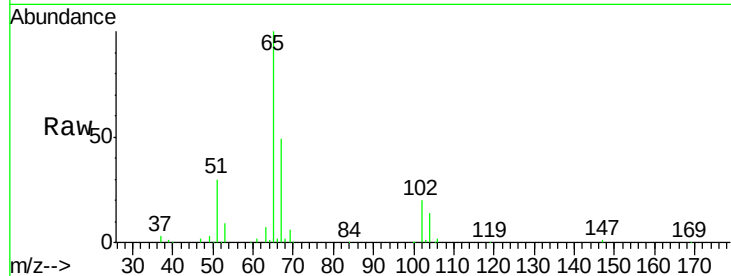

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW016418.D
 Acq: 31 Aug 2020 18:05

Tgt Ion: 114 Resp: 236139
 Ion Ratio Lower Upper
 114 100
 63 19.3 0.0 37.8
 88 15.9 0.0 31.2

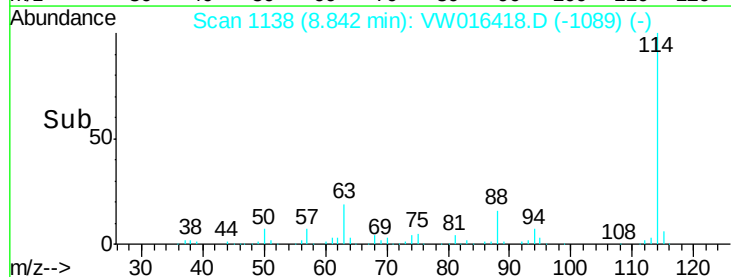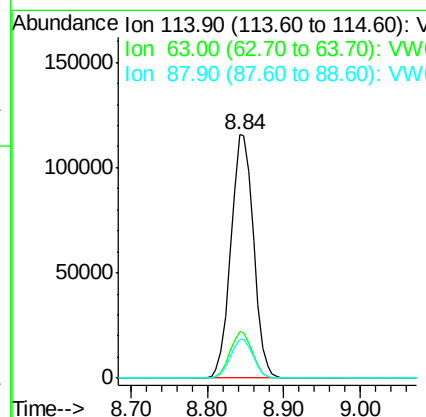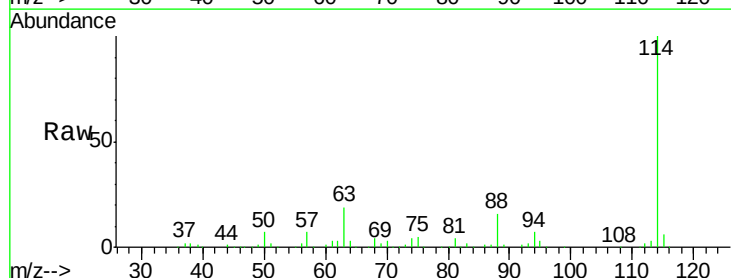

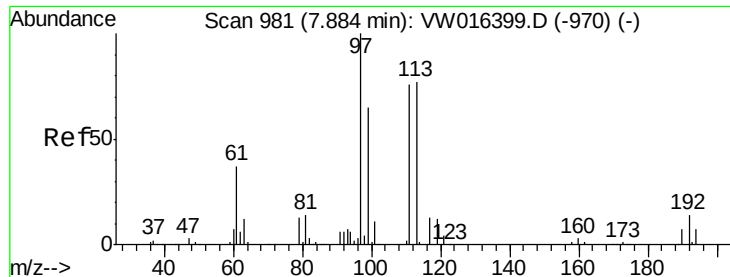

#35

Dibromofluoromethane

Concen: 51.242 ug/l

RT: 7.89 min Scan# 982

Delta R.T. 0.01 min

Lab File: VW016418.D

Acq: 31 Aug 2020 18:05

Instrument :

MSVOA_W

ClientSampleId :

LINDEN-BH-02-A


Tot Ion:113 Resp: 76591

Ion Ratio Lower Upper

113 100

111 101.2 82.1 123.1




192 19.0 15.5 23.3

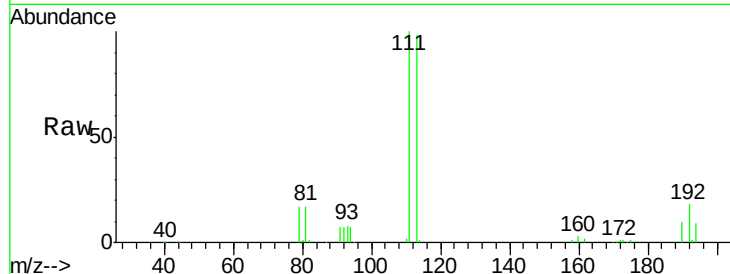

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

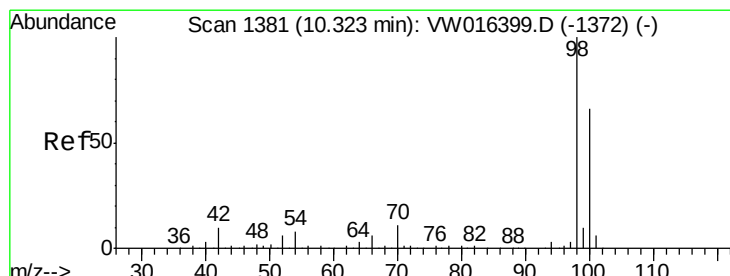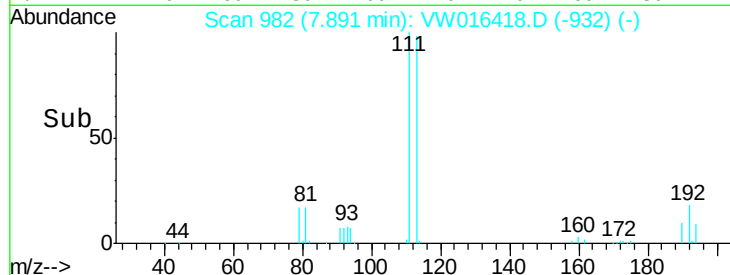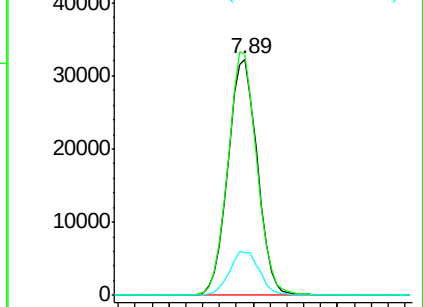

#50

Toluene-d8

Concen: 49.918 ug/l

RT: 10.33 min Scan# 1382

Delta R.T. 0.01 min

Lab File: VW016418.D


Acq: 31 Aug 2020 18:05

Tgt Ion: 98 Resp: 279394

Ion Ratio Lower Upper



98 100


100 66.7 52.6 78.8

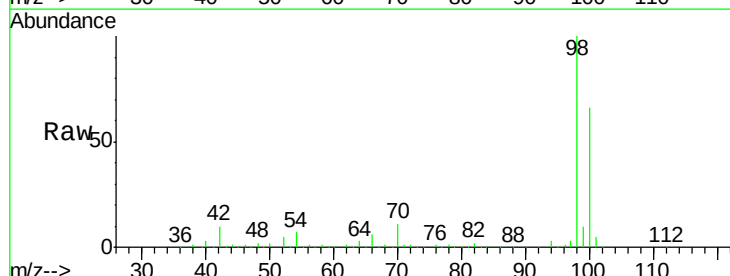

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

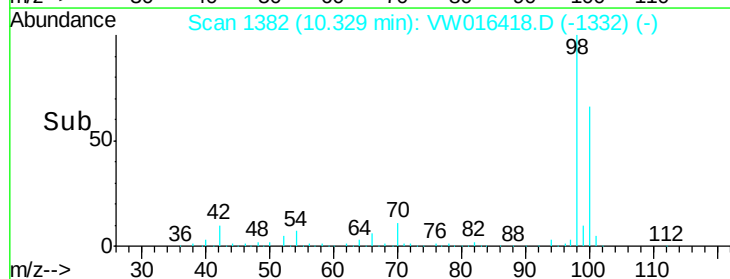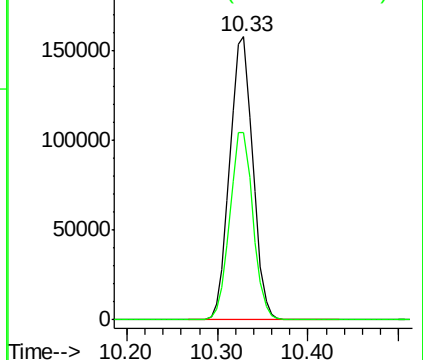

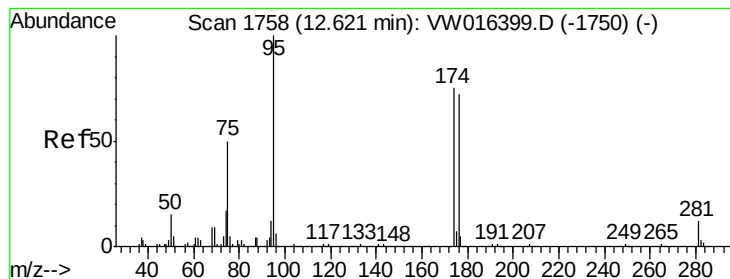

#62

4-Bromofluorobenzene

Concen: 50.292 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW016418.D

Acq: 31 Aug 2020 18:05

Instrument :

MSVOA_W

ClientSampleId :

LINDEN-BH-02-A


Tot Ion: 95 Resp: 105555

Ion Ratio Lower Upper

95 100

174 77.0 0.0 152.0




176 74.4 0.0 145.6

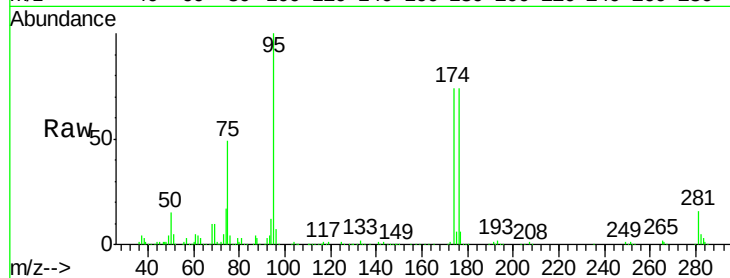

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

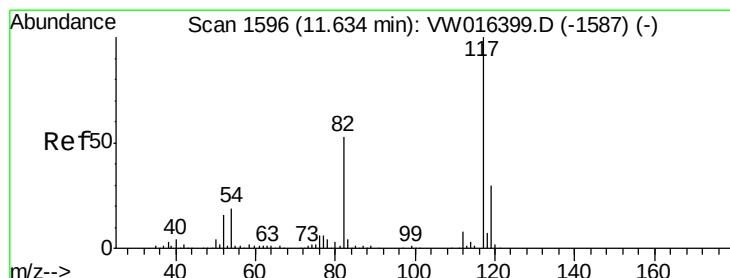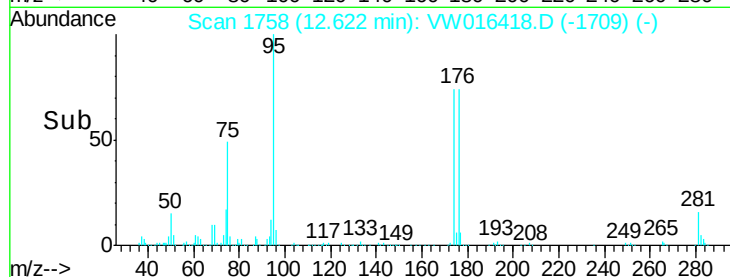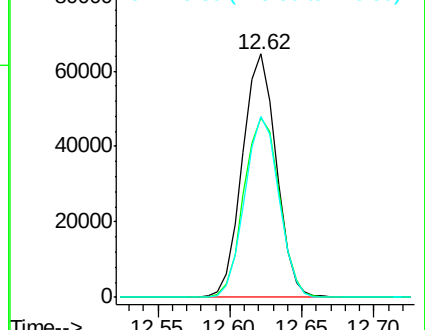

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. 0.00 min

Lab File: VW016418.D

Acq: 31 Aug 2020 18:05


Tgt Ion: 117 Resp: 218731

Ion Ratio Lower Upper

117 100

82 54.2 42.2 63.4



119 31.8 24.2 36.4

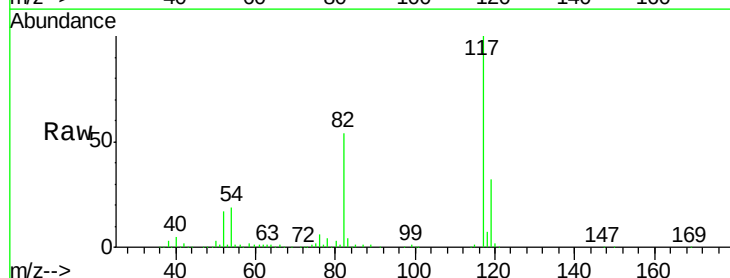


Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW

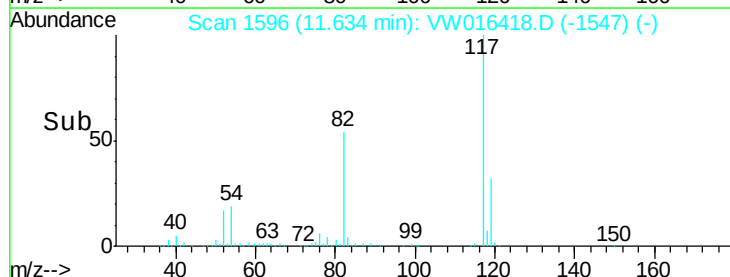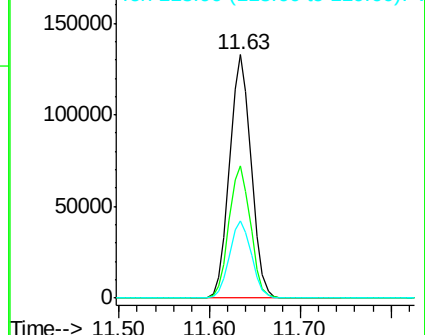

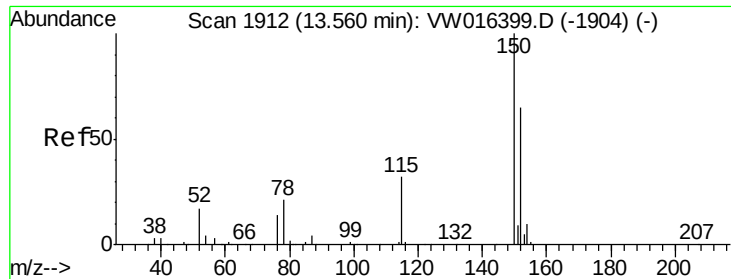

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. 0.00 min

Lab File: VW016418.D

Acq: 31 Aug 2020 18:05

Instrument :

MSVOA_W

ClientSampleId :

LINDEN-BH-02-A


Tot Ion:152 Resp: 103053

Ion Ratio Lower Upper

152 100

115 62.2 30.9 92.5

150 152.6 0.0 351.0

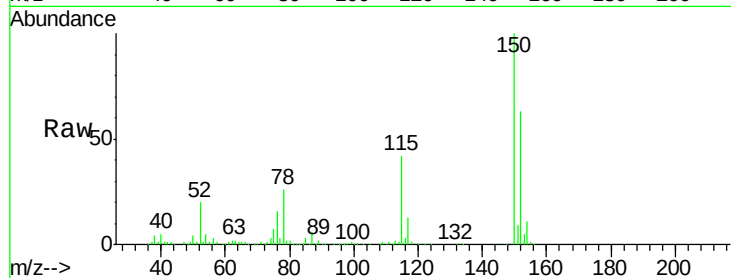

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

