




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083123\
 Data File : VW026977.D
 Acq On : 31 Aug 2023 15:02
 Operator : SY/MD
 Sample : VIBLK502
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK502

Manual IntegrationsAPPROVED

Quant Time: Sep 01 00:48:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 01 00:44:05 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/01/2023
 Supervised By :Mahesh Dadoda 09/05/2023

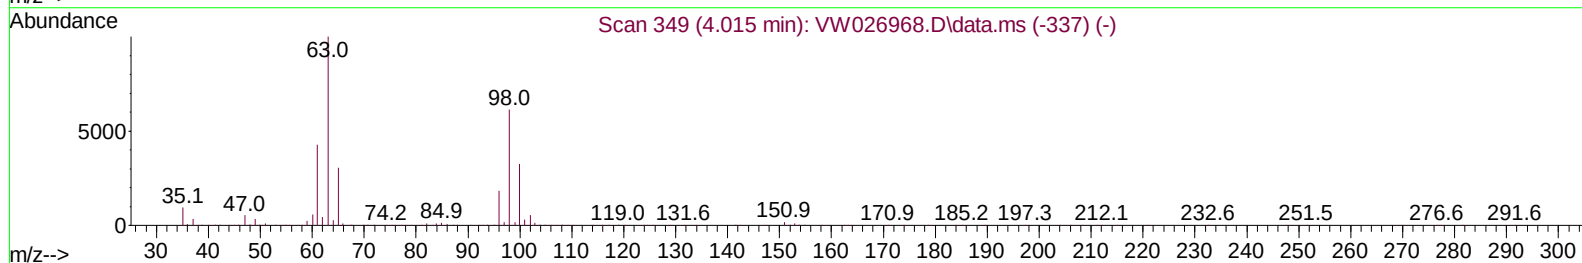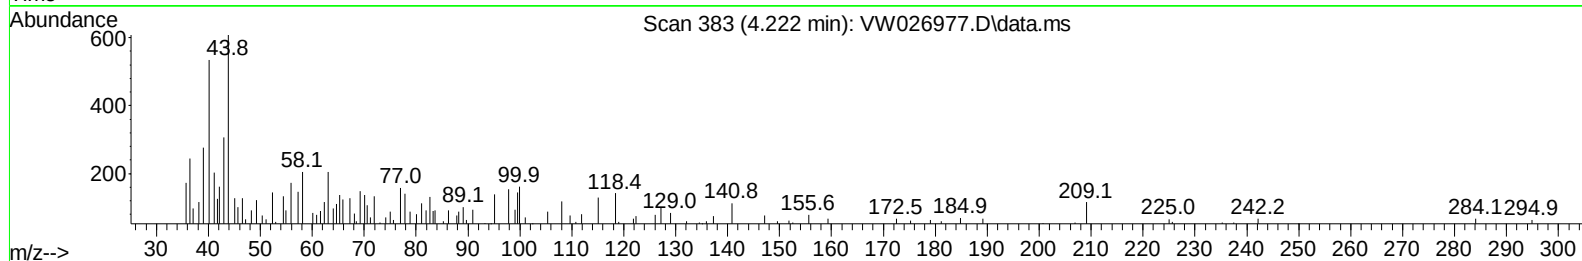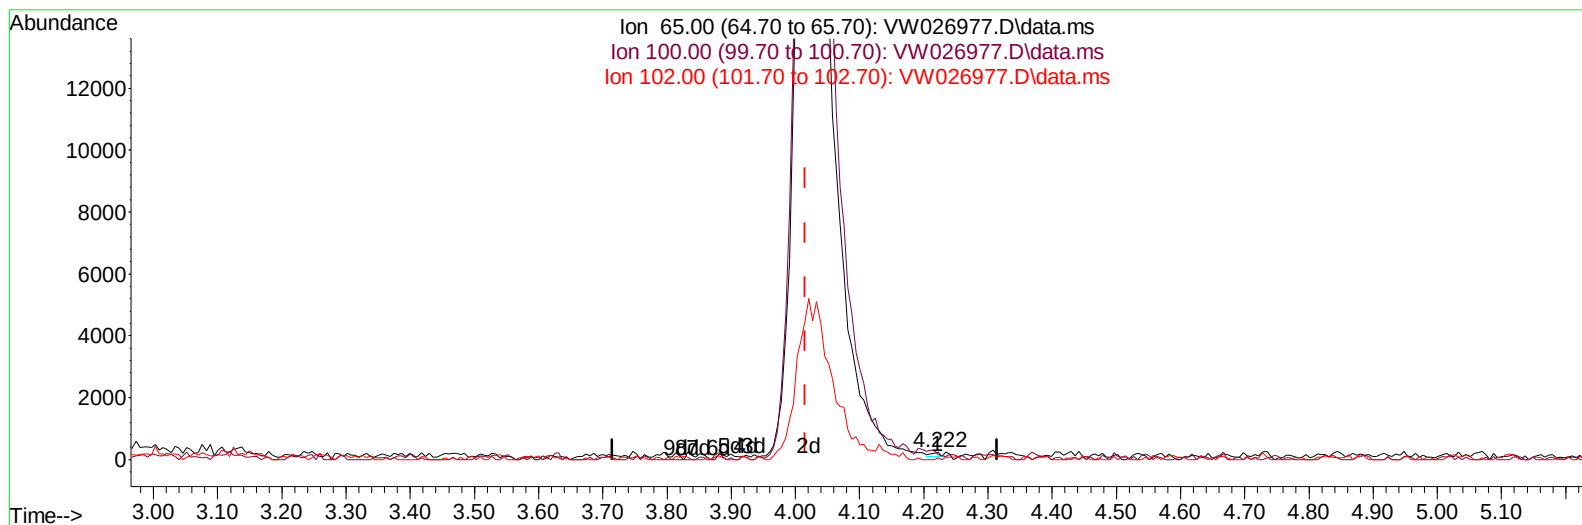

TIC: VW026977.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.222min (+ 0.207) 0.02 ug/L

response 127

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	124.90	110.24
102.00	16.90	14.96
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083123\
Data File : VW026977.D
Acq On : 31 Aug 2023 15:02
Operator : SY/MD
Sample : VIBLK502
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK502

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/01/2023
Supervised By :Mahesh Dadoda 09/05/2023

Quant Time: Sep 01 00:48:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 01 00:44:05 2023
Response via : Initial Calibration

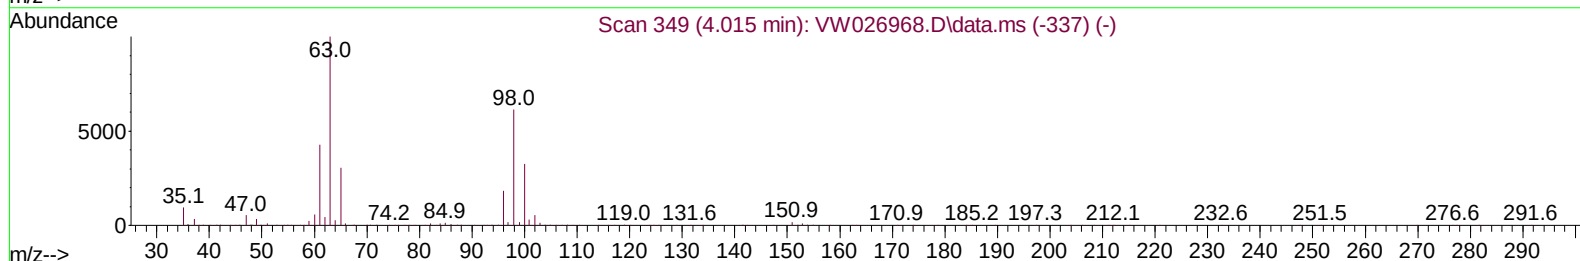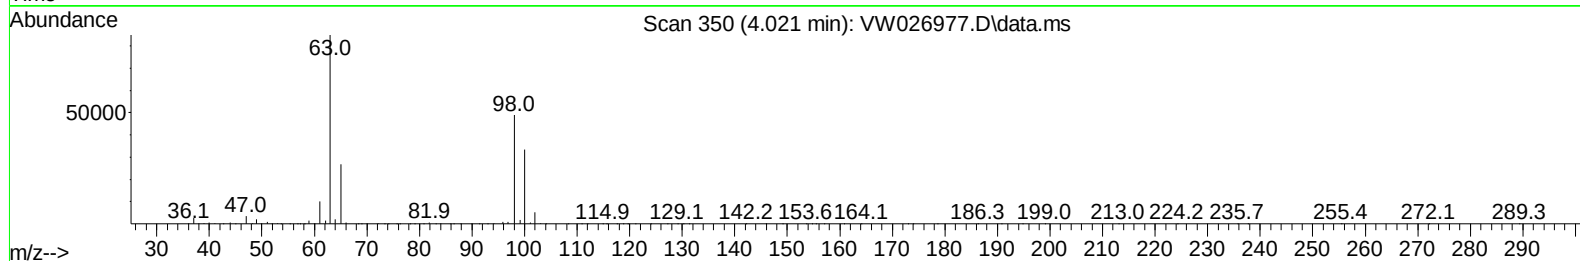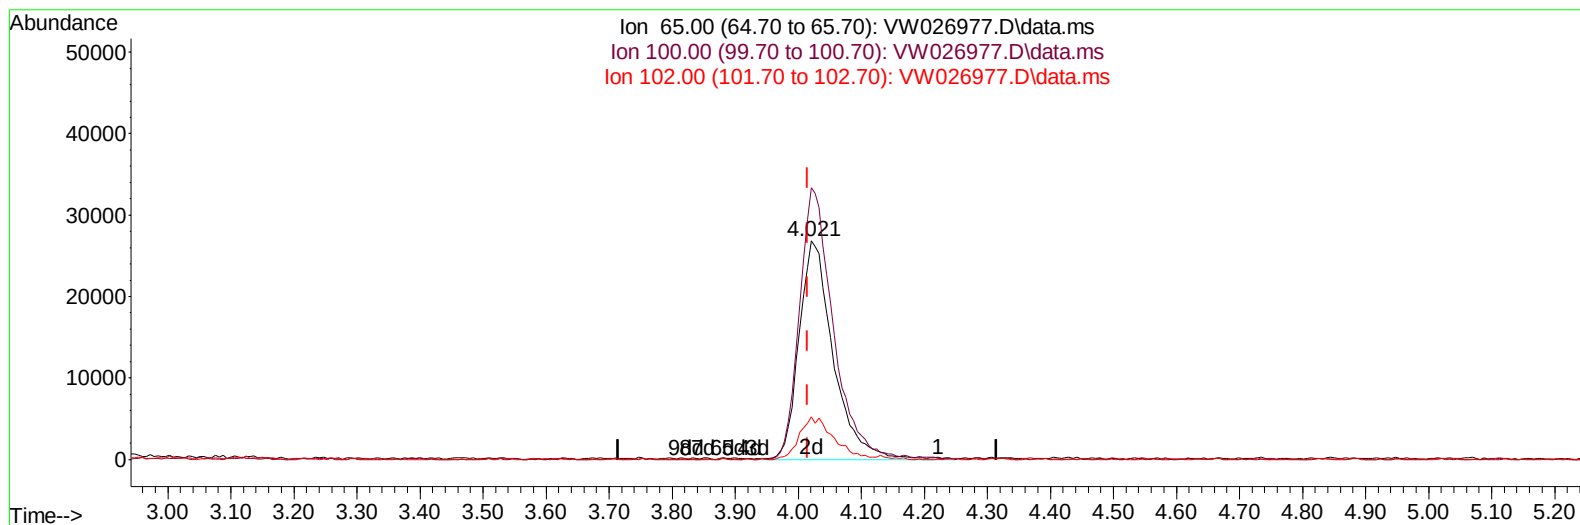

TIC: VW026977.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (+ 0.006) 17.19 ug/L m

response 101434

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	124.90	0.14#
102.00	16.90	0.02#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083123\
 Data File : VW026977.D
 Acq On : 31 Aug 2023 15:02
 Operator : SY/MD
 Sample : VIBLK502
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK502

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/01/2023
 Supervised By :Mahesh Dadoda 09/05/2023

Quant Time: Sep 01 00:48:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 01 00:44:05 2023
 Response via : Initial Calibration

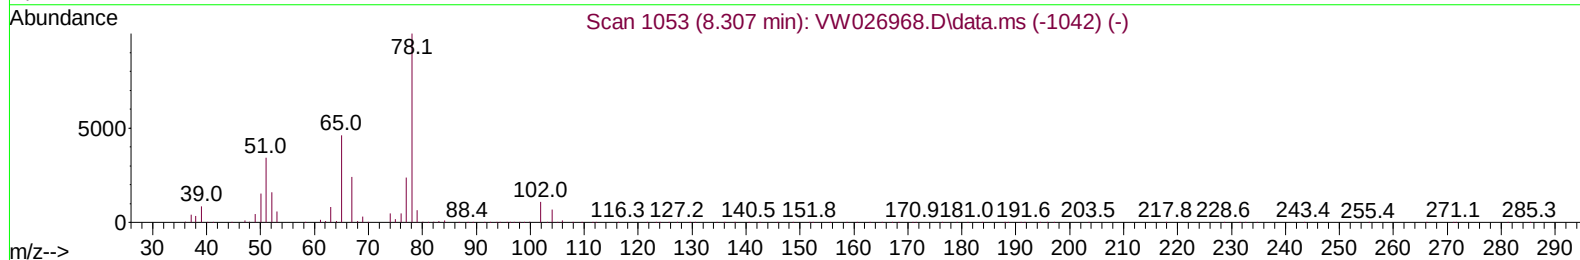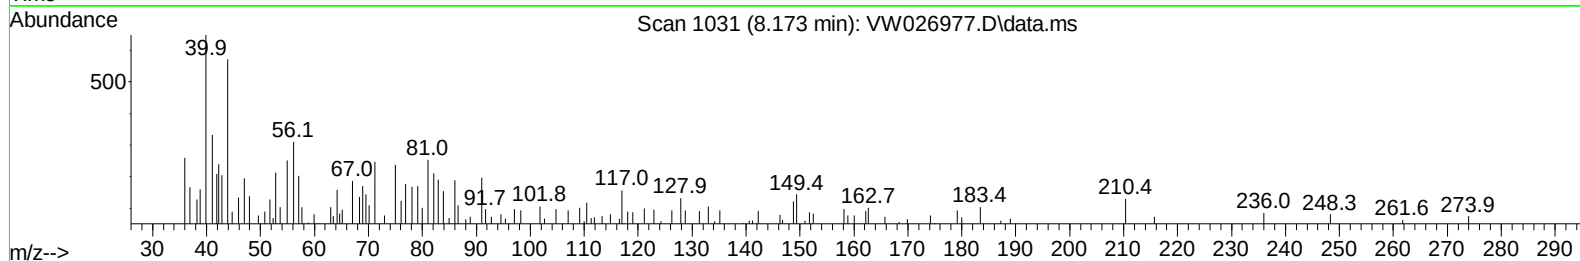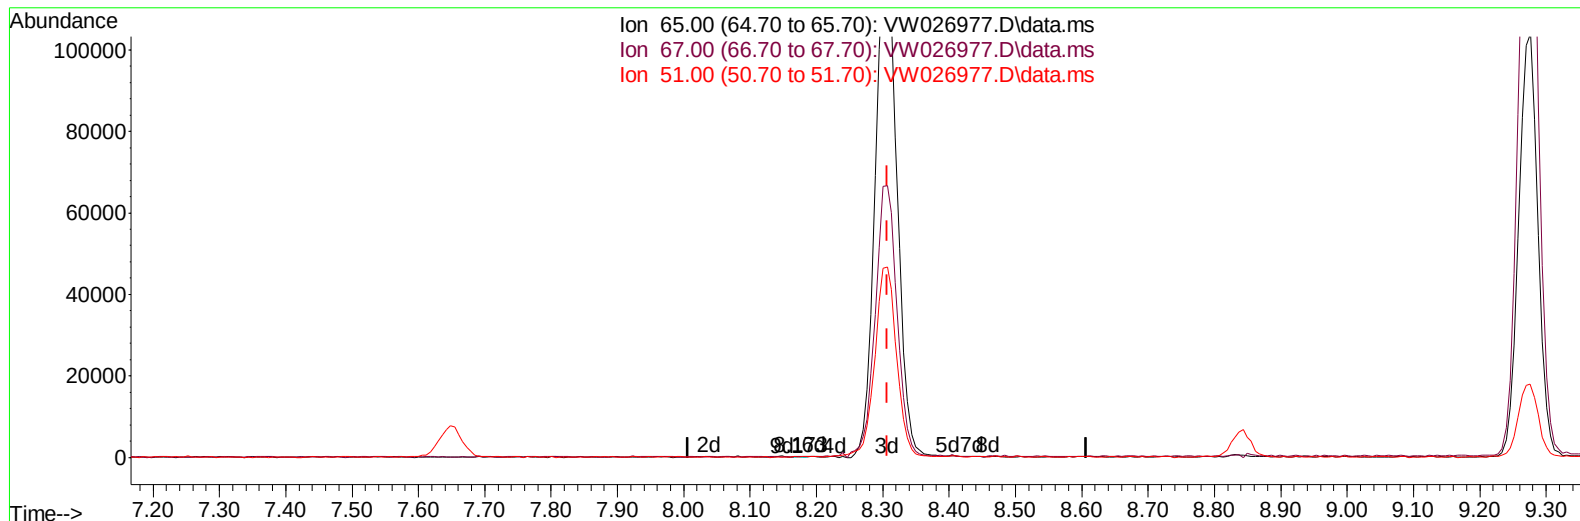

TIC: VW026977.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.173min (-0.134) 0.00 ug/L

response 63

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	65.08
51.00	112.90	106.35
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083123\
 Data File : VW026977.D
 Acq On : 31 Aug 2023 15:02
 Operator : SY/MD
 Sample : VIBLK502
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK502

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/01/2023
 Supervised By :Mahesh Dadoda 09/05/2023

Quant Time: Sep 01 00:48:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 01 00:44:05 2023
 Response via : Initial Calibration

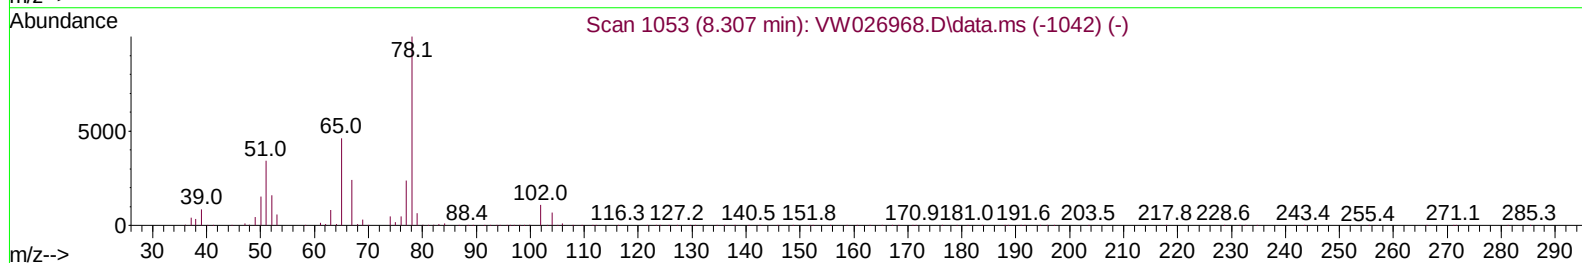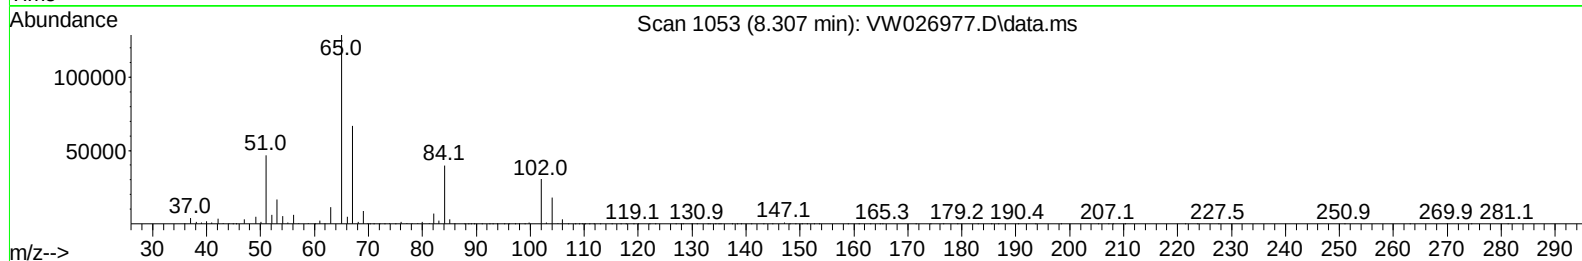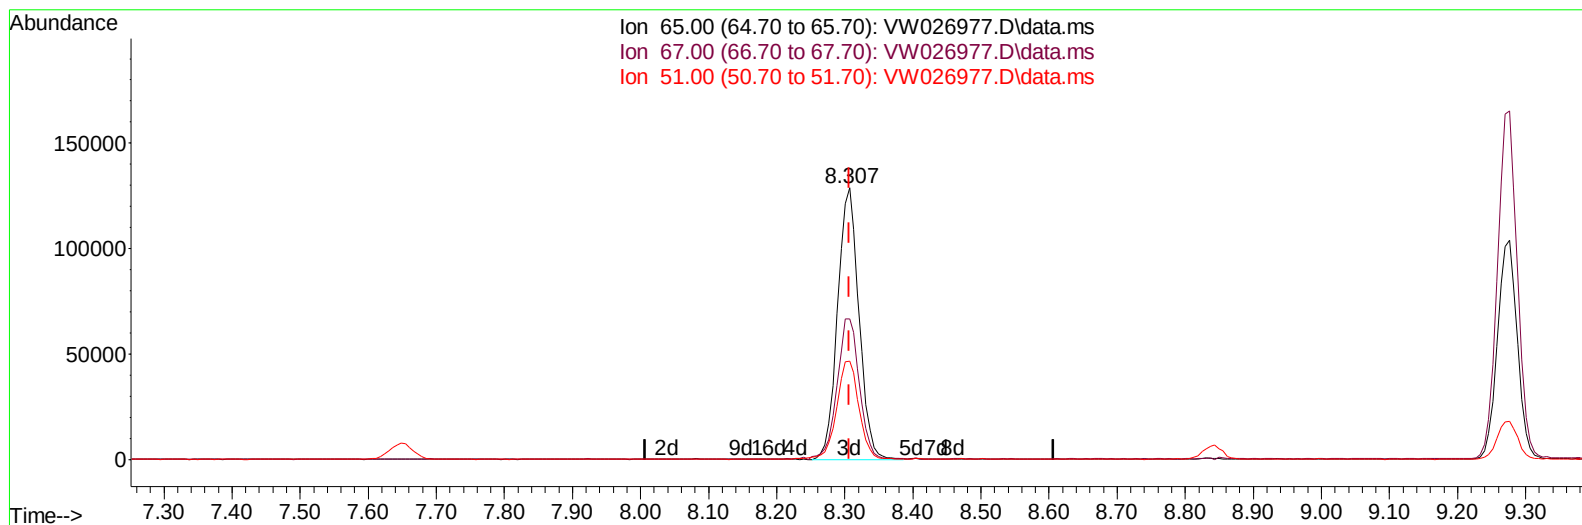

TIC: VW026977.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 20.93 ug/L m

response 282870

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.60	0.01#
51.00	112.90	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083123\
 Data File : VW026977.D
 Acq On : 31 Aug 2023 15:02
 Operator : SY/MD
 Sample : VIBLK502
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK502

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/01/2023
 Supervised By :Mahesh Dadoda 09/05/2023

Quant Time: Sep 01 00:48:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 01 00:44:05 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		729649	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		703502	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		396598	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		250420	20.878	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	83.520%	
7) Chloroethane-d5	2.893	69		225063	25.234	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	100.920%	
11) 1,1-Dichloroethene-d2	4.021	65		101434m	17.194	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	68.760%	
21) 2-Butanone-d5	7.075	46		158286	45.913	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	91.820%	
24) Chloroform-d	7.648	84		516275	21.082	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	84.320%	
26) 1,2-Dichloroethane-d4	8.307	65		282870m	20.931	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	83.720%	
32) Benzene-d6	8.276	84		1065301	21.972	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	87.880%	
36) 1,2-Dichloropropane-d6	9.276	67		333046	22.052	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	88.200%	
41) Toluene-d8	10.325	98		948451	22.789	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	91.160%	
43) trans-1,3-Dichloroprop...	10.575	79		130679	20.957	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	83.840%	
47) 2-Hexanone-d5	10.922	63		93642	59.008	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	118.020%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		306586	25.705	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	102.840%	
66) 1,2-Dichlorobenzene-d4	13.848	152		355374	25.035	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	100.120%	
Target Compounds							
13) Acetone	4.119	43		11496	3.354	ug/L	84
16) Methylene chloride	4.923	84		141717	10.041	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW083123\
Data File : VW026977.D
Acq On : 31 Aug 2023 15:02
Operator : SY/MD
Sample : VIBLK502
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK502

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/01/2023
Supervised By :Mahesh Dadoda 09/05/2023

Quant Time: Sep 01 00:48:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 01 00:44:05 2023
Response via : Initial Calibration

