


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW090118\
 Data File : VW005053.D
 Acq On : 31 Aug 2018 22:57
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W090118S.M
 Title : SW846 8260
 Last Update : Sat Sep 01 03:35:05 2018

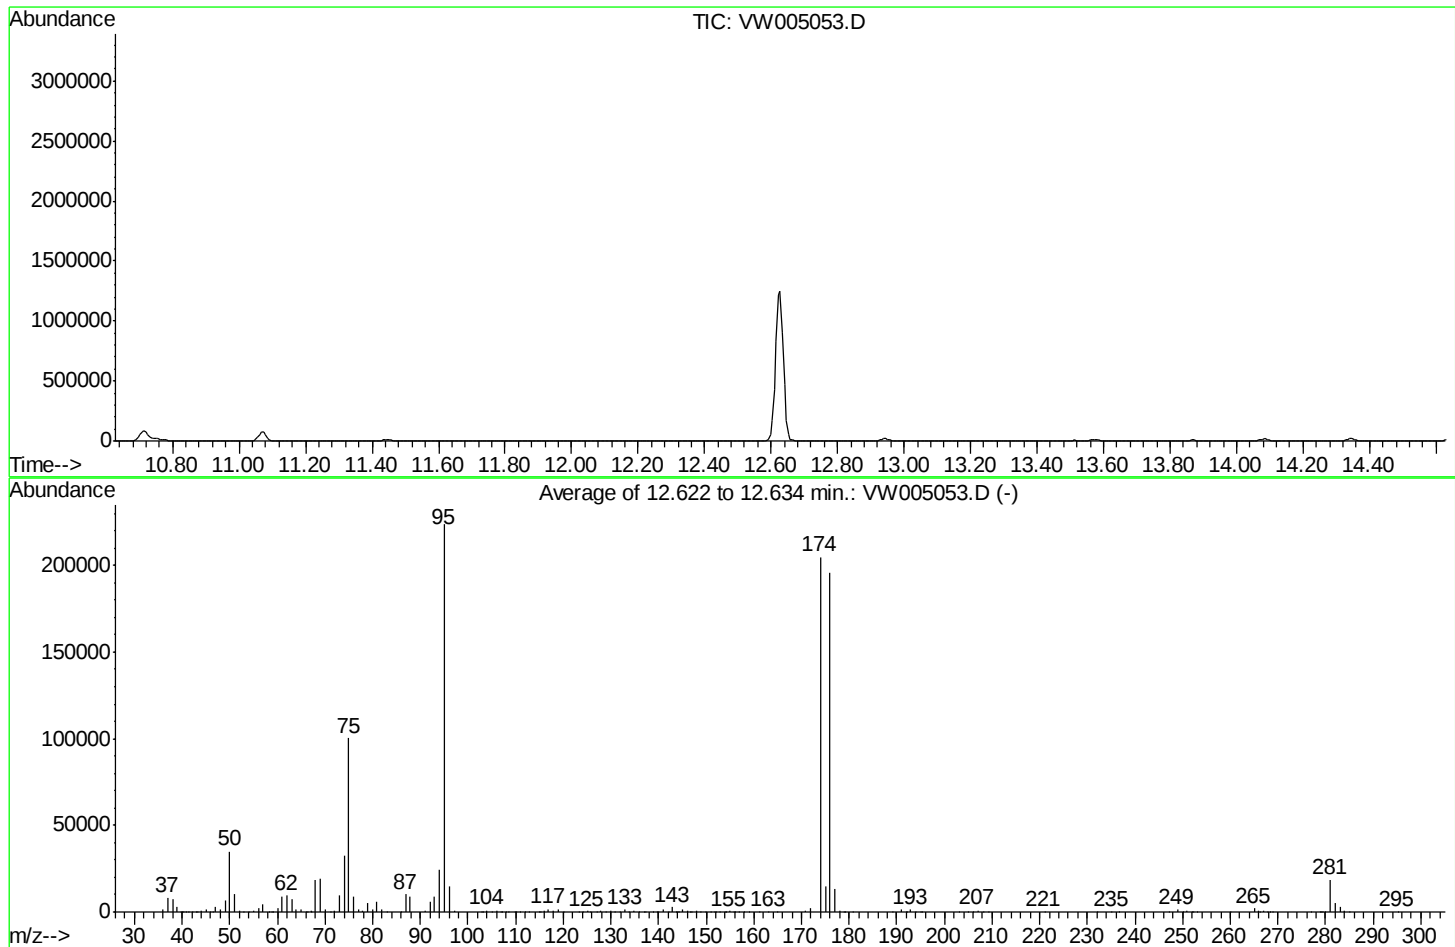

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	34816	PASS
75	95	30	60	44.8	100240	PASS
95	95	100	100	100.0	223701	PASS
96	95	5	9	6.6	14745	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.6	204842	PASS
175	174	5	9	7.3	14881	PASS
176	174	95	101	95.7	195968	PASS
177	176	5	9	6.7	13106	PASS