


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW090119\
Data File : VW012463.D
Acq On : 01 Sep 2019 22:05
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W082319S.M
Title : SW846 8260
Last Update : Mon Aug 26 07:18:31 2019

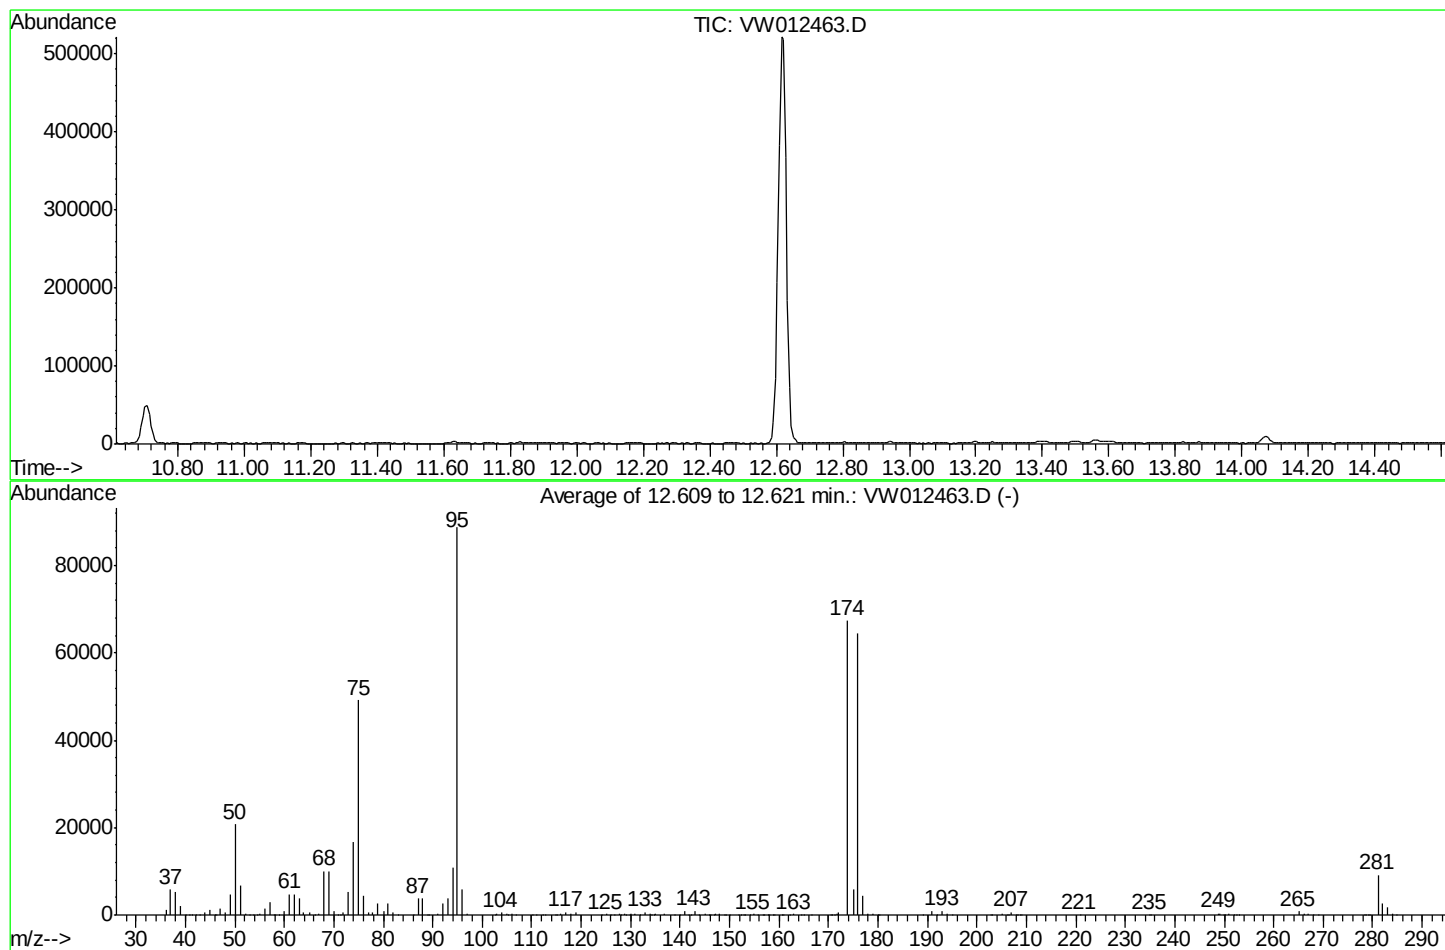

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	20797	PASS
75	95	30	60	55.5	49229	PASS
95	95	100	100	100.0	88760	PASS
96	95	5	9	6.6	5875	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.8	67322	PASS
175	174	5	9	8.6	5763	PASS
176	174	95	101	95.7	64426	PASS
177	176	5	9	6.9	4462	PASS