




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026983.D
 Acq On : 01 Sep 2023 09:46
 Operator : SY/MD
 Sample : VSTDCCC025
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 LabSampleId :
 VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:29:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 01 00:44:05 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

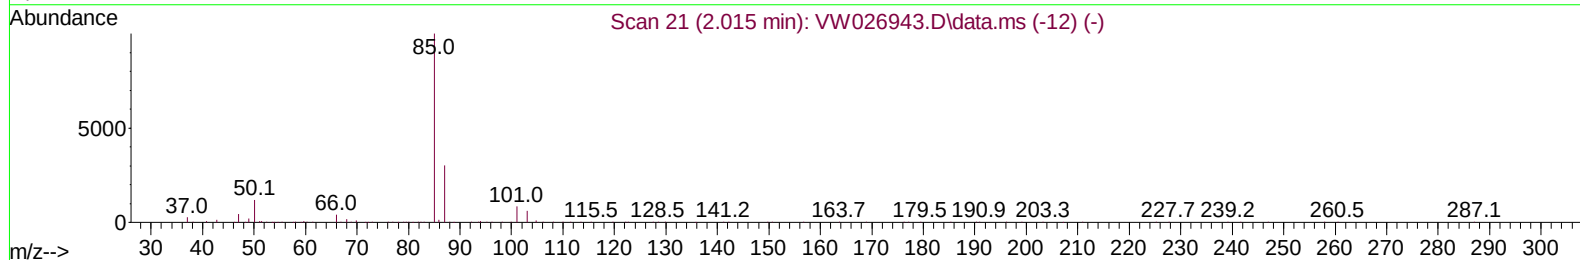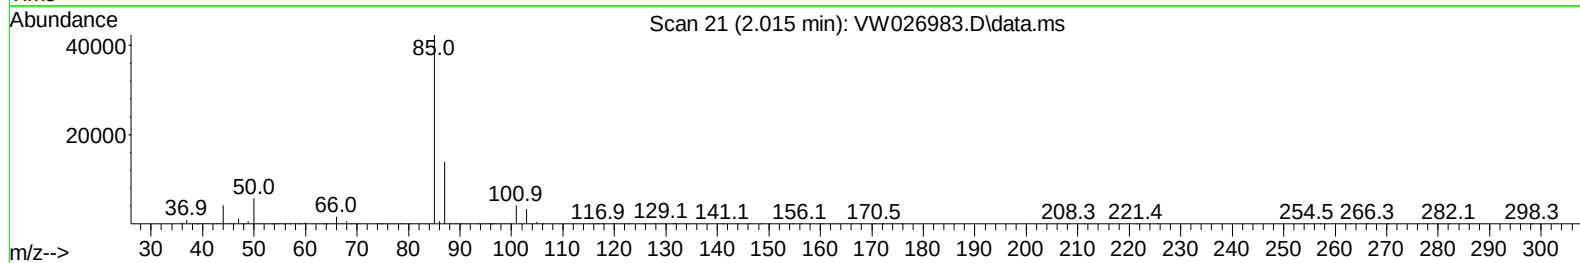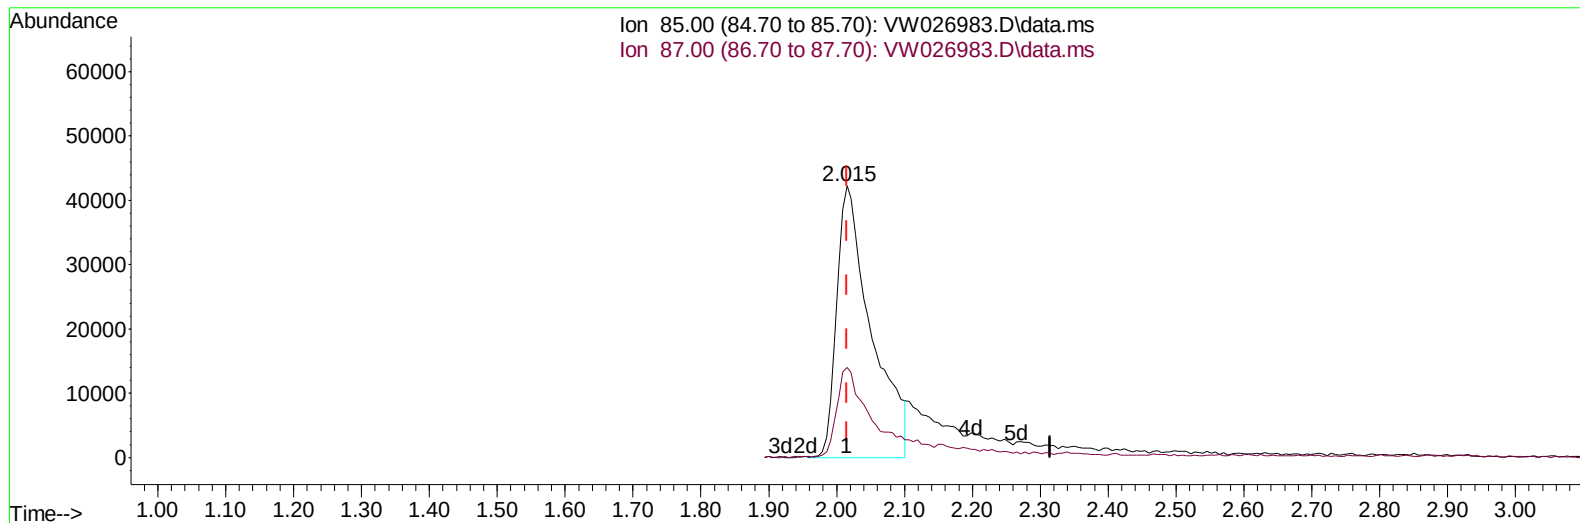

TIC: VW026983.D\data.ms

(2) Dichlorodifluoromethane (T)

2.015min (+ 0.000) 15.68 ug/L

response 149123

Ion	Exp%	Act%
85.00	100.00	100.00
87.00	24.40	27.21
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026983.D
 Acq On : 01 Sep 2023 09:46
 Operator : SY/MD
 Sample : VSTDCCC025
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 LabSampleId :
 VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:29:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 01 00:44:05 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

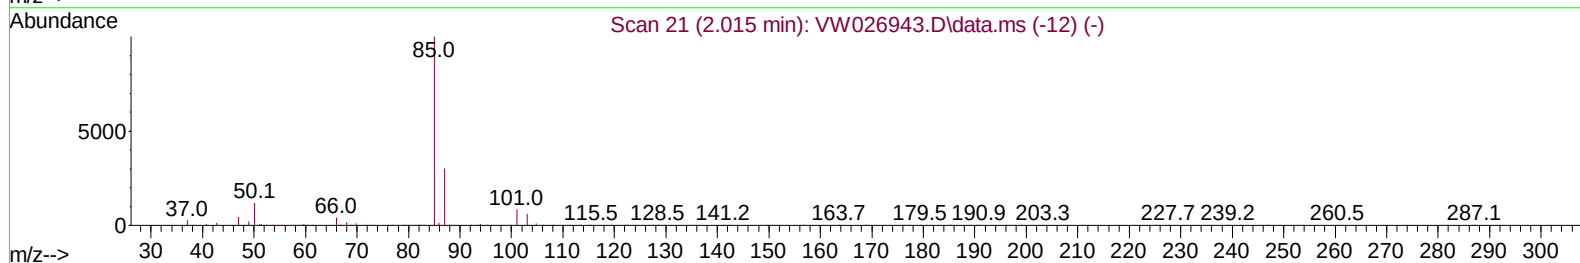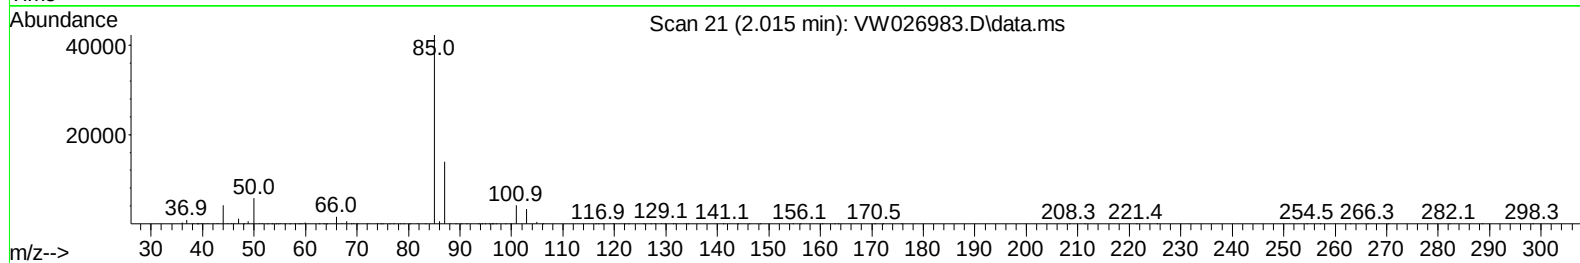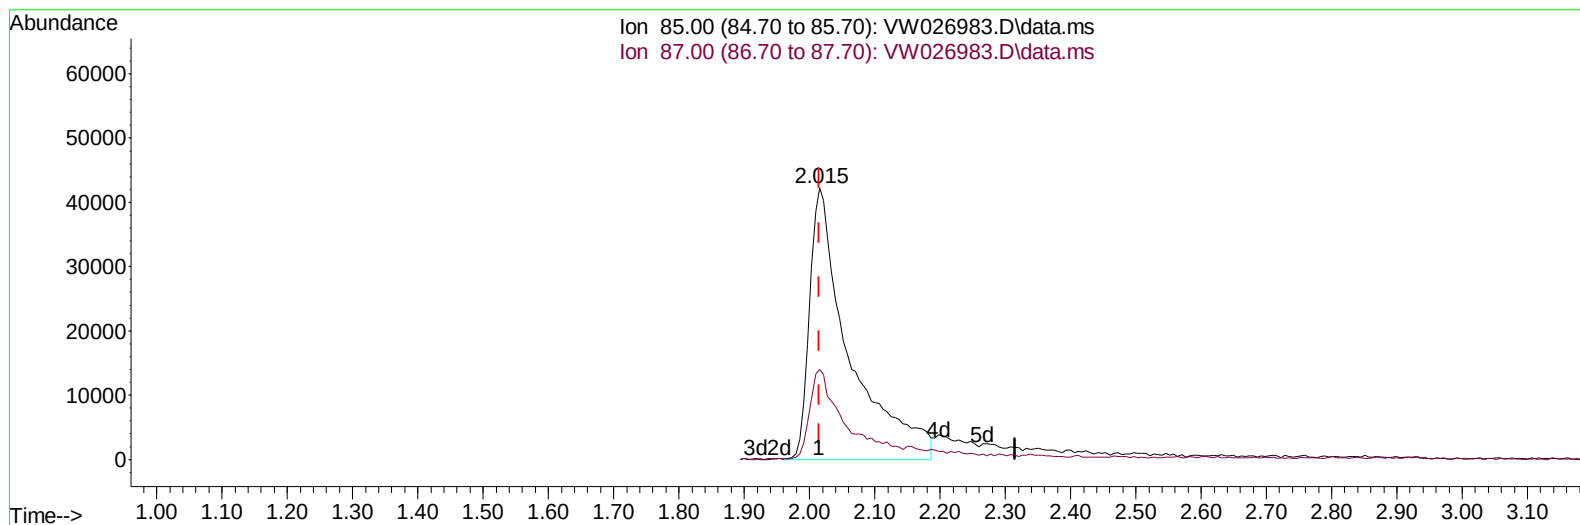

TIC: VW026983.D\data.ms

(2) Dichlorodifluoromethane (T)

2.015min (+ 0.000) 18.80 ug/L m

response 178827

Ion	Exp%	Act%
85.00	100.00	100.00
87.00	24.40	22.69
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026983.D
 Acq On : 01 Sep 2023 09:46
 Operator : SY/MD
 Sample : VSTDCCC025
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 LabSampleId :
 VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:29:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 01 00:44:05 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

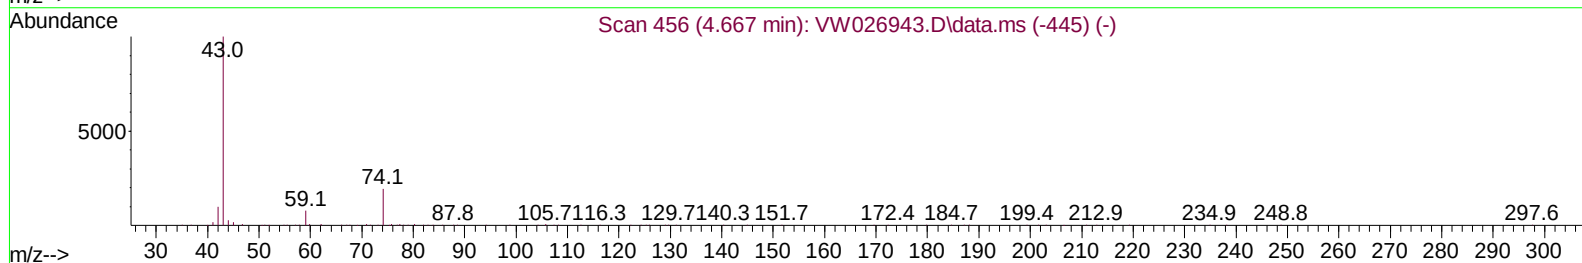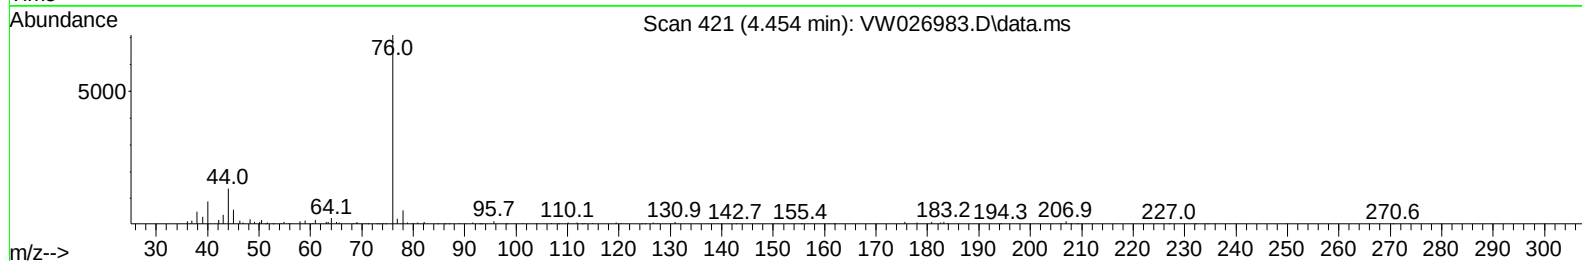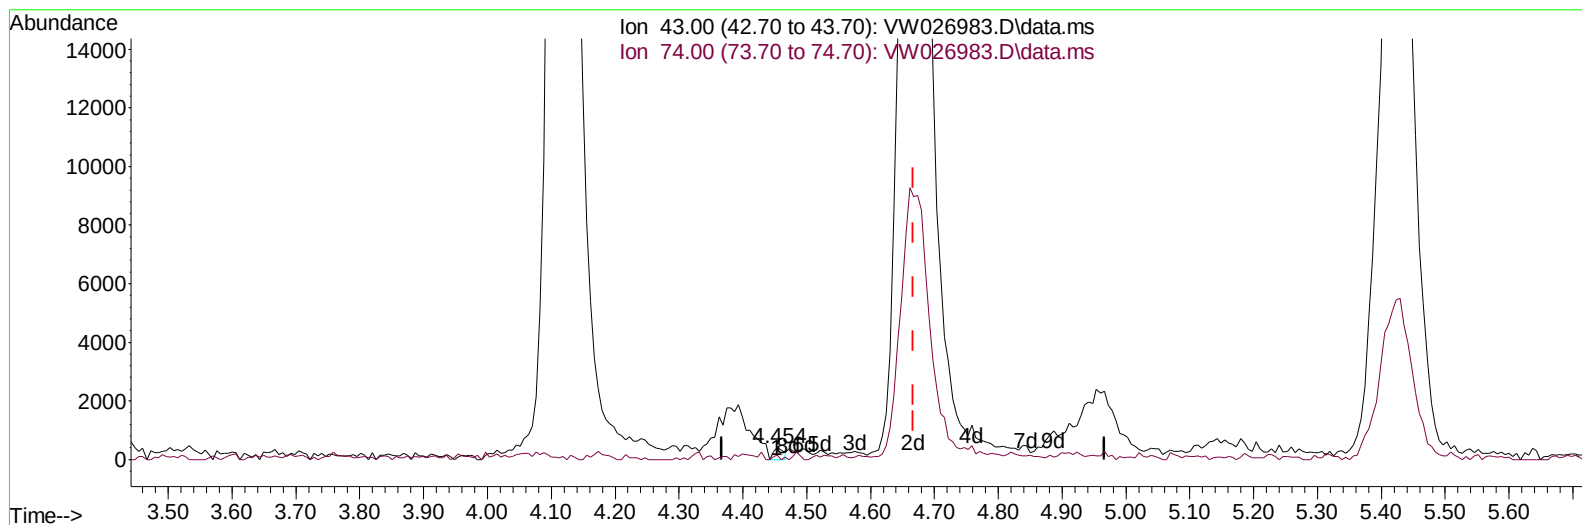

TIC: VW026983.D\data.ms

(15) Methyl Acetate (T)

4.454min (-0.213) 0.07 ug/L

response 439

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	20.50	20.73
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026983.D
 Acq On : 01 Sep 2023 09:46
 Operator : SY/MD
 Sample : VSTDCCC025
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 LabSampleId :
 VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:29:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 01 00:44:05 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

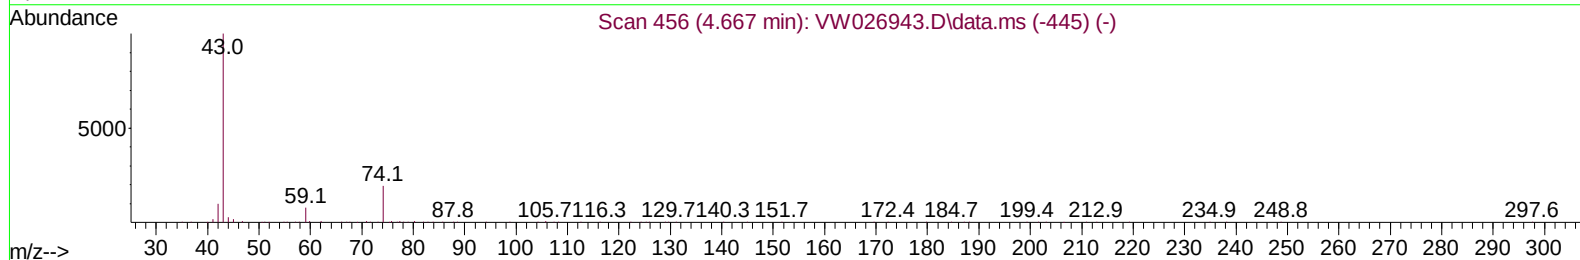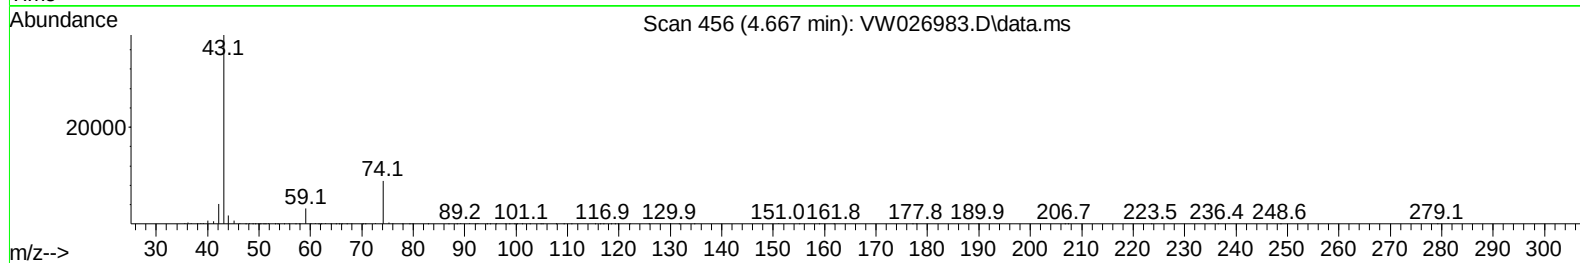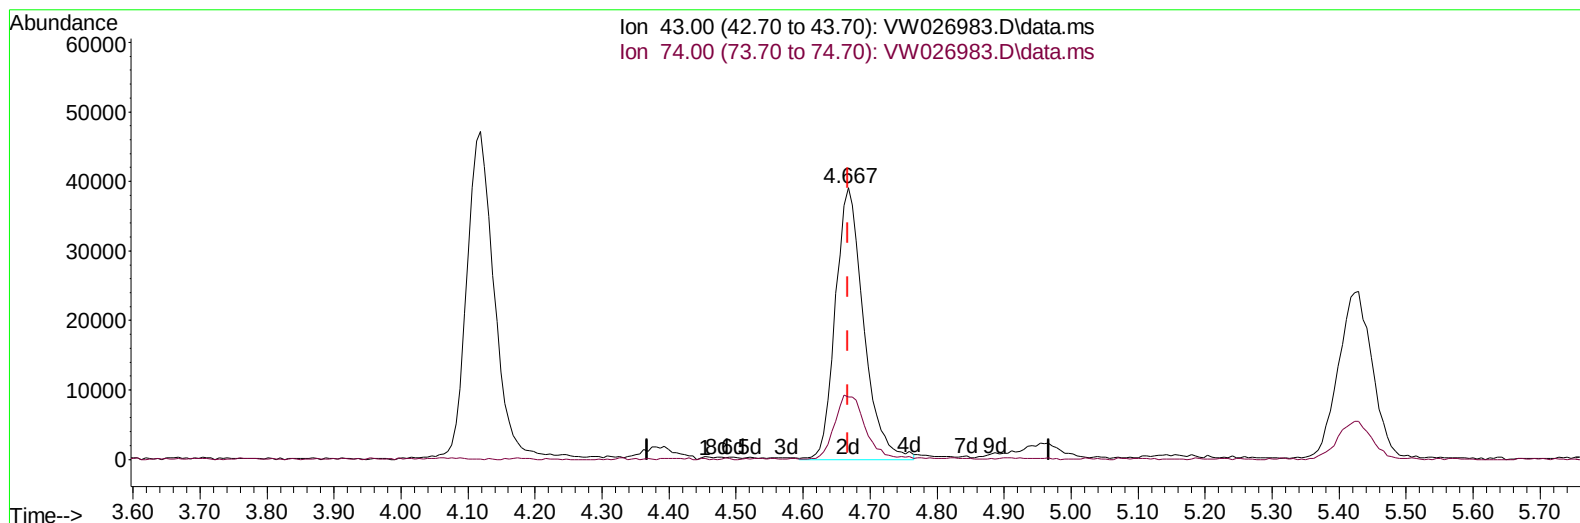

TIC: VW026983.D\data.ms

(15) Methyl Acetate (T)

4.667min (+ 0.000) 17.43 ug/L m

response 114737

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	20.50	0.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026983.D
 Acq On : 01 Sep 2023 09:46
 Operator : SY/MD
 Sample : VSTDCCC025
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 LabSampleId :
 VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:29:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 01 00:44:05 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	699601	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	660110	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	373916	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	266147	23.142	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	92.560%	
7) Chloroethane-d5	2.893	69	244085	28.542	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	114.160%	
11) 1,1-Dichloroethene-d2	4.021	65	107962	19.087	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	76.360%	
21) 2-Butanone-d5	7.075	46	146036	44.180	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	88.360%	
24) Chloroform-d	7.648	84	575236	24.498	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	98.000%	
26) 1,2-Dichloroethane-d4	8.307	65	287578	22.193	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	88.760%	
32) Benzene-d6	8.270	84	1148370	25.242	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	100.960%	
36) 1,2-Dichloropropane-d6	9.270	67	347385	24.514	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	98.040%	
41) Toluene-d8	10.319	98	1034332	26.486	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	105.960%	
43) trans-1,3-Dichloroprop...	10.575	79	135248	23.115	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	92.480%	
47) 2-Hexanone-d5	10.922	63	78899	52.986	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	105.980%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	304068	27.170	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	108.680%	
66) 1,2-Dichlorobenzene-d4	13.849	152	371814	27.782	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	111.120%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.015	85	178827m	18.800	ug/L	
3) Chloromethane	2.216	50	235001	18.068	ug/L	99
5) Vinyl chloride	2.369	62	299869	24.117	ug/L	98
6) Bromomethane	2.783	94	193894	26.765	ug/L	97
8) Chloroethane	2.930	64	200288	26.884	ug/L	99
9) Trichlorofluoromethane	3.259	101	183519	17.985	ug/L	100
10) 1,1,2-Trichloro-1,2,2-...	4.070	101	262150	23.784	ug/L	93
12) 1,1-Dichloroethene	4.045	96	237559	22.973	ug/L	81
13) Acetone	4.119	43	132513	40.318	ug/L	92
14) Carbon disulfide	4.393	76	606412	16.301	ug/L	99
15) Methyl Acetate	4.667	43	114737m	17.428	ug/L	
16) Methylene chloride	4.917	84	284296	21.007	ug/L	88
17) trans-1,2-Dichloroethene	5.423	96	261310	22.646	ug/L	87
18) Methyl tert-butyl Ether	5.429	73	424869	24.334	ug/L	96
19) 1,1-Dichloroethane	6.216	63	521774	21.970	ug/L	99
20) cis-1,2-Dichloroethene	7.167	96	314096	25.324	ug/L	86
22) 2-Butanone	7.167	43	169673	35.031	ug/L	88
23) Bromochloromethane	7.514	128	133983	25.008	ug/L #	79

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026983.D
 Acq On : 01 Sep 2023 09:46
 Operator : SY/MD
 Sample : VSTDCCC025
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 LabSampleId :
 VSTDCCC025

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:29:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 01 00:44:05 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
25) Chloroform	7.679	83	520247	22.675	ug/L	98
27) 1,2-Dichloroethane	8.398	62	325976	20.366	ug/L	95
29) Cyclohexane	7.953	56	408782	20.025	ug/L	90
30) 1,1,1-Trichloroethane	7.874	97	406196	23.578	ug/L	98
31) Carbon tetrachloride	8.069	117	351817	22.335	ug/L	94
33) Benzene	8.325	78	1148341	23.888	ug/L	100
34) Trichloroethene	9.093	95	298990	24.421	ug/L	94
35) Methylcyclohexane	9.337	83	483859	23.102	ug/L	91
37) 1,2-Dichloropropane	9.368	63	296389	22.510	ug/L #	97
38) Bromodichloromethane	9.642	83	368693	23.869	ug/L	99
39) cis-1,3-Dichloropropene	10.069	75	459268	24.246	ug/L	98
40) 4-Methyl-2-pentanone	10.209	43	328806	38.390	ug/L #	92
42) Toluene	10.386	91	1261406	25.940	ug/L	100
44) trans-1,3-Dichloropropene	10.605	75	386436	23.702	ug/L	96
45) 1,1,2-Trichloroethane	10.788	97	227108	25.220	ug/L	95
46) Tetrachloroethene	10.861	164	234566	26.372	ug/L	95
48) 2-Hexanone	10.965	43	230982	39.634	ug/L #	92
49) Dibromochloromethane	11.123	129	244779	25.989	ug/L	96
50) 1,2-Dibromoethane	11.233	107	209398	24.782	ug/L	92
51) Chlorobenzene	11.654	112	806539	26.257	ug/L	98
52) Ethylbenzene	11.727	91	1399648	25.667	ug/L	97
53) m,p-Xylene	11.837	106	533222	26.394	ug/L	96
54) o-Xylene	12.160	106	522420	27.708	ug/L	98
55) Styrene	12.178	104	904518	27.591	ug/L	98
57) 1,1,2,2-Tetrachloroethane	12.709	83	267870	23.488	ug/L	100
59) Bromoform	12.349	173	139742	23.857	ug/L	97
60) Isopropylbenzene	12.459	105	1432218	25.763	ug/L	98
61) 1,2,3-Trichloropropane	12.763	75	186373	20.548	ug/L	97
62) 1,3,5-Trimethylbenzene	12.940	105	1196678	27.234	ug/L	97
63) 1,2,4-Trimethylbenzene	13.245	105	1167280	27.109	ug/L	100
64) 1,3-Dichlorobenzene	13.495	146	618467	25.581	ug/L	91
65) 1,4-Dichlorobenzene	13.574	146	649426	25.739	ug/L	99
67) 1,2-Dichlorobenzene	13.867	146	570867	25.966	ug/L	97
68) 1,2-Dibromo-3-chloropr...	14.477	75	40950	18.728	ug/L	93
69) 1,3,5-Trichlorobenzene	14.623	180	453835	27.785	ug/L	98
70) 1,2,4-trichlorobenzene	15.129	180	379297	27.388	ug/L	97
71) Naphthalene	15.360	128	661871	25.055	ug/L	99
72) 1,2,3-Trichlorobenzene	15.549	180	334072	26.745	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

