




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
Data File : VW026984.D
Acq On : 01 Sep 2023 11:12
Operator : SY/MD
Sample : VW0901SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK565

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:33:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 02 00:33:01 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/04/2023
Supervised By :Mahesh Dadoda 09/04/2023

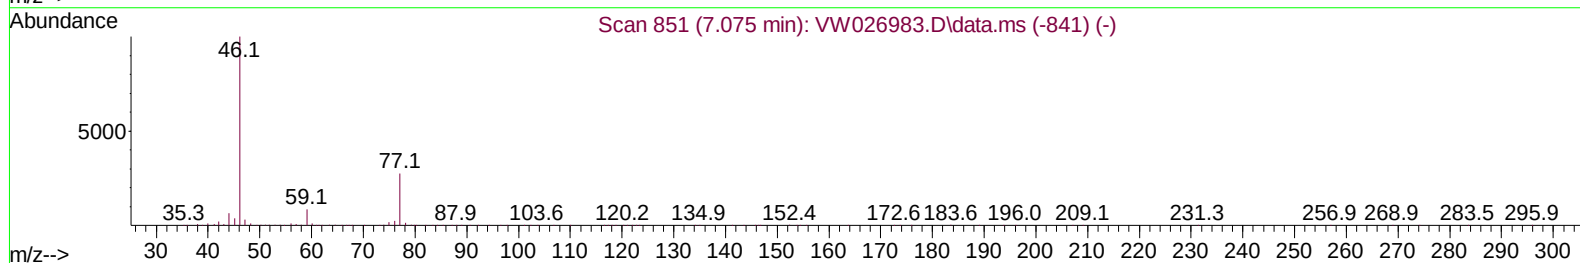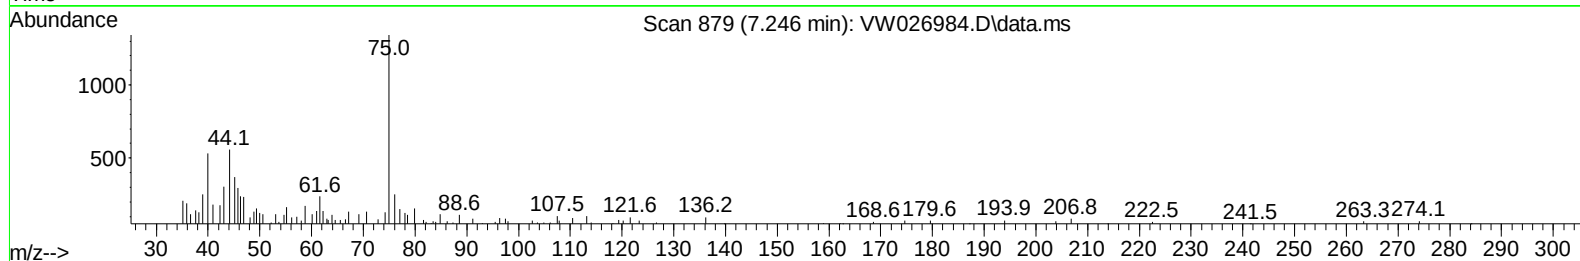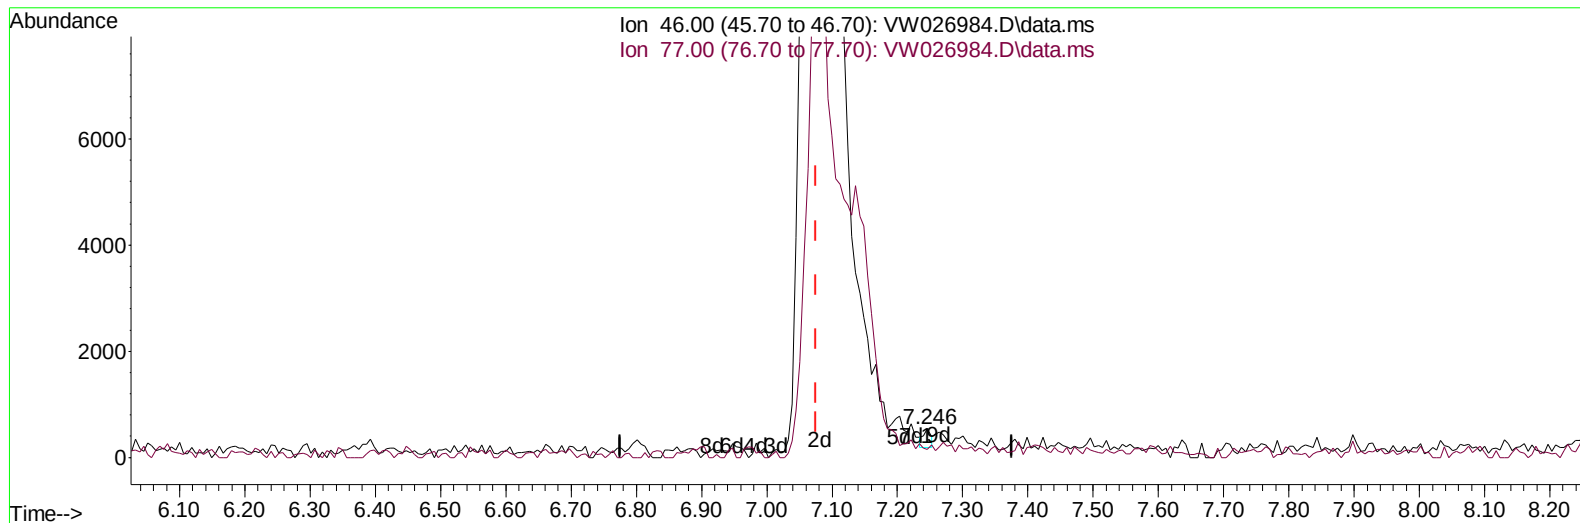

TIC: VW026984.D\data.ms

(21) 2-Butanone-d5 (S)

7.246min (+ 0.171) 0.09 ug/L

response	281
Ion	Exp% Act%
46.00	100.00 100.00
77.00	20.60 14.95
0.00	0.00 0.00
0.00	0.00 0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026984.D
 Acq On : 01 Sep 2023 11:12
 Operator : SY/MD
 Sample : VW0901SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK565

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:33:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 02 00:33:01 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

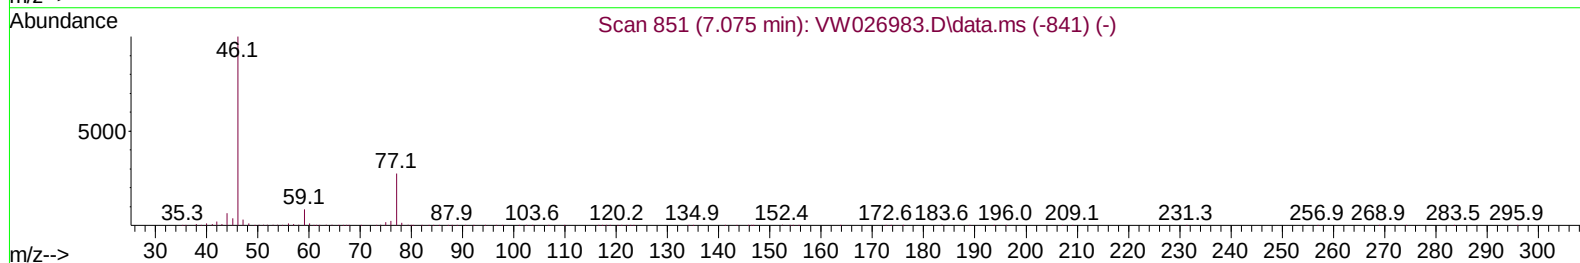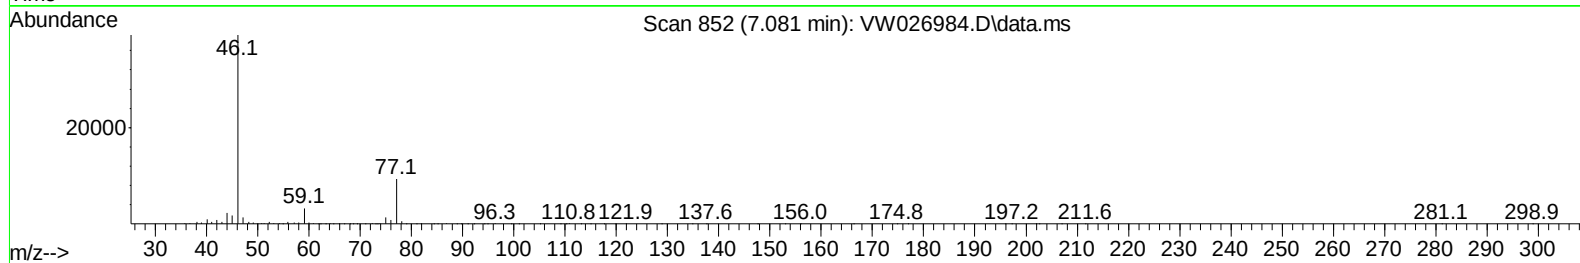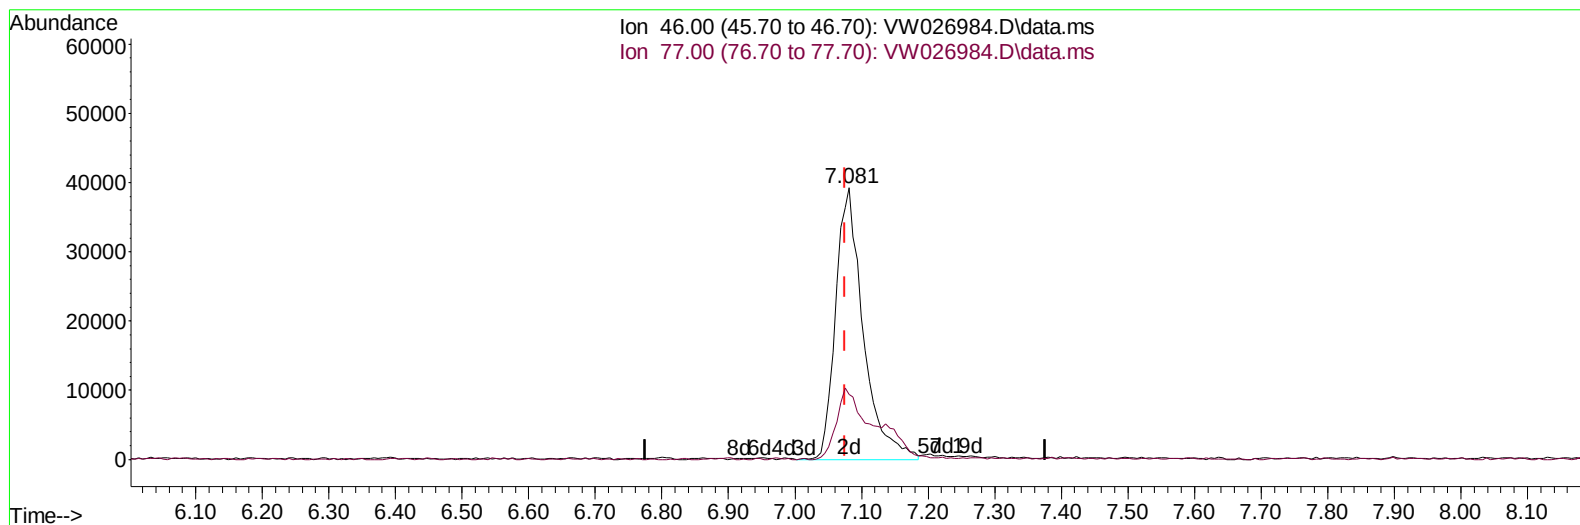

TIC: VW026984.D\data.ms

(21) 2-Butanone-d5 (S)

7.081min (+ 0.006) 35.45 ug/L m

response 112987

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.60	0.04#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026984.D
 Acq On : 01 Sep 2023 11:12
 Operator : SY/MD
 Sample : VW0901SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK565

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

Quant Time: Sep 02 00:33:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 02 00:33:01 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		674621	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		646114	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152		330900	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		211254	19.049	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	76.200%	
7) Chloroethane-d5	2.899	69		198805	24.108	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	96.440%	
11) 1,1-Dichloroethene-d2	4.027	65		85570	15.688	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	62.760%	
21) 2-Butanone-d5	7.081	46		112987m	35.447	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	70.900%	
24) Chloroform-d	7.654	84		456113	20.144	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	80.560%	
26) 1,2-Dichloroethane-d4	8.307	65		236375	18.917	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	75.680%	
32) Benzene-d6	8.276	84		922782	20.723	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	82.880%	
36) 1,2-Dichloropropane-d6	9.276	67		278152	20.053	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	80.200%	
41) Toluene-d8	10.325	98		805375	21.070	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	84.280%	
43) trans-1,3-Dichloroprop...	10.581	79		101840	17.783	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	71.120%	
47) 2-Hexanone-d5	10.922	63		57606	39.524	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	79.040%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		243140	22.197	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	88.800%	
66) 1,2-Dichlorobenzene-d4	13.848	152		291536	24.615	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	98.480%	
Target Compounds							
13) Acetone	4.125	43		11214	3.538	ug/L	73
16) Methylene chloride	4.923	84		22709	1.740	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
Data File : VW026984.D
Acq On : 01 Sep 2023 11:12
Operator : SY/MD
Sample : VW0901SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK565

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/04/2023
Supervised By :Mahesh Dadoda 09/04/2023

Quant Time: Sep 02 00:33:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 02 00:33:01 2023
Response via : Initial Calibration

