




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026985.D
 Acq On : 01 Sep 2023 11:36
 Operator : SY/MD
 Sample : 04175-13
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Quant Time: Sep 02 00:33:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 02 00:33:01 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

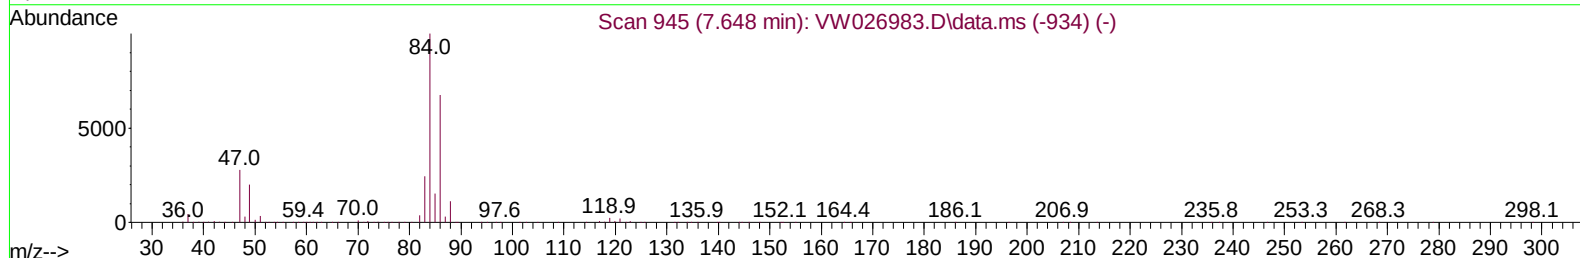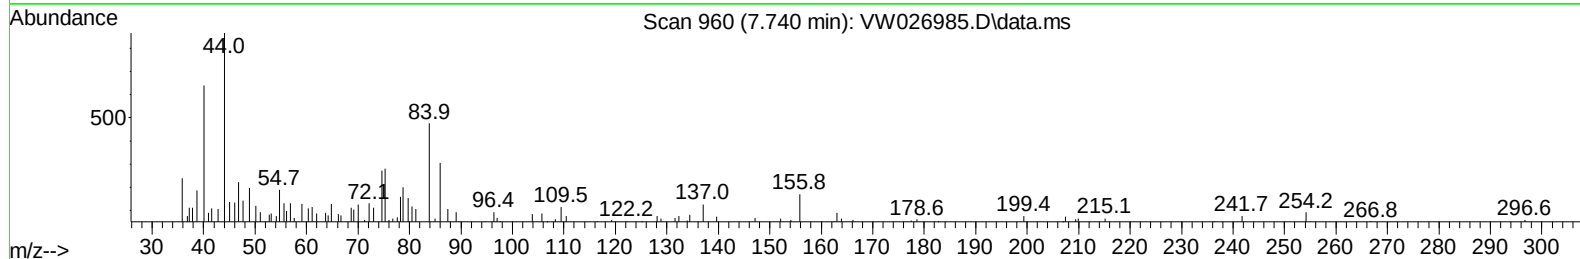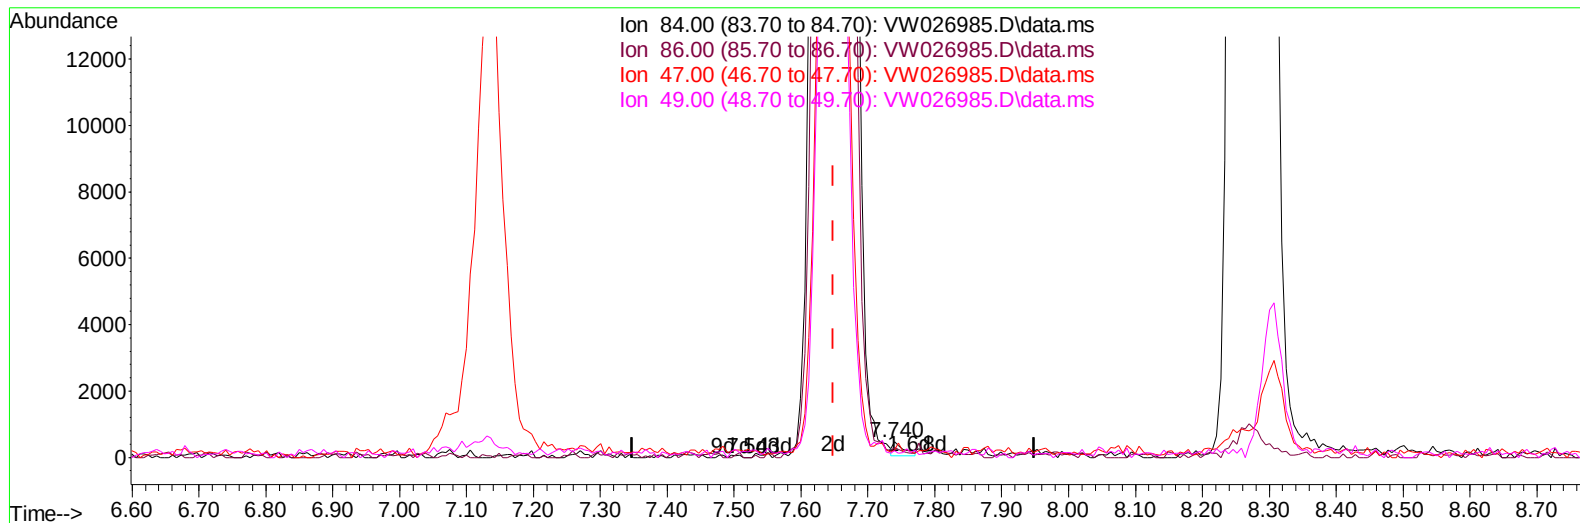

TIC: VW026985.D\data.ms

(24) Chloroform-d (S)

7.740min (+ 0.091) 0.02 ug/L

response 511

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	72.80
47.00	49.30	34.83
49.00	28.20	22.70




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026985.D
 Acq On : 01 Sep 2023 11:36
 Operator : SY/MD
 Sample : 04175-13
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

Quant Time: Sep 02 00:33:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 02 00:33:01 2023
 Response via : Initial Calibration

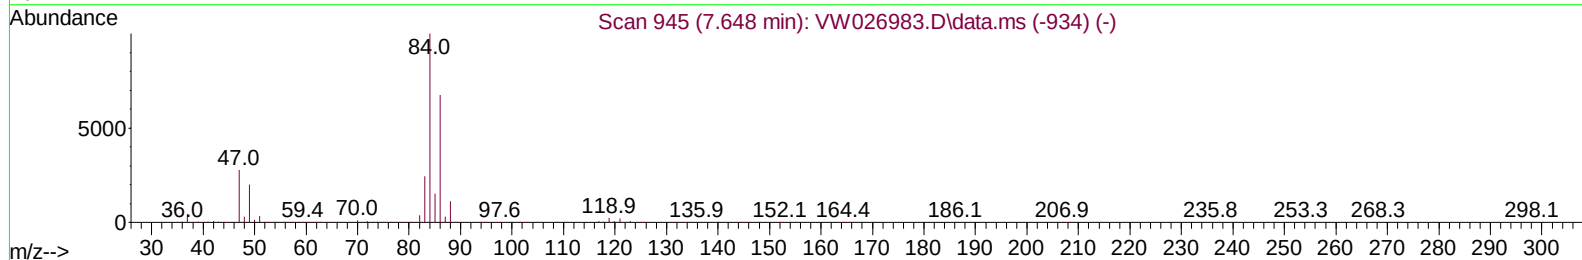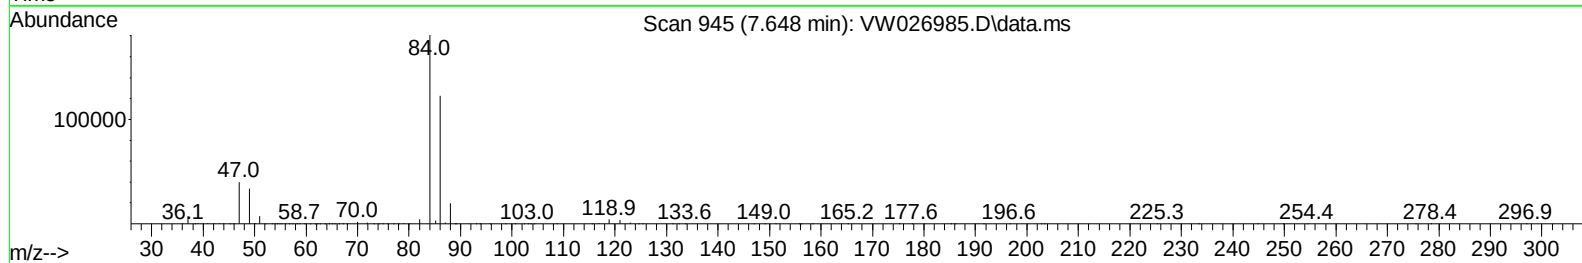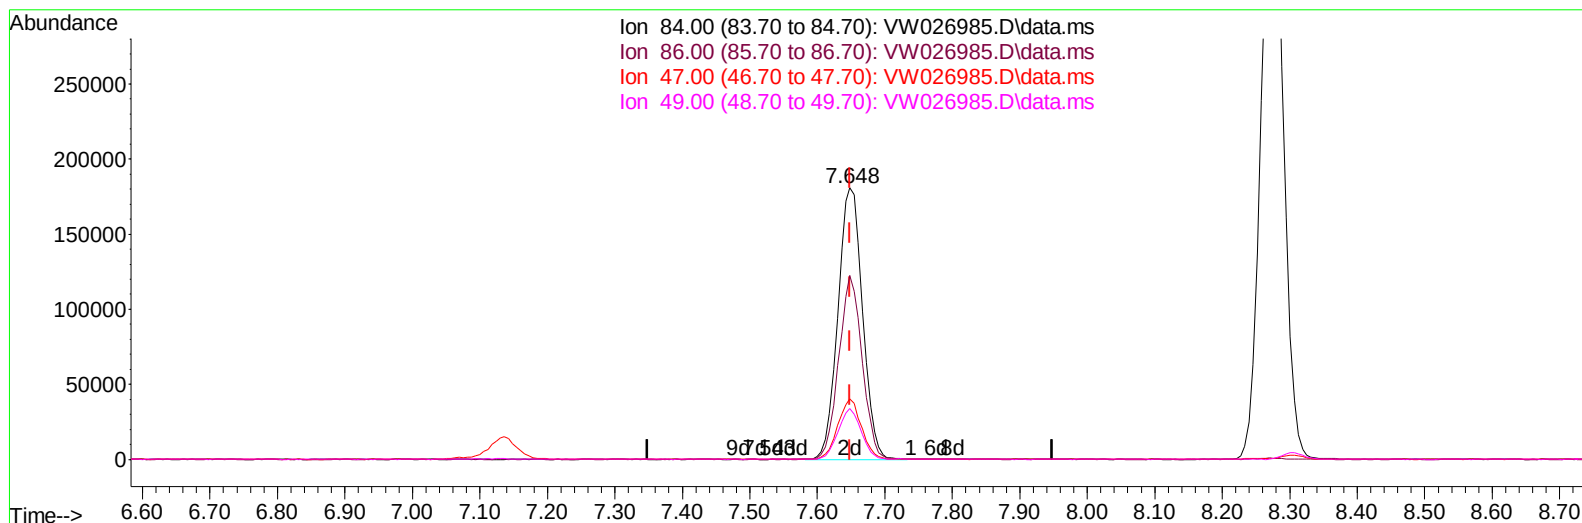

TIC: VW026985.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 19.93 ug/L m

response 457500

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.80	0.08#
47.00	49.30	0.04#
49.00	28.20	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026985.D
 Acq On : 01 Sep 2023 11:36
 Operator : SY/MD
 Sample : 04175-13
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/04/2023
 Supervised By :Mahesh Dadoda 09/04/2023

Quant Time: Sep 02 00:33:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 02 00:33:01 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		683795	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		651324	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		347299	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		219625	19.538	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	78.160%	
7) Chloroethane-d5	2.893	69		198511	23.749	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	95.000%	
11) 1,1-Dichloroethene-d2	4.021	65		88028	15.922	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	63.680%	
21) 2-Butanone-d5	7.075	46		137558	42.577	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	85.160%	
24) Chloroform-d	7.648	84		457500m	19.935	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	79.720%	
26) 1,2-Dichloroethane-d4	8.307	65		248914	19.654	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	78.600%	
32) Benzene-d6	8.276	84		937489	20.885	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	83.520%	
36) 1,2-Dichloropropane-d6	9.270	67		287911	20.591	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	82.360%	
41) Toluene-d8	10.325	98		804410	20.876	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	83.520%	
43) trans-1,3-Dichloroprop...	10.575	79		110527	19.145	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	76.600%	
47) 2-Hexanone-d5	10.922	63		70066	47.689	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	95.380%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		273775	24.793	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	99.160%	
66) 1,2-Dichlorobenzene-d4	13.848	152		306387	24.648	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	98.600%	
Target Compounds							
13) Acetone	4.125	43		10083	3.139	ug/L	95
16) Methylene chloride	4.923	84		50124	3.789	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
Data File : VW026985.D
Acq On : 01 Sep 2023 11:36
Operator : SY/MD
Sample : 04175-13
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/04/2023
Supervised By :Mahesh Dadoda 09/04/2023

Quant Time: Sep 02 00:33:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 02 00:33:01 2023
Response via : Initial Calibration

