

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
 Data File : VW026986.D
 Acq On : 01 Sep 2023 12:00
 Operator : SY/MD
 Sample : 04235-04
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Sep 02 00:34:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 02 00:33:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	661361	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	646088	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	341560	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	200464	18.438	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.760%
7) Chloroethane-d5	2.899	69	184317	22.799	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.200%
11) 1,1-Dichloroethene-d2	4.021	65	78880	14.752	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.000%
21) 2-Butanone-d5	7.075	46	113890	36.447	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.900%
24) Chloroform-d	7.648	84	414327	18.666	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.680%
26) 1,2-Dichloroethane-d4	8.307	65	221374	18.072	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	72.280%
32) Benzene-d6	8.276	84	844183	18.959	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.840%
36) 1,2-Dichloropropane-d6	9.276	67	257253	18.547	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.200%
41) Toluene-d8	10.325	98	728750	19.066	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.280%
43) trans-1,3-Dichloroprop...	10.581	79	95471	16.671	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.680%
47) 2-Hexanone-d5	10.922	63	58442	40.100	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.200%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	238956	21.815	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	278546	22.784	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.120%
Target Compounds						Qvalue
16) Methylene chloride	4.929	84	59369	4.641	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090123\
Data File : VW026986.D
Acq On : 01 Sep 2023 12:00
Operator : SY/MD
Sample : 04235-04
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Sep 02 00:34:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM081023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 02 00:33:01 2023
Response via : Initial Calibration

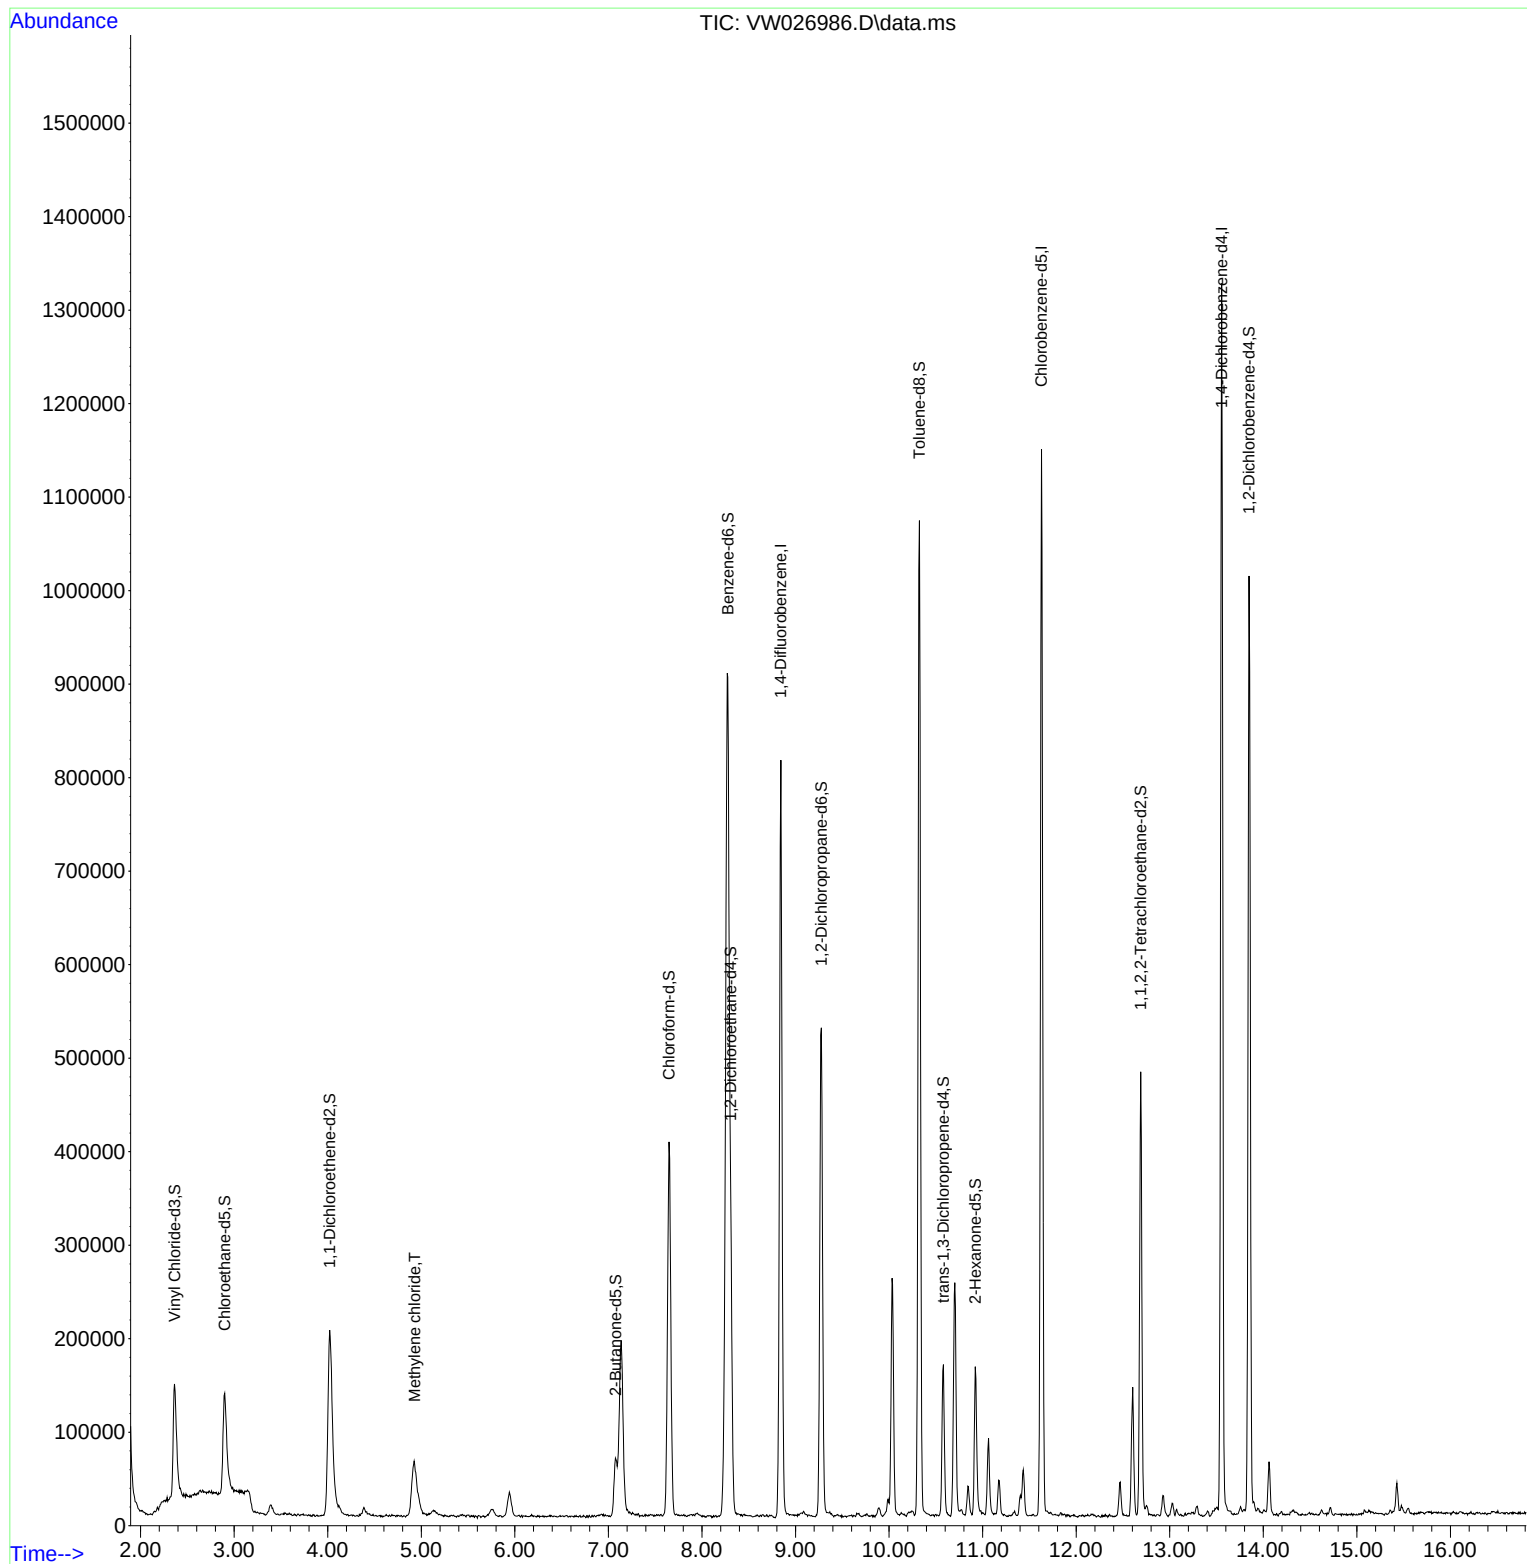

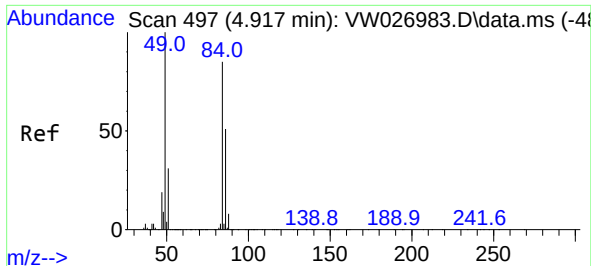

#16
Methylene chloride
Concen: 4.641 ug/L
RT: 4.929 min Scan# 49
Delta R.T. 0.012 min
Lab File: VW026986.D
Acq: 01 Sep 2023 12:00

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 59369
Ion Ratio Lower Upper
84 100
86 59.0 43.5 80.9
49 109.3 96.0 178.2

