


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090320\
Data File : VW016454.D
Acq On : 03 Sep 2020 18:30
Operator : SY/VA
Sample : VIBLK19
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VIBLK19

Manual Integrations
APPROVED

MMDadoda
9/4/2020 3:37:04 PM

Quant Time: Sep 04 06:17:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 04 04:59:18 2020
Response via : Initial Calibration

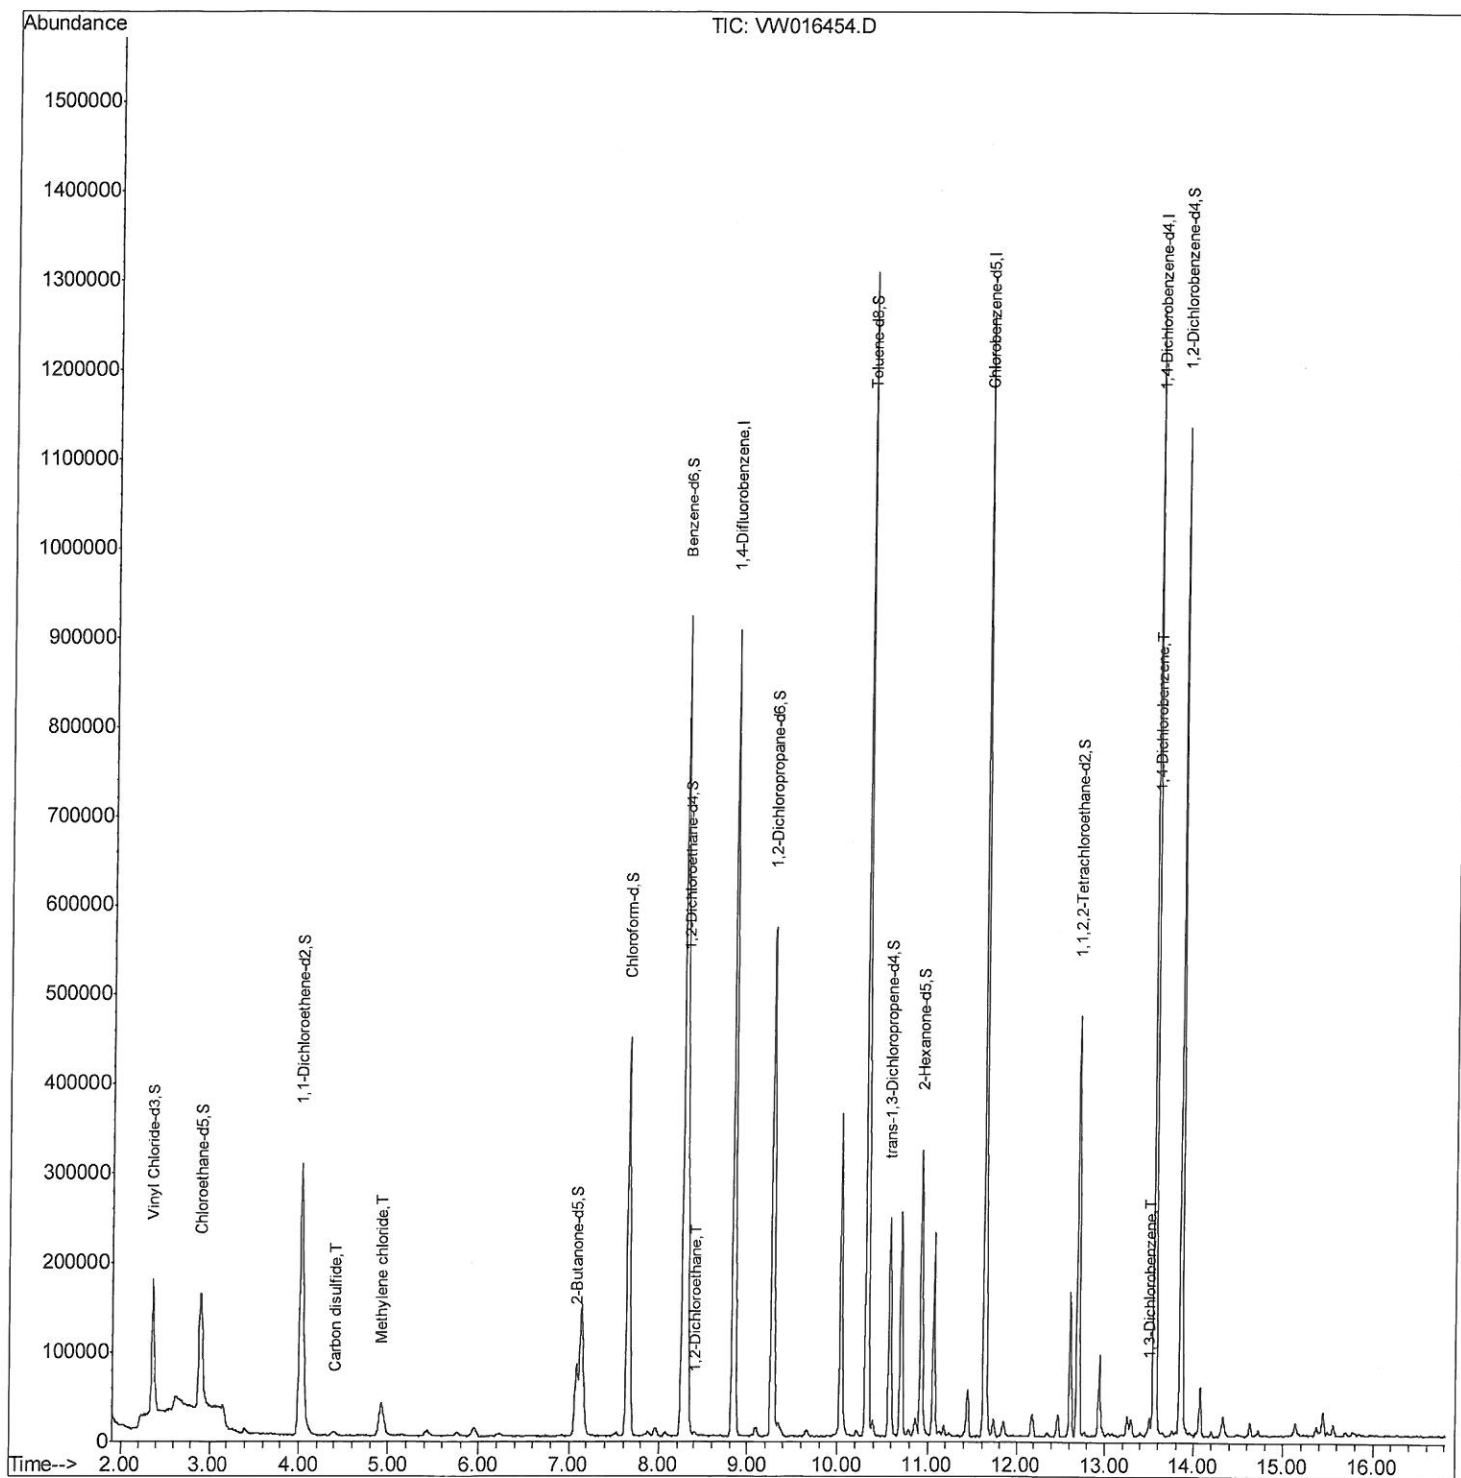

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090320\
 Data File : VW016454.D
 Acq On : 03 Sep 2020 18:30
 Operator : SY/VA
 Sample : VIBLK19
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK19

Manual Integrations
 APPROVED

MMDadoda
 9/4/2020 3:37:04 PM

Quant Time: Sep 04 05:37:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 04 04:59:18 2020
 Response via : Initial Calibration

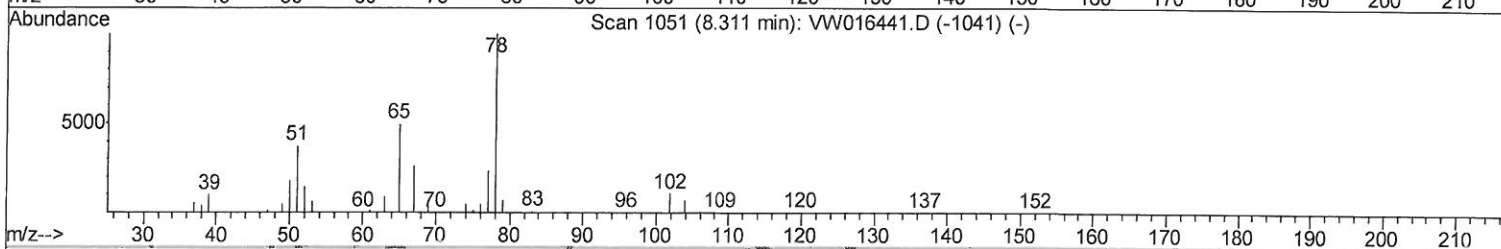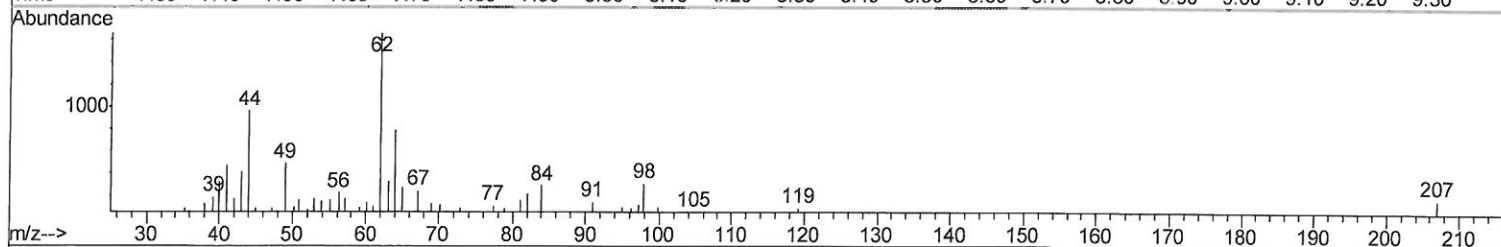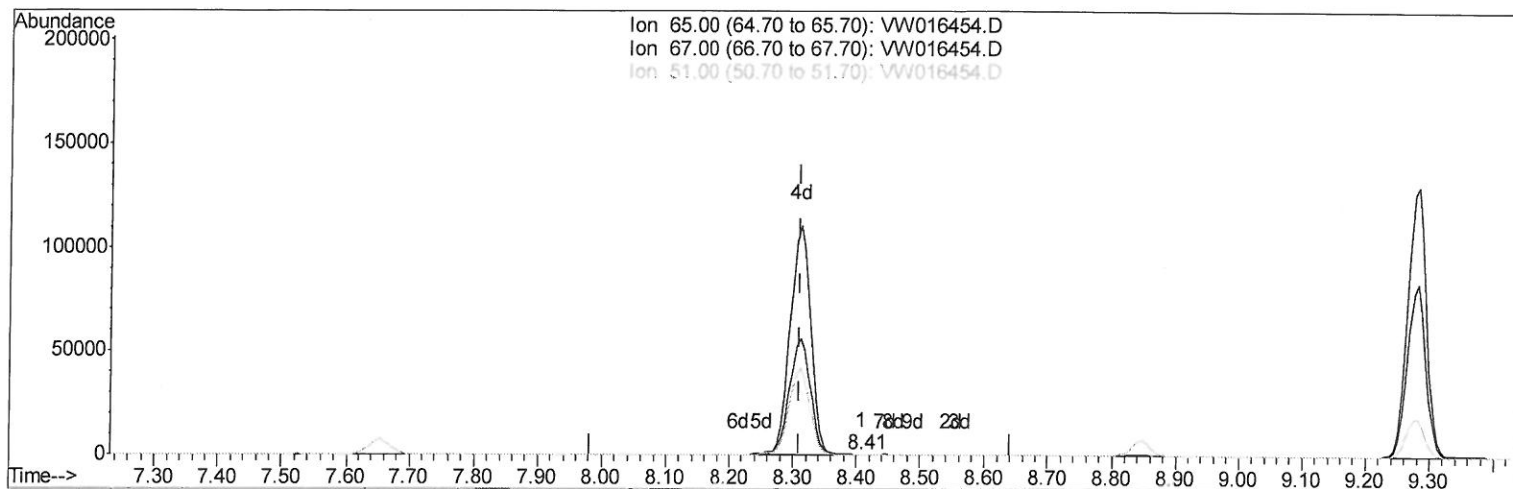

TIC: VW016454.D

(26) 1,2-Dichloroethane-d4 (S)

8.409min (+0.098) 0.03ug/L

response 320

Ion	Exp%	Act%
65.00	100	100
67.00	53.50	52.50
51.00	104.30	78.13
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090320\
 Data File : VW016454.D
 Acq On : 03 Sep 2020 18:30
 Operator : SY/VA
 Sample : VIBLK19
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK19

Manual Integrations
 APPROVED

MMDadoda
 9/4/2020 3:37:04 PM

Quant Time: Sep 04 05:37:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 04 04:59:18 2020
 Response via : Initial Calibration

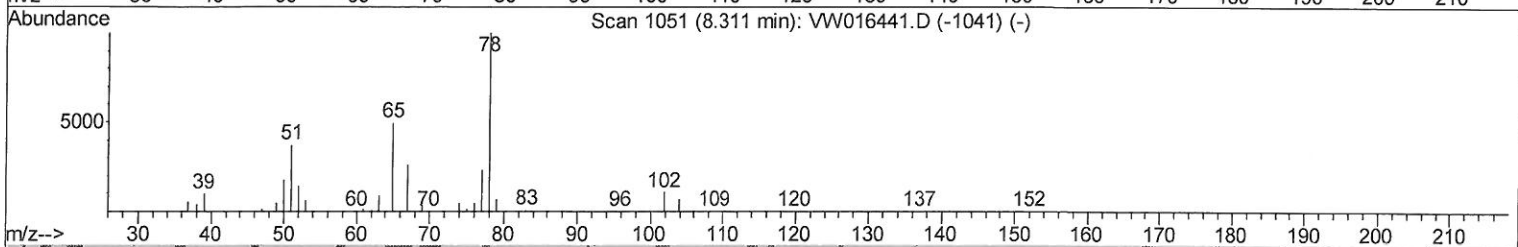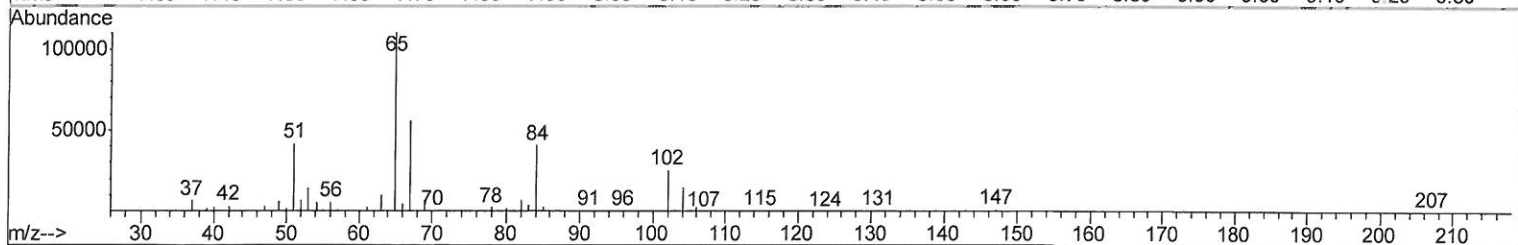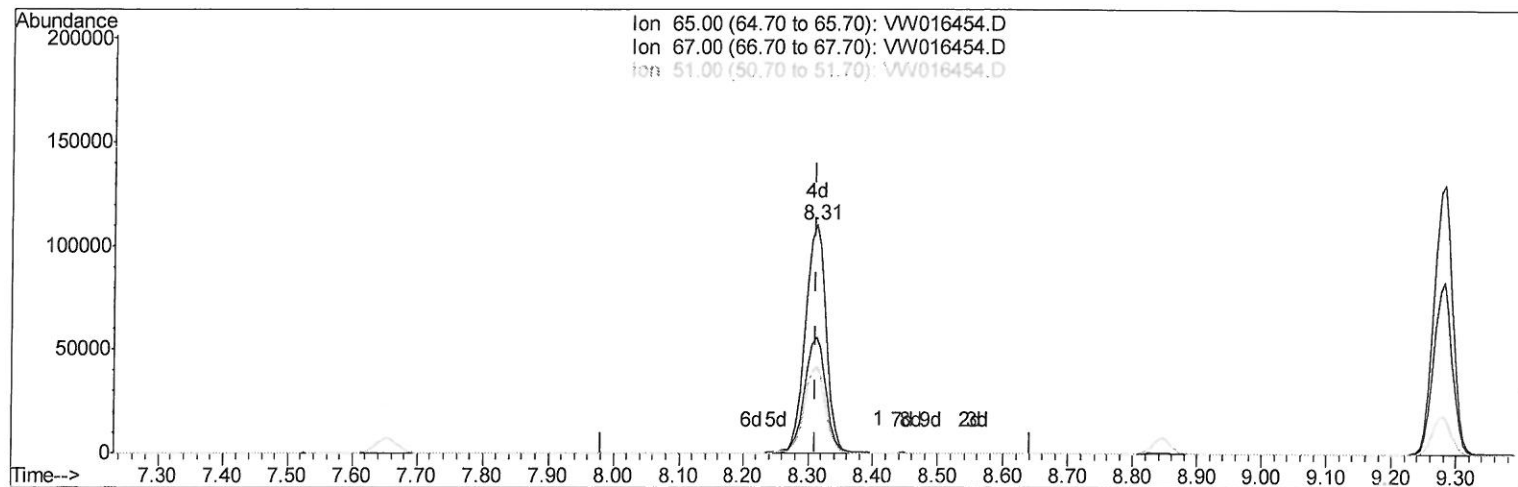

TIC: VW016454.D

(26) 1,2-Dichloroethane-d4 (S)

8.311min (+0.000) 24.67ug/L m

response 245454

Ion	Exp%	Act%
65.00	100	100
67.00	53.50	0.07#
51.00	104.30	0.10#
0.00	0.00	0.00

209/08/20 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090320\
 Data File : VW016454.D
 Acq On : 03 Sep 2020 18:30
 Operator : SY/VA
 Sample : VIBLK19
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK19

Manual Integrations
 APPROVED

MMDadoda
 9/4/2020 3:37:04 PM

Quant Time: Sep 04 06:17:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 04 04:59:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	776808	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	704373	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	325366	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	199281	24.18	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.72%
7) Chloroethane-d5	2.90	69	183380	24.78	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.12%
10) 1,1-Dichloroethene-d2	4.03	63	319685	16.87	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.48%
20) 2-Butanone-d5	7.08	46	137739	46.80	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.60%
24) Chloroform-d	7.65	84	438563	24.10	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.40%
26) 1,2-Dichloroethane-d4	8.31	65	245454m	24.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.68%
29) Benzene-d6	8.28	84	881090	24.61	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.44%
33) 1,2-Dichloropropane-d6	9.28	67	260370	24.75	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.00%
37) Toluene-d8	10.33	98	867931	25.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.00%
38) trans-1,3-Dichloropropene-	10.58	79	130049	24.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.00%
39) 2-Hexanone-d5	10.93	63	110902	51.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.16%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	226126	25.42	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.68%
61) 1,2-Dichlorobenzene-d4	13.86	152	299807	26.66	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.64%

09/28/2020

Target Compounds

					Ovalue
14) Carbon disulfide	4.40	76	6638	0.227 ug/L	97
16) Methylene chloride	4.92	84	31167	2.571 ug/L	94
27) 1,2-Dichloroethane	8.40	62	3708	0.311 ug/L #	84
63) 1,3-Dichlorobenzene	13.50	146	6437	0.314 ug/L	93
64) 1,4-Dichlorobenzene	13.58	146	6825	0.336 ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed