


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW090418\
 Data File : VW005076.D
 Acq On : 04 Sep 2018 12:10
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090118S.M
 Title : SW846 8260
 Last Update : Sat Sep 01 03:35:05 2018

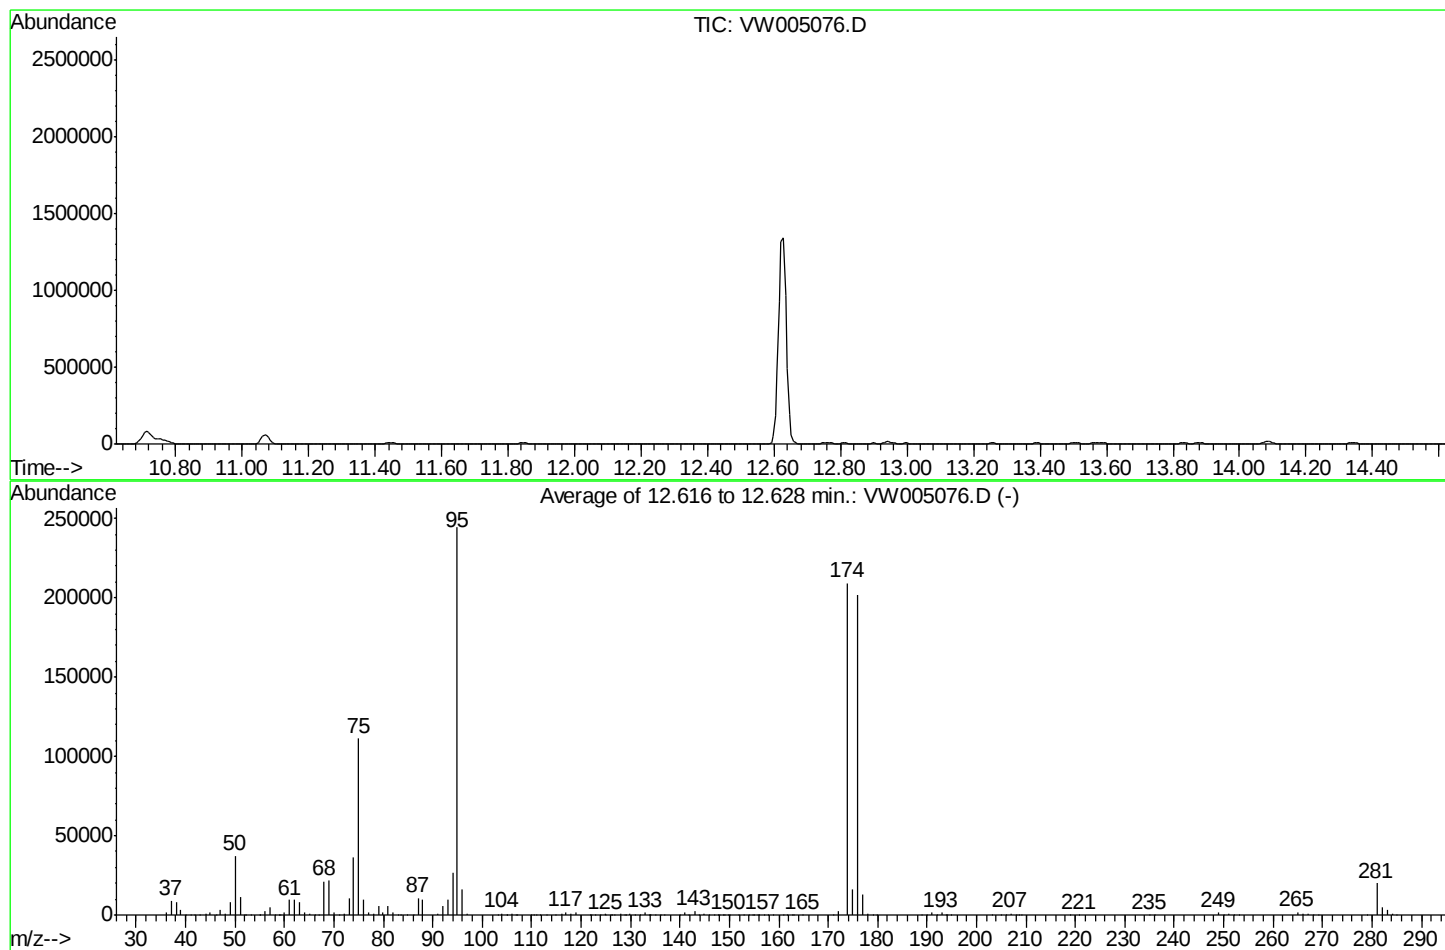

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	37461	PASS
75	95	30	60	45.5	111189	PASS
95	95	100	100	100.0	244437	PASS
96	95	5	9	6.6	16030	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.5	209109	PASS
175	174	5	9	7.7	16023	PASS
176	174	95	101	96.6	201984	PASS
177	176	5	9	6.6	13257	PASS