


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW090618\
 Data File : VW005153.D
 Acq On : 06 Sep 2018 10:11
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090118S.M
 Title : SW846 8260
 Last Update : Sat Sep 01 03:35:05 2018

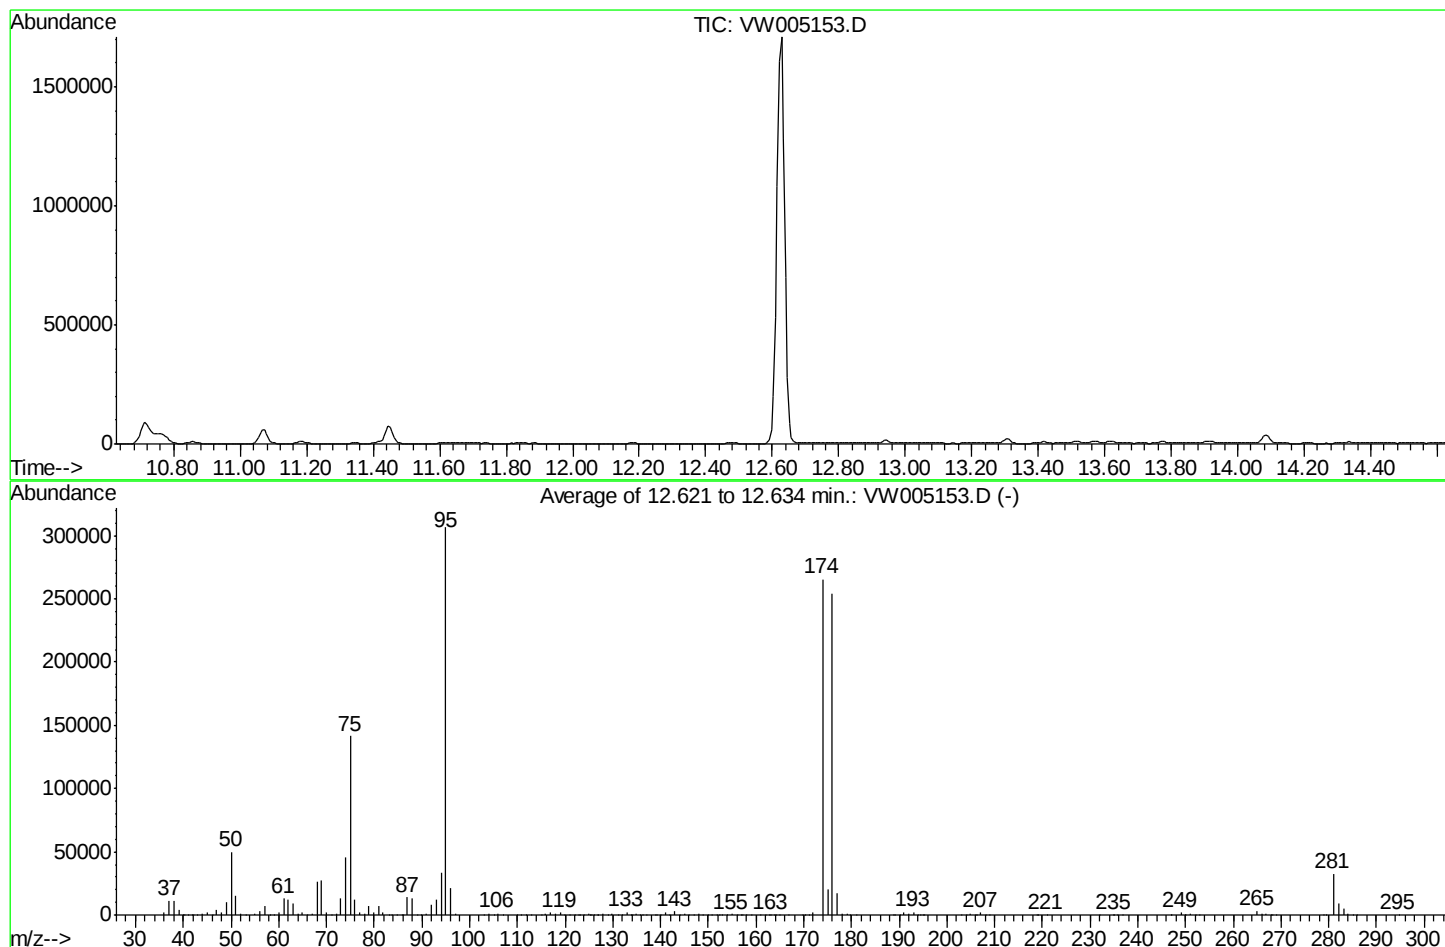

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	50034	PASS
75	95	30	60	46.1	141480	PASS
95	95	100	100	100.0	306581	PASS
96	95	5	9	6.9	21290	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.6	265621	PASS
175	174	5	9	7.6	20152	PASS
176	174	95	101	95.8	254464	PASS
177	176	5	9	6.6	16856	PASS