


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW090718\
Data File : VW005201.D
Acq On : 07 Sep 2018 10:05
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090118S.M
Title : SW846 8260
Last Update : Sat Sep 08 02:36:58 2018

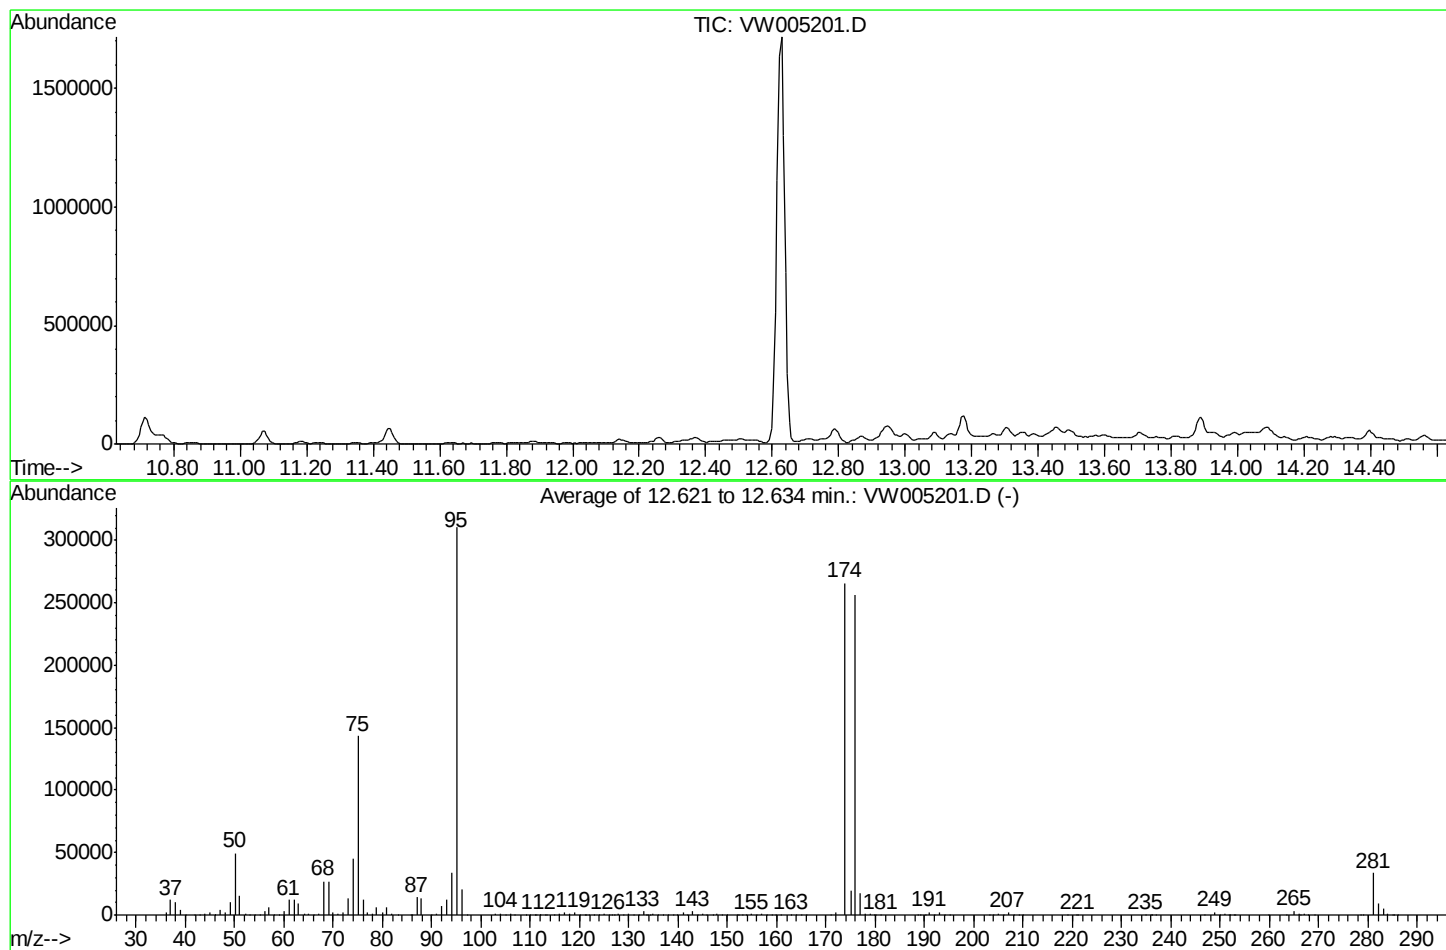

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	49629	PASS
75	95	30	60	46.1	143136	PASS
95	95	100	100	100.0	310533	PASS
96	95	5	9	6.5	20238	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.6	265920	PASS
175	174	5	9	7.4	19650	PASS
176	174	95	101	96.5	256490	PASS
177	176	5	9	6.9	17607	PASS