


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090721\
Data File : VW019978.D
Acq On : 07 Sep 2021 10:24
Operator : SY/VA
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W090721S.M
Title : SW846 8260
Last Update : Wed Sep 08 12:18:21 2021

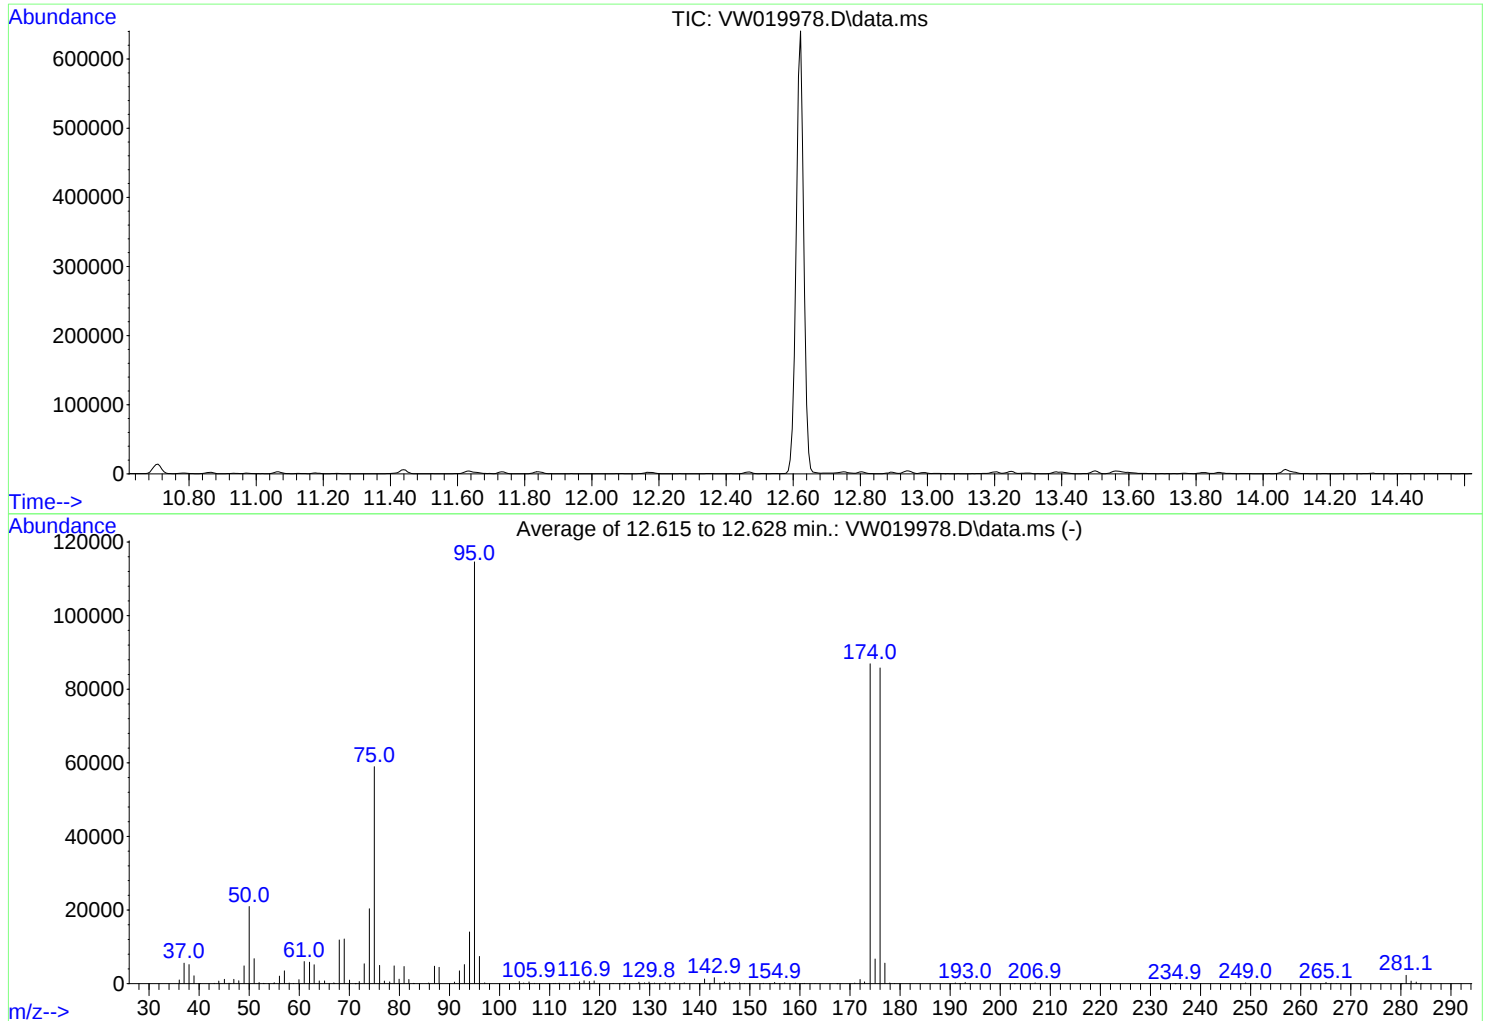

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	20941	PASS
75	95	30	60	51.4	58968	PASS
95	95	100	100	100.0	114627	PASS
96	95	5	9	6.5	7414	PASS
173	174	0.00	2	0.5	476	PASS
174	95	50	100	75.8	86923	PASS
175	174	5	9	7.7	6683	PASS
176	174	95	101	98.7	85811	PASS
177	176	5	9	6.5	5555	PASS