

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090722\
 Data File : VW024569.D
 Acq On : 07 Sep 2022 13:16
 Operator : SY/VA
 Sample : N4483-01RE
 Misc : 6.40g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW351

Quant Time: Sep 08 01:19:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 07 04:52:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	338864	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	317372	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	105148	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	102006	14.580	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.320%
7) Chloroethane-d5	2.879	69	108860	20.926	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.720%
11) 1,1-Dichloroethene-d2	4.013	63	65884	8.926	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	35.720%#
21) 2-Butanone-d5	7.080	46	63237	56.030	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.060%
24) Chloroform-d	7.647	84	206169	23.888	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.560%
26) 1,2-Dichloroethane-d4	8.305	65	129354	26.583	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.320%
32) Benzene-d6	8.275	84	305872	19.593	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.360%
36) 1,2-Dichloropropane-d6	9.275	67	116240	25.254	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.000%
41) Toluene-d8	10.323	98	236492	15.539	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	62.160%
43) trans-1,3-Dichloroprop...	10.573	79	43514	21.095	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.400%
47) 2-Hexanone-d5	10.927	63	51565	60.948	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.900%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	123860	28.076	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	112.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	87002	26.124	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.480%
Target Compounds					Qvalue	
48) 2-Hexanone	10.951	43	6446	3.167	ug/L #	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090722\
Data File : VW024569.D
Acq On : 07 Sep 2022 13:16
Operator : SY/VA
Sample : N4483-01RE
Misc : 6.40g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW351


Quant Time: Sep 08 01:19:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 07 04:52:14 2022
Response via : Initial Calibration

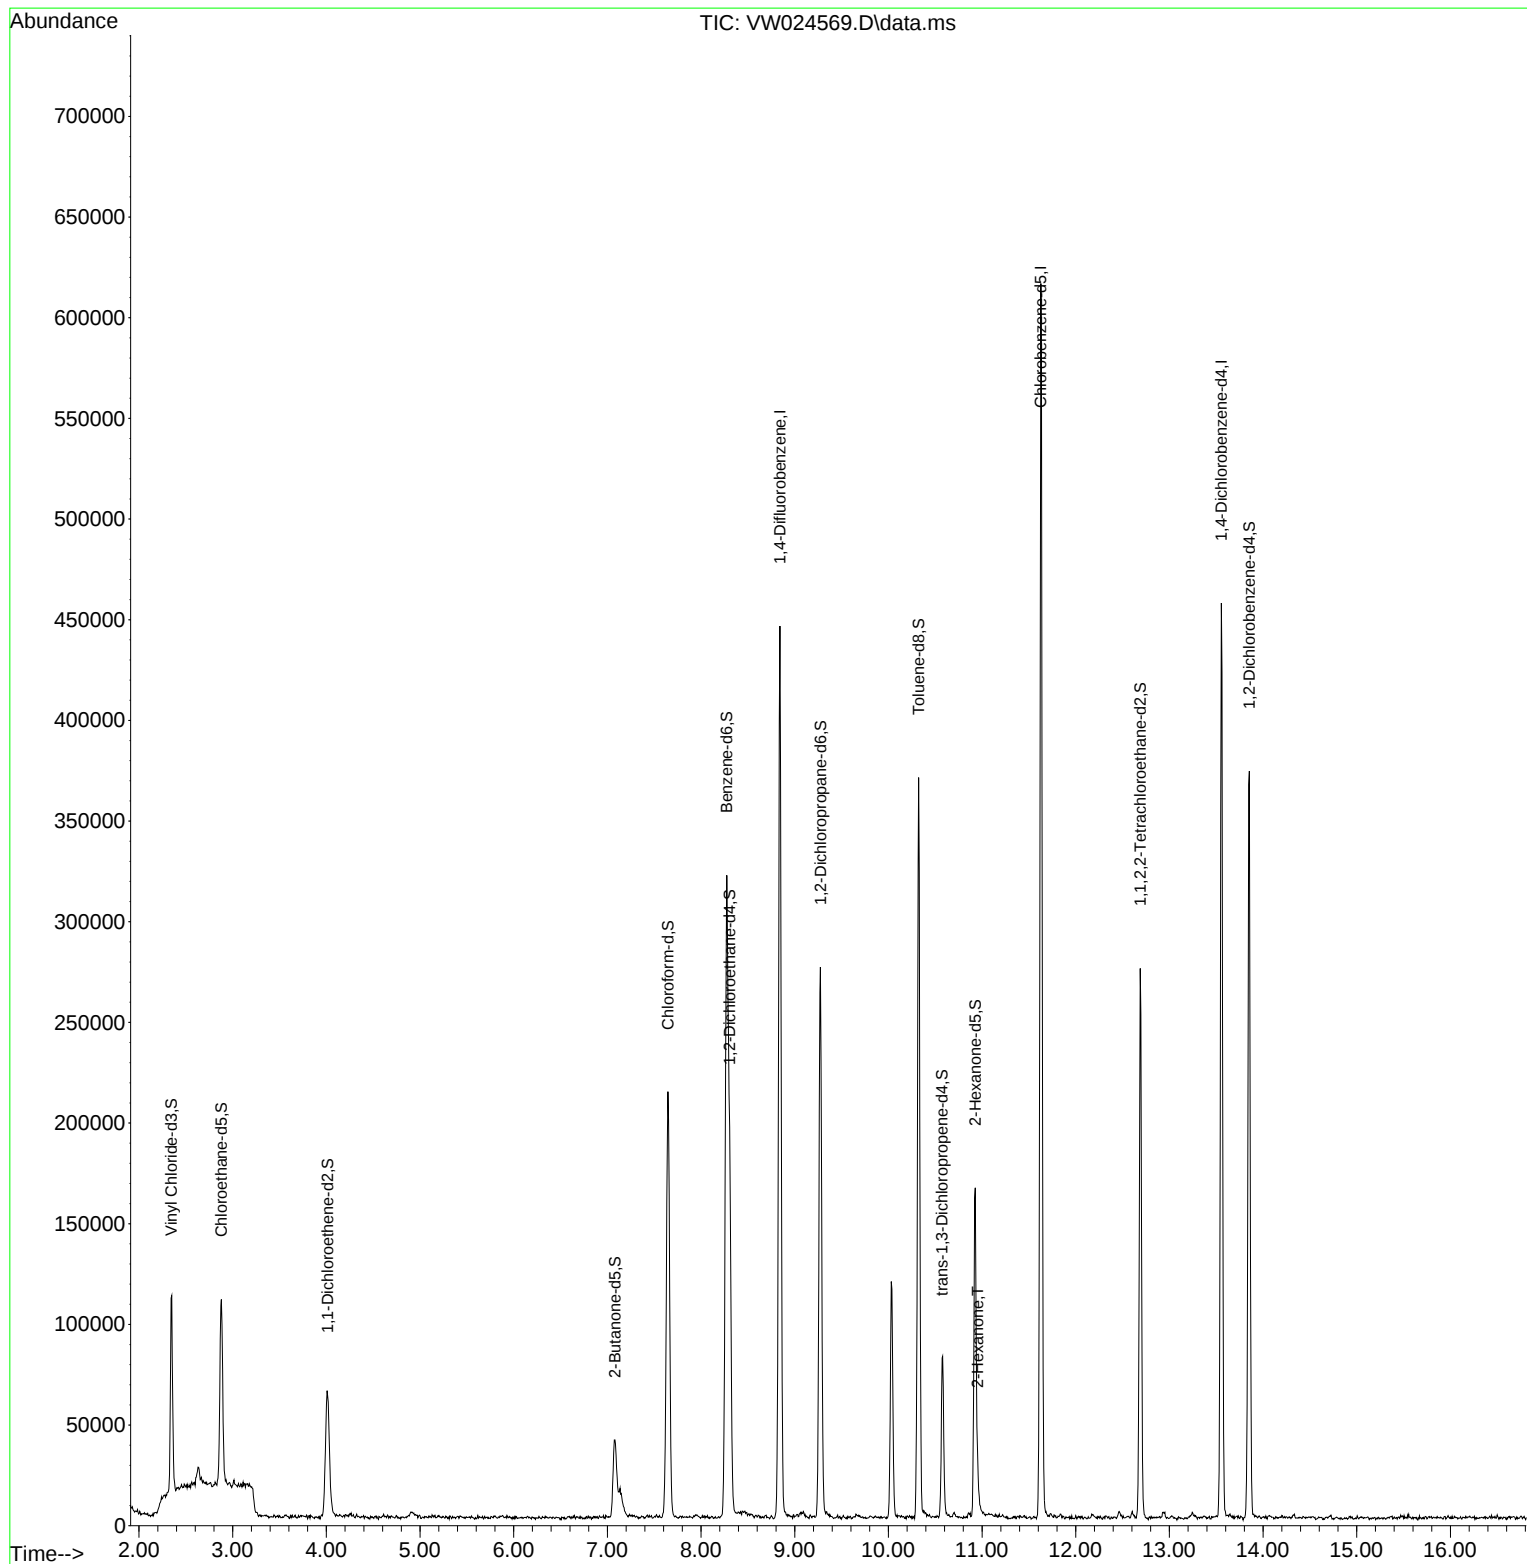

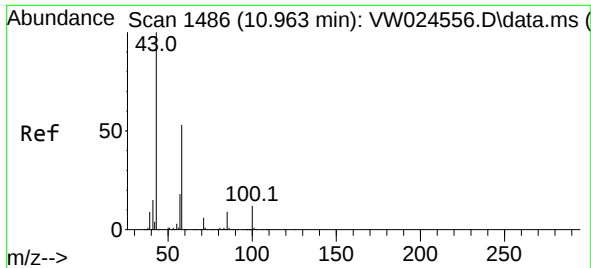

#48
 2-Hexanone
 Concen: 3.167 ug/L
 RT: 10.951 min Scan# 14
 Delta R.T. -0.012 min
 Lab File: VW024569.D
 Acq: 07 Sep 2022 13:16

Instrument :
 MSVOA_W
 ClientSampleId :
 EW351

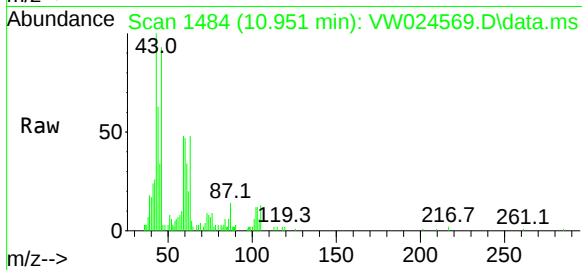

Tgt Ion: 43	Resp: 6446
Ion Ratio	Lower Upper
43	100
58	0.0 43.7 65.5#
57	0.0 15.3 22.9#
100	0.9 11.2 16.8#

