



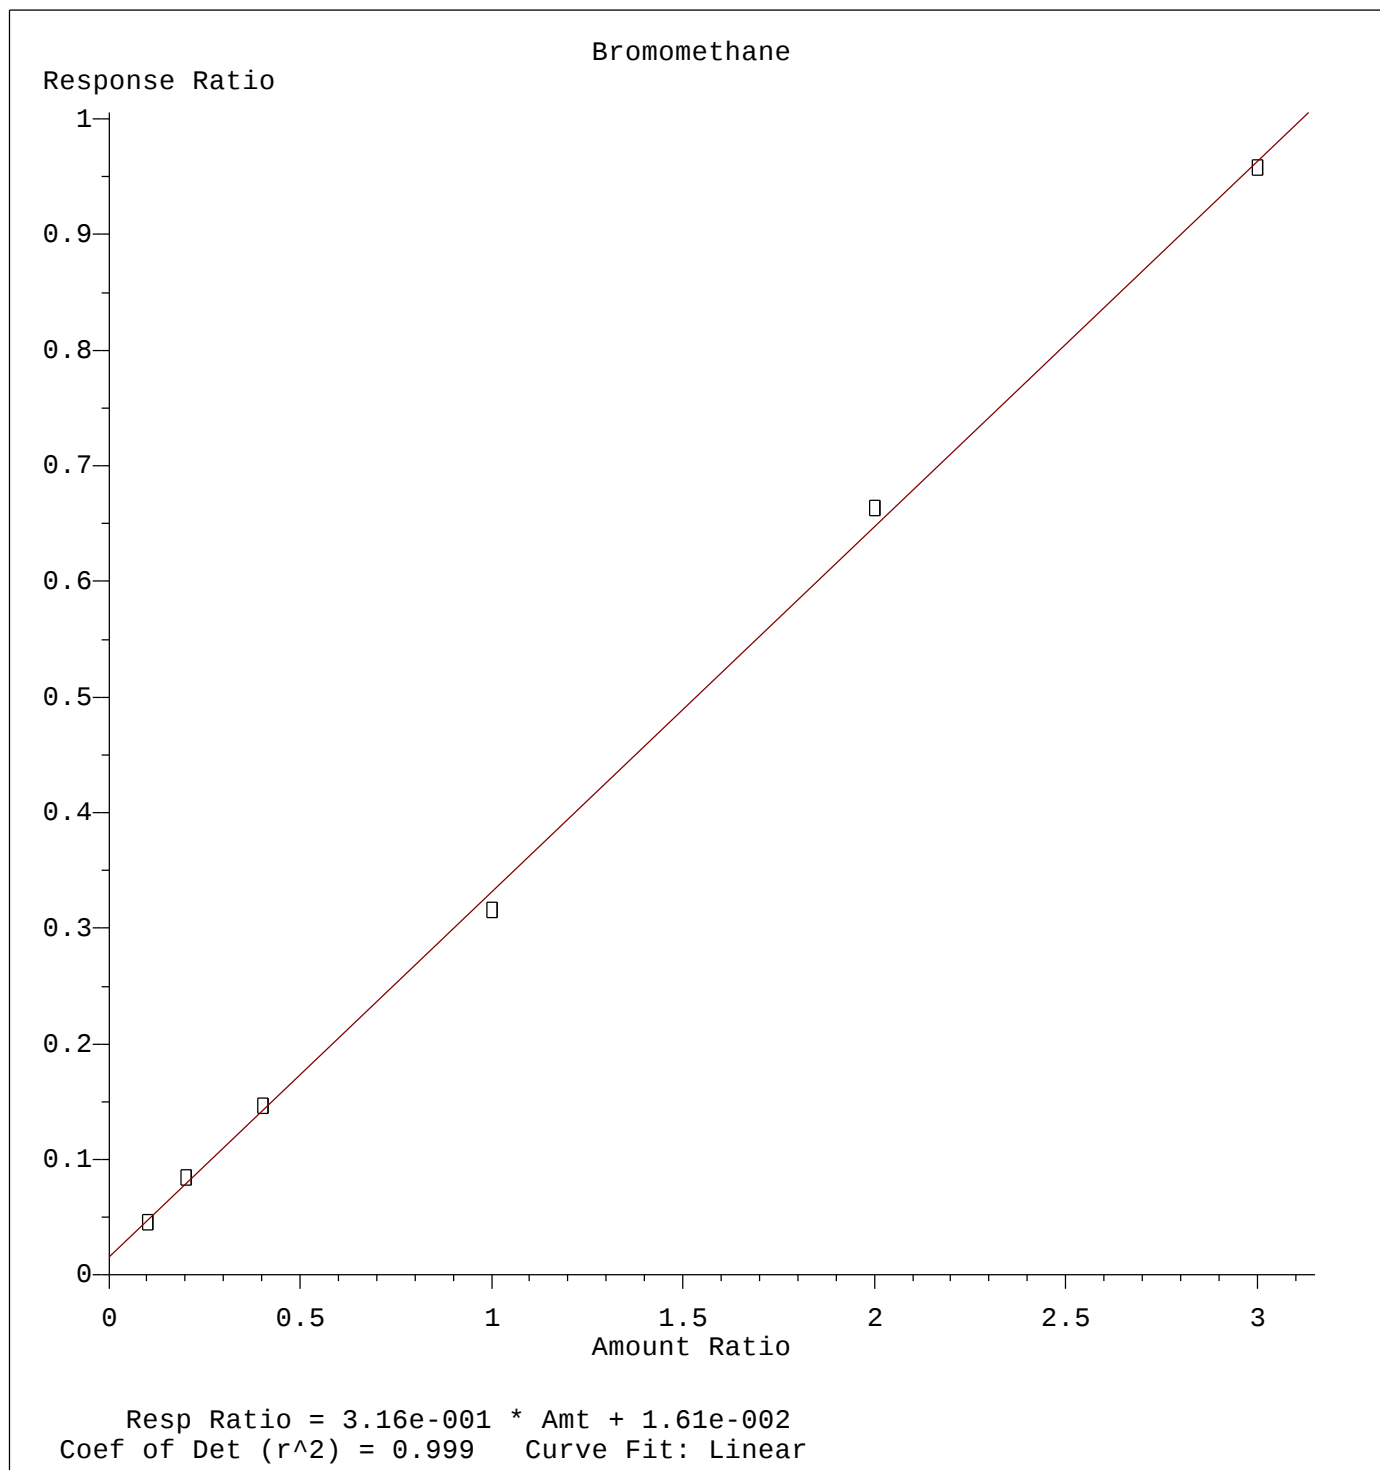

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090818S.M
Calibration Table Last Updated: Sat Sep 08 03:55:32 2018

Naphthalene

Response Ratio

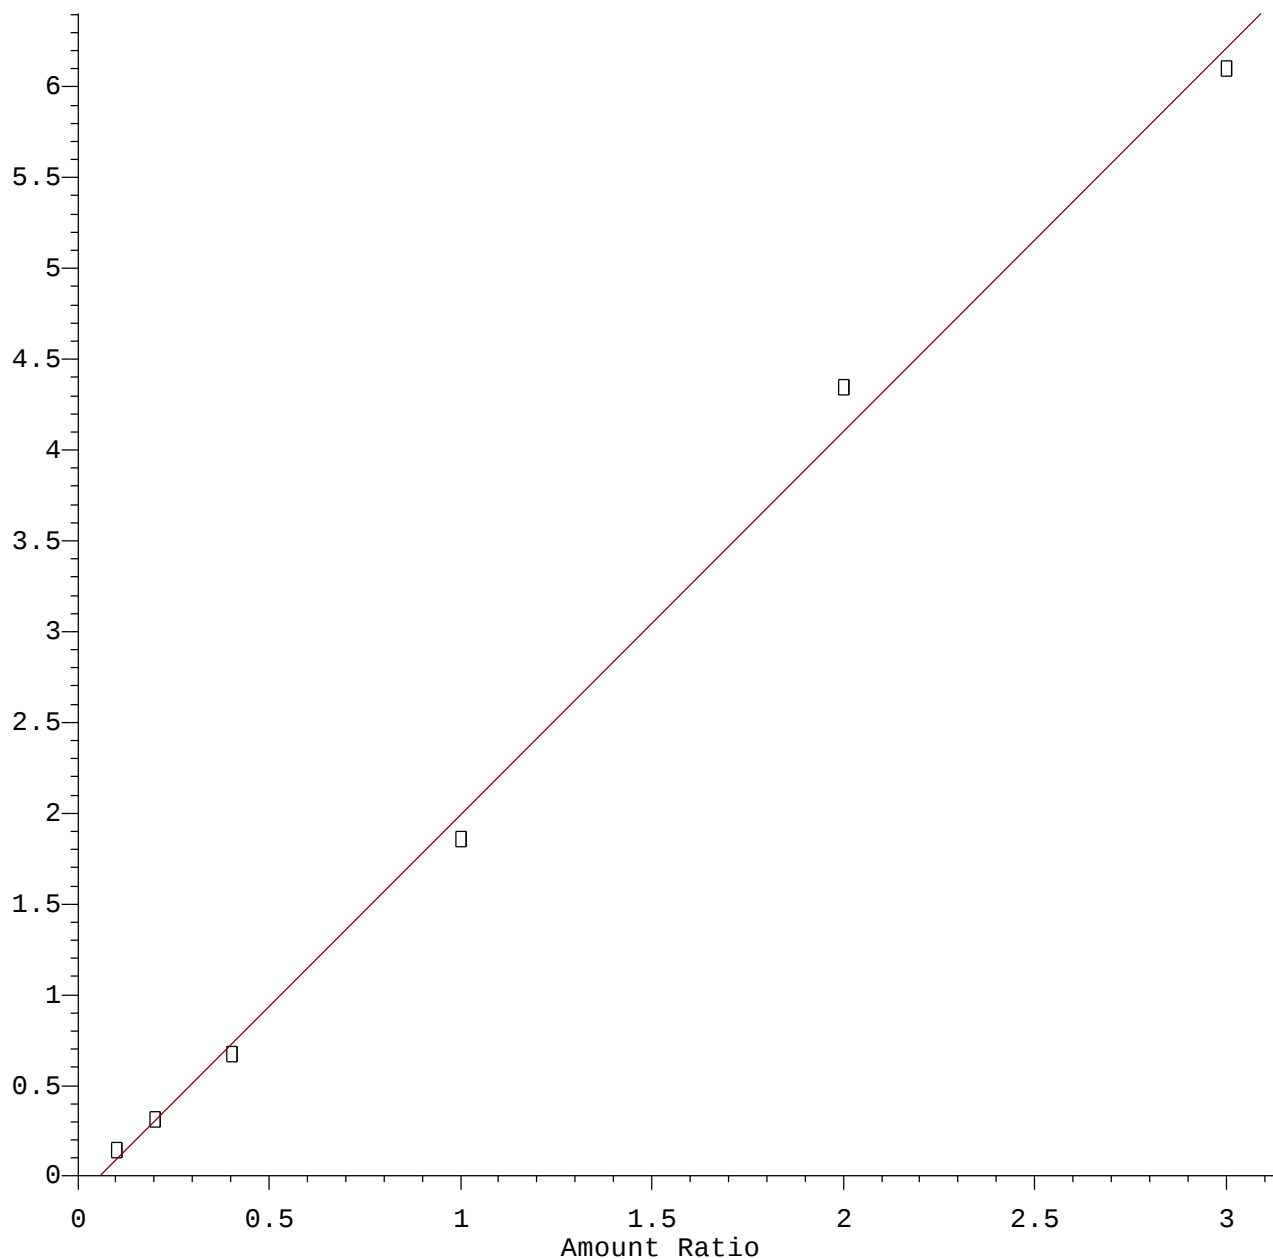


Resp Ratio = 2.11e+000 * Amt - 1.20e-001
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090818S.M
Calibration Table Last Updated: Sat Sep 08 03:55:32 2018


Methylene Chloride

Response Ratio

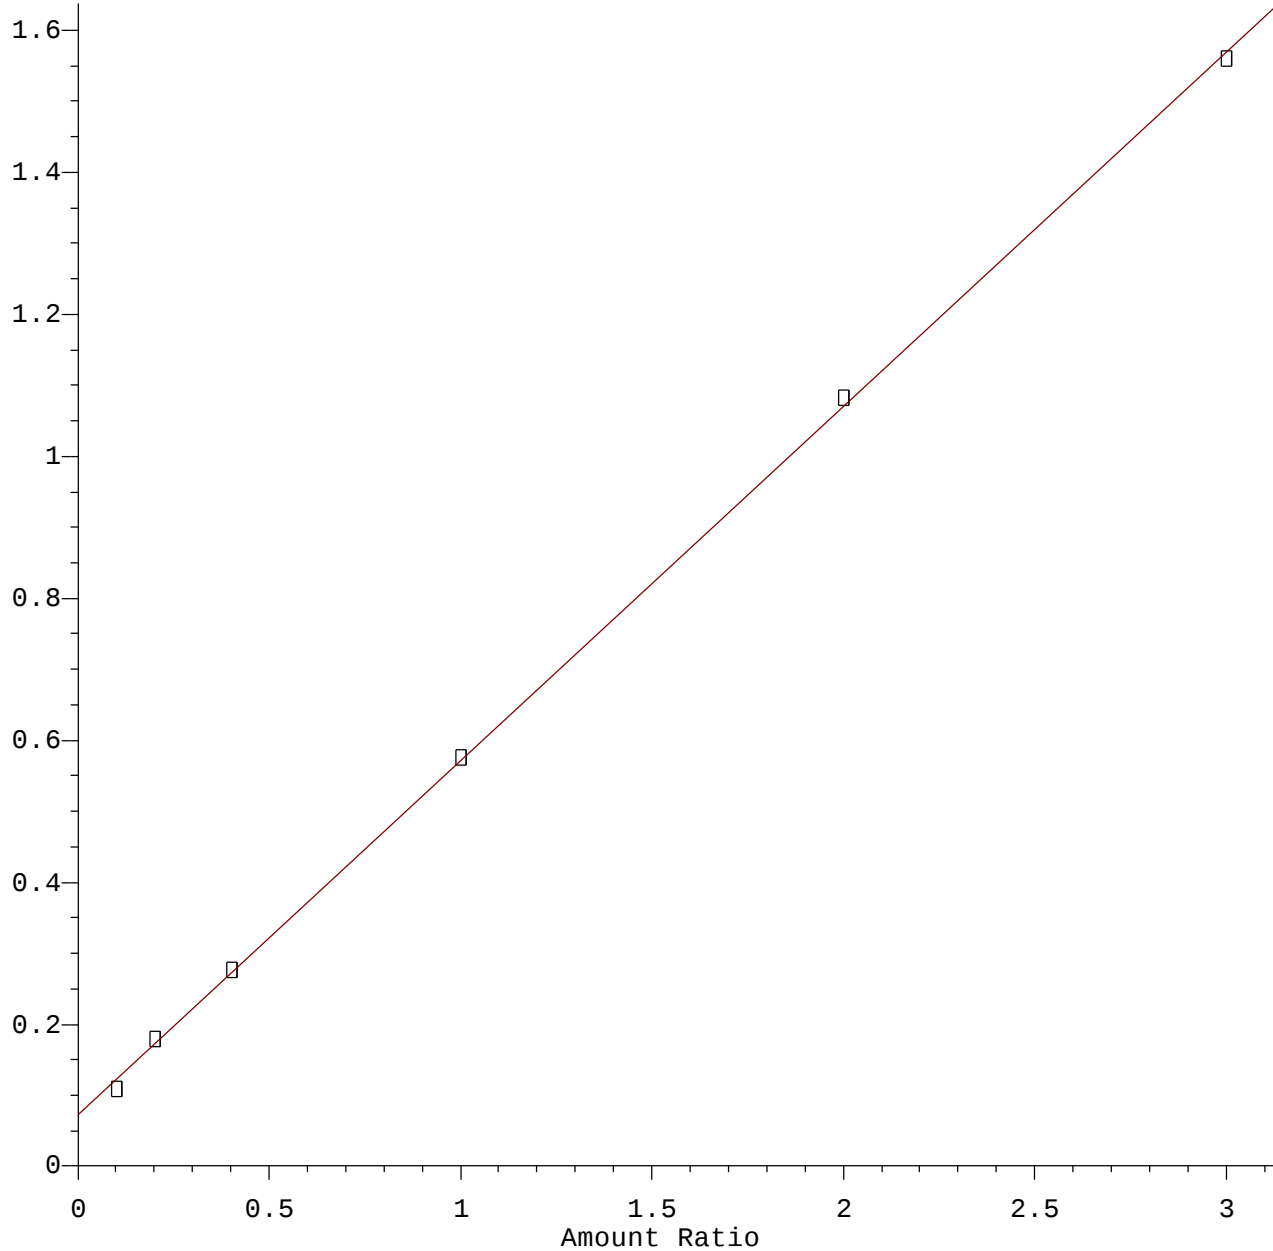

Resp Ratio = $4.99 \times 10^{-1} \times \text{Amt} + 7.32 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090818S.M
Calibration Table Last Updated: Sat Sep 08 03:55:32 2018

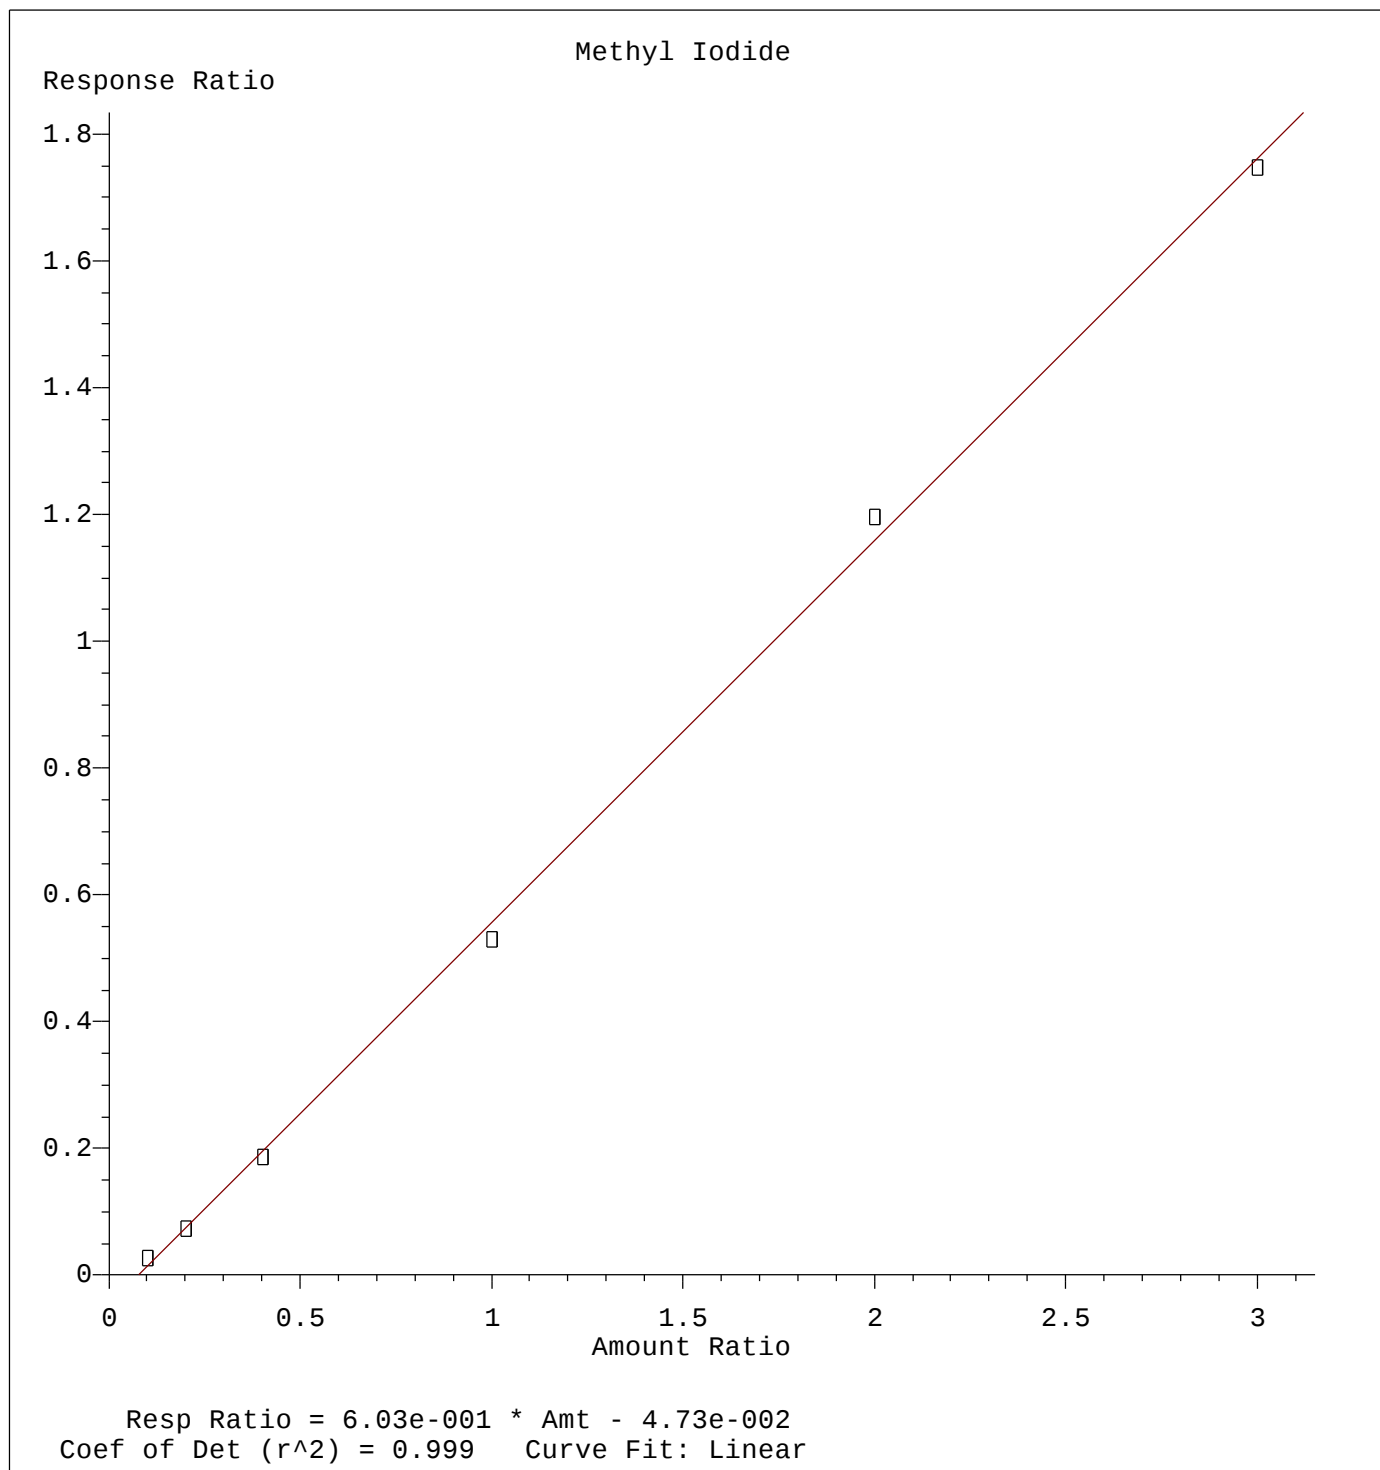

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090818S.M
Calibration Table Last Updated: Sat Sep 08 03:55:32 2018