

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090819\
 Data File : VW012780.D
 Acq On : 08 Sep 2019 19:53
 Operator : SY/VA
 Sample : K4603-18
 Misc : 4.62G/5ML/MSVOA W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 PAR-12-F3-(3.11)

Quant Time: Sep 09 08:16:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090719S.M
 Quant Title : SW846 8260
 QLast Update : Sun Sep 08 05:04:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	203507	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	304805	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	249742	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.55	152	96035	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	119755	52.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.34%	
35) Dibromofluoromethane	7.88	113	91352	50.41	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.82%	
50) Toluene-d8	10.32	98	359550	50.64	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.28%	
62) 4-Bromofluorobenzene	12.62	95	109151	42.35	ug/l	0.00
Spiked Amount 50.000			Recovery	=	84.70%	
Target Compounds						
29) Tetrahydrofuran	7.55	42	4356	8.702	ug/l	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW090819\
Data File : VW012780.D
Acq On : 08 Sep 2019 19:53
Operator : SY/VA
Sample : K4603-18
Misc : 4.62G/5ML/MSVOA W/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
PAR-12-F3-(3.11)

Quant Time: Sep 09 08:16:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W090719S.M
Quant Title : SW846 8260
QLast Update : Sun Sep 08 05:04:40 2019
Response via : Initial Calibration

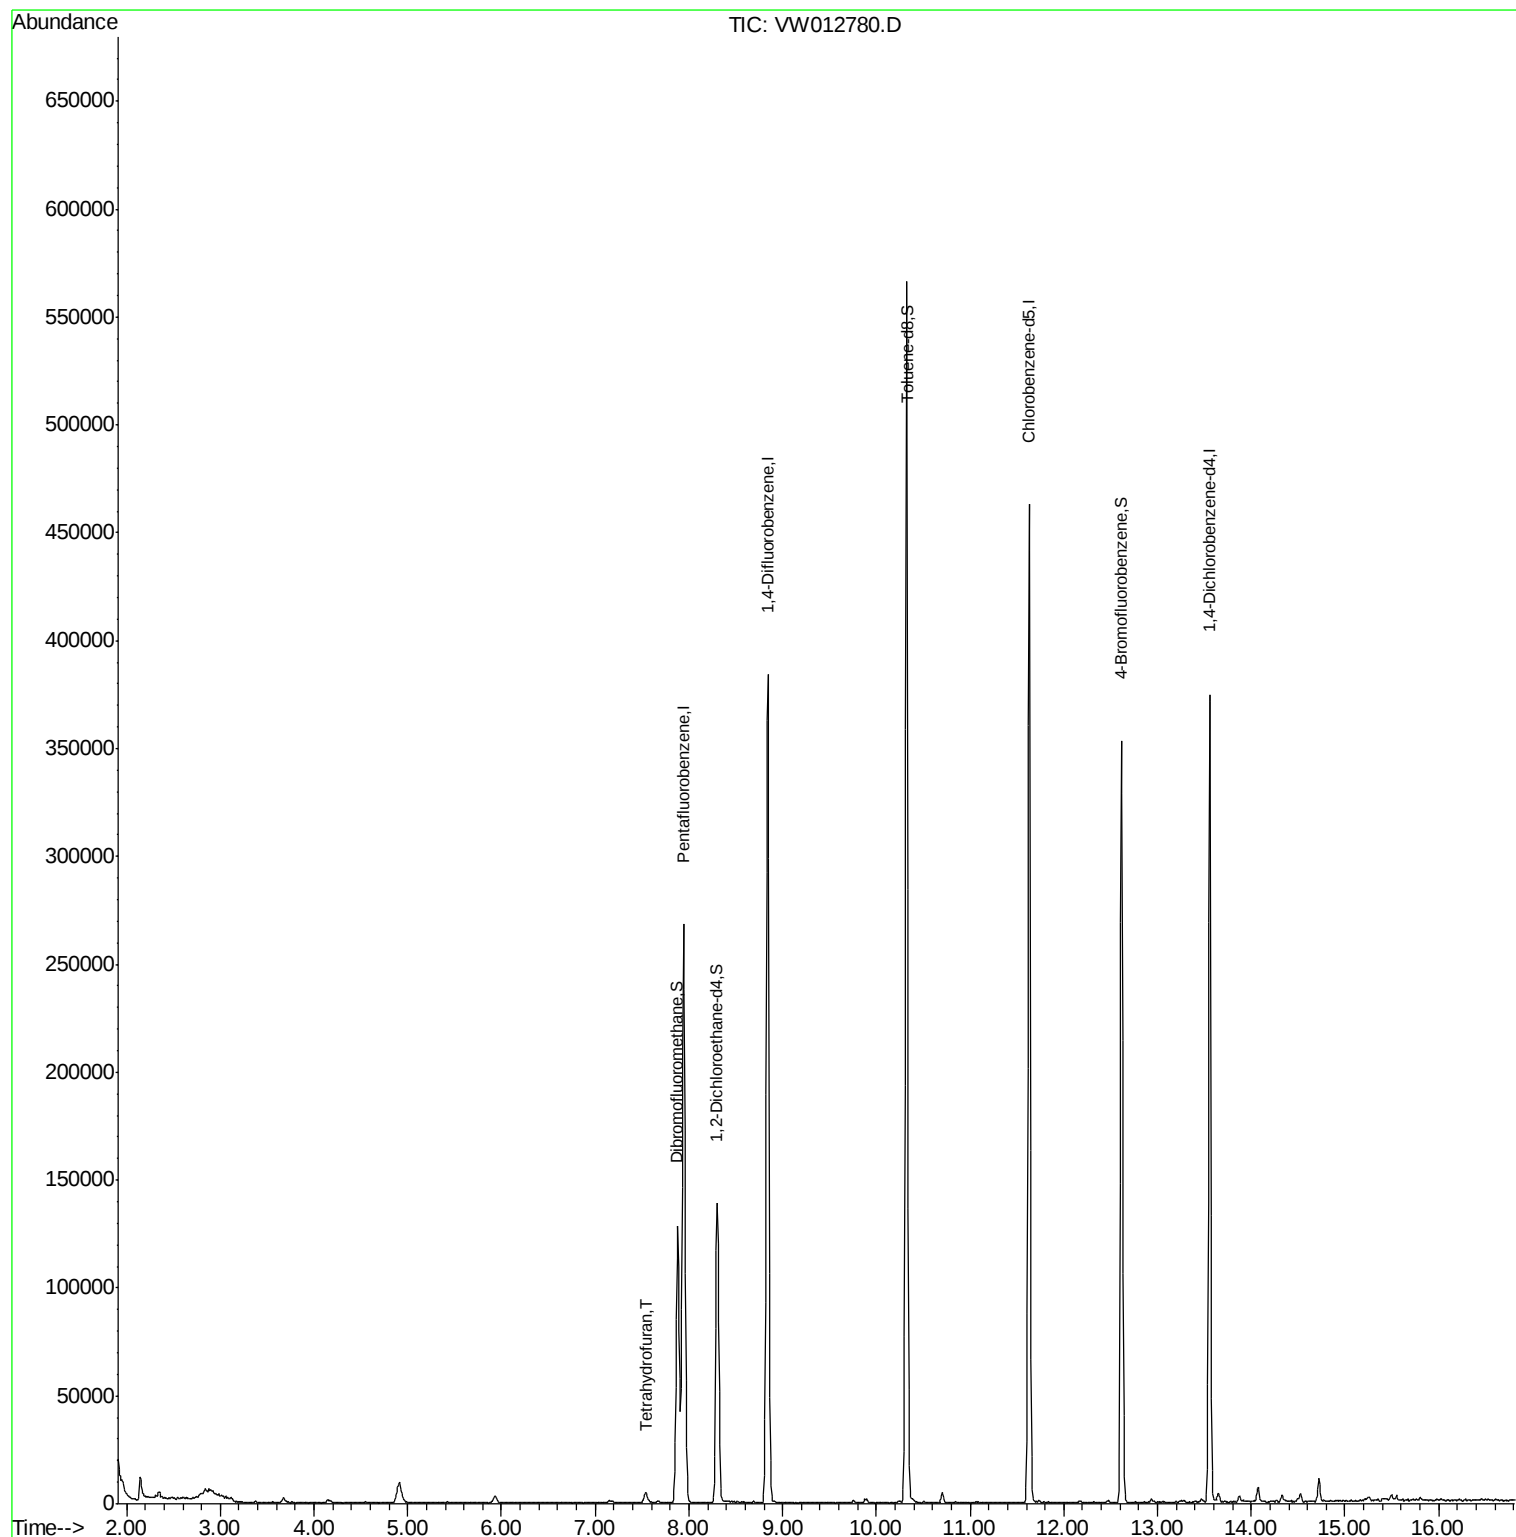

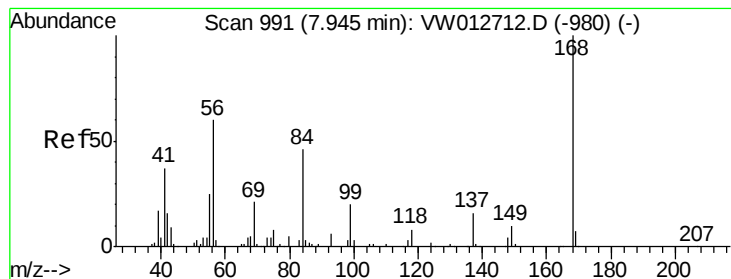

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW012780.D

Acq: 08 Sep 2019 19:53

Instrument :

MSVOA_W

ClientSampleId :


PAR-12-F3-(3.11)

Tot Ion:168 Resp: 203507

Ion Ratio Lower Upper

168 100

99 59.3 47.8 71.6

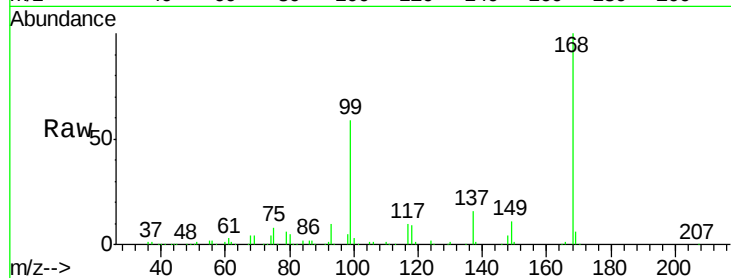

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time-->

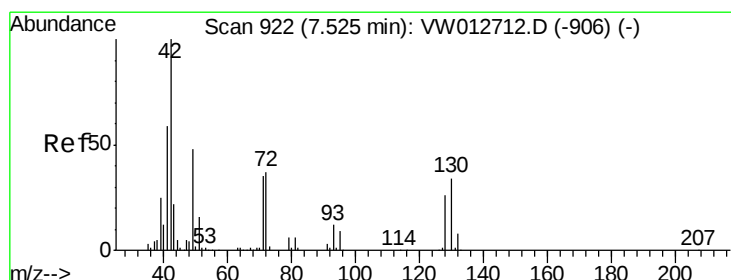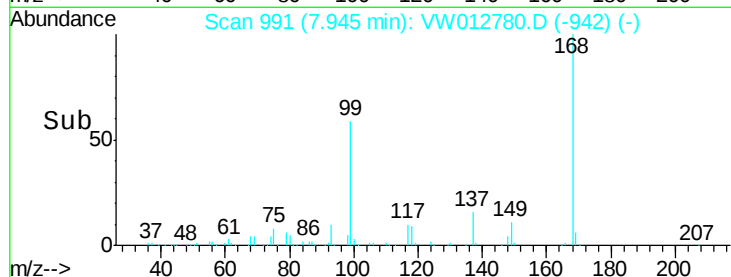

#29

Tetrahydrofuran

Concen: 8.702 ug/l

RT: 7.55 min Scan# 926

Delta R.T. 0.02 min

Lab File: VW012780.D

Acq: 08 Sep 2019 19:53


Tgt Ion: 42 Resp: 4356

Ion Ratio Lower Upper

42 100

72 36.5 28.4 42.6

71 34.7 27.1 40.7

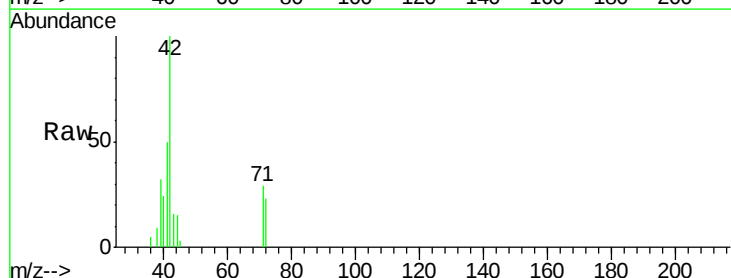

Abundance Ion 42.00 (41.70 to 42.70): VW

Ion 72.00 (71.70 to 72.70): VW

Ion 71.00 (70.70 to 71.70): VW

2000


1500


1000

500

0

Time-->




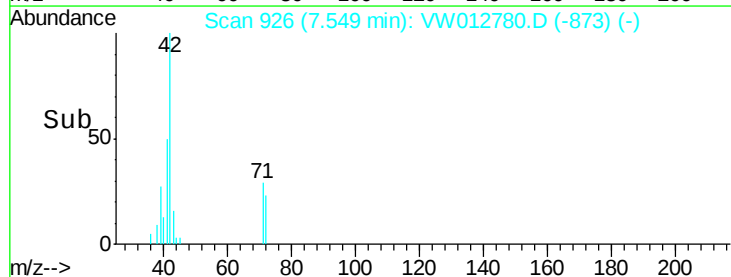


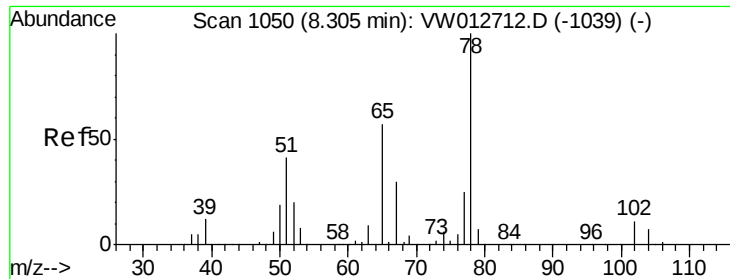

#33
 1,2-Dichloroethane-d4
 Concen: 52.666 ug/l
 RT: 8.30 min Scan# 1049
 Delta R.T. -0.01 min
 Lab File: VW012780.D
 Acq: 08 Sep 2019 19:53




Instrument :
 MSVOA_W
 ClientSampleId :
 PAR-12-F3-(3.11)

Tot Ion: 65 Resp: 119755
 Ion Ratio Lower Upper
 65 100
 67 49.7 0.0 101.8

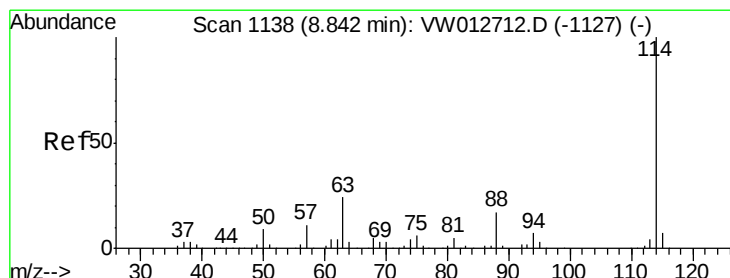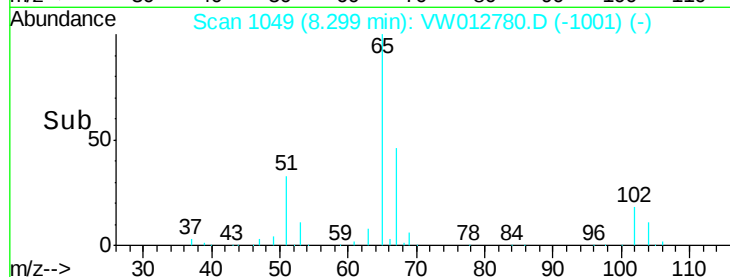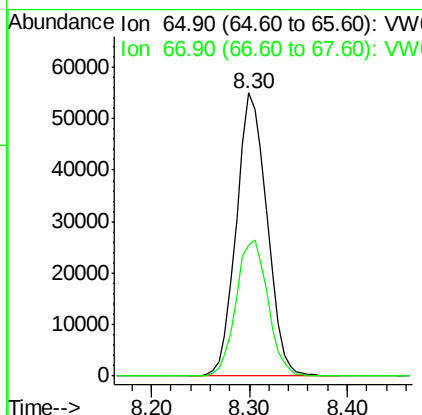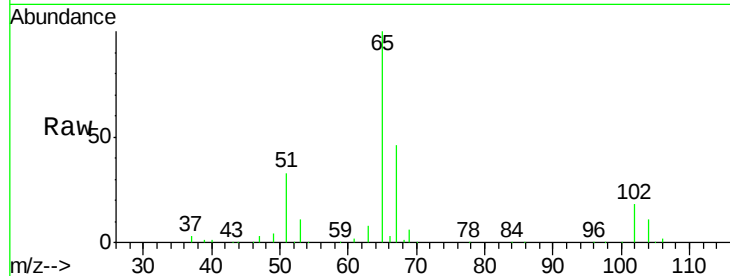

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW012780.D
 Acq: 08 Sep 2019 19:53

Tgt Ion: 114 Resp: 304805
 Ion Ratio Lower Upper
 114 100
 63 23.3 0.0 47.2
 88 15.8 0.0 34.0

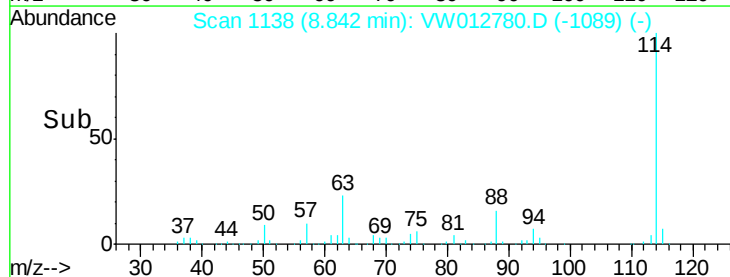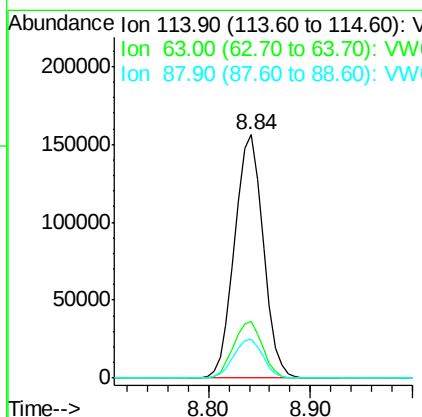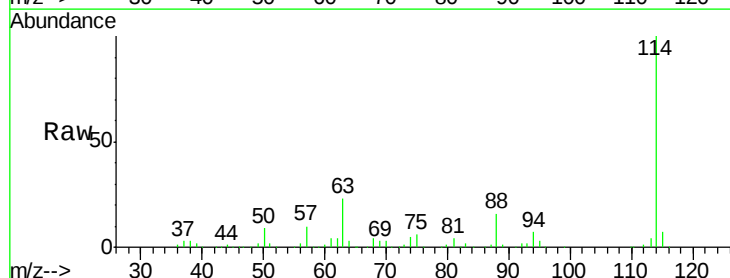



#35

Dibromofluoromethane

Concen: 50.411 ug/l

RT: 7.88 min Scan# 980

Delta R.T. -0.01 min

Lab File: VW012780.D

Acq: 08 Sep 2019 19:53

Instrument :

MSVOA_W

ClientSampleId :

PAR-12-F3-(3.11)


Tot Ion:113 Resp: 91352

Ion Ratio Lower Upper

113 100

111 102.7 80.2 120.4




192 22.5 17.3 25.9

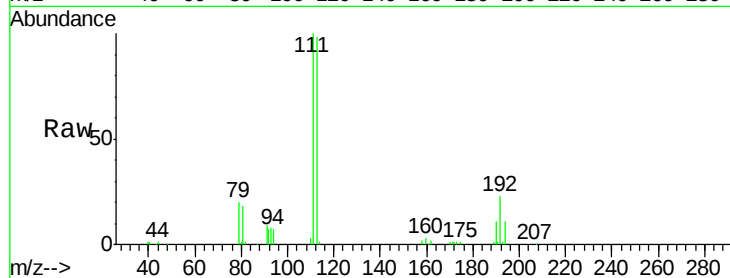

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

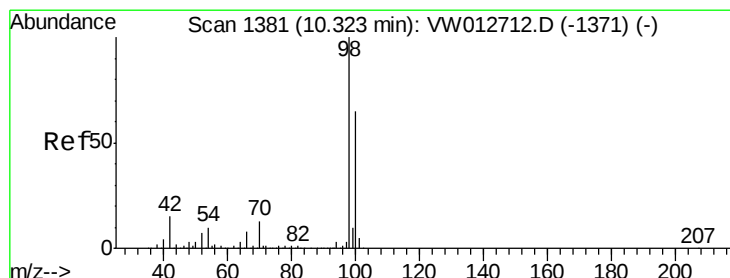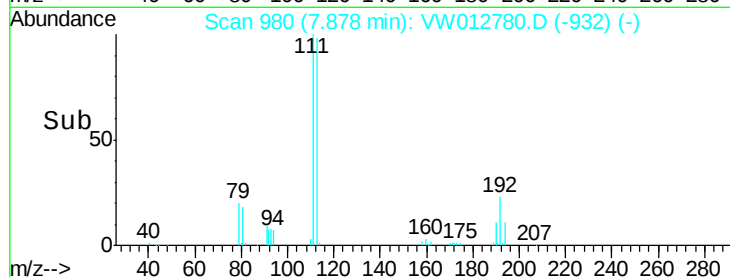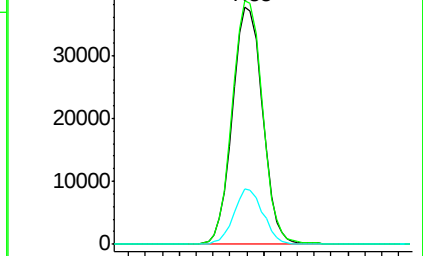

#50

Toluene-d8

Concen: 50.644 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW012780.D


Acq: 08 Sep 2019 19:53

Tgt Ion: 98 Resp: 359550

Ion Ratio Lower Upper



98 100


100 65.4 52.2 78.4

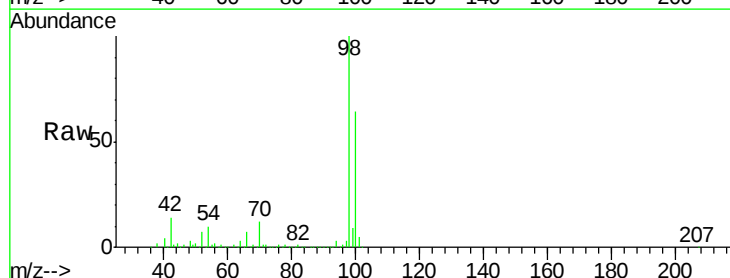

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

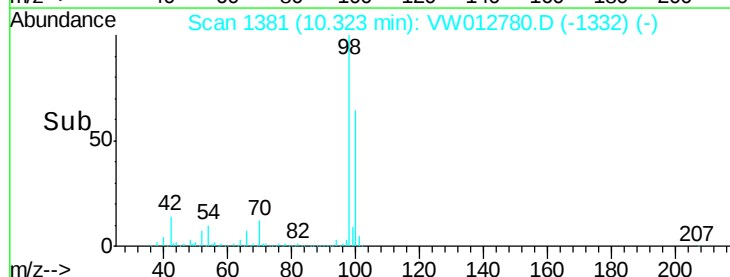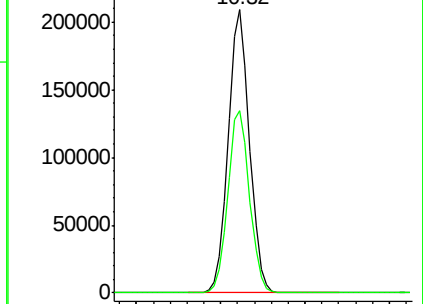

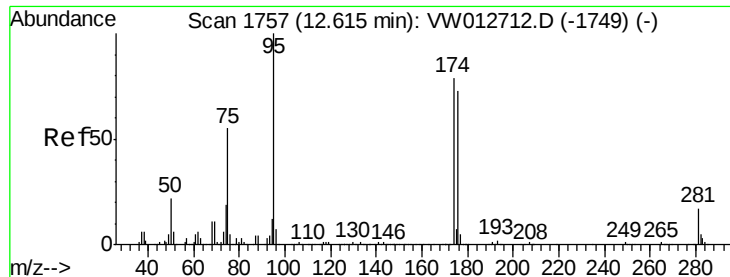

#62

4-Bromofluorobenzene

Concen: 42.350 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. 0.00 min

Lab File: VW012780.D

Acq: 08 Sep 2019 19:53

Instrument :

MSVOA_W

ClientSampleId :

PAR-12-F3-(3.11)


Tot Ion: 95 Resp: 109151

Ion Ratio Lower Upper

95 100

174 84.3 0.0 161.0




176 79.7 0.0 156.4

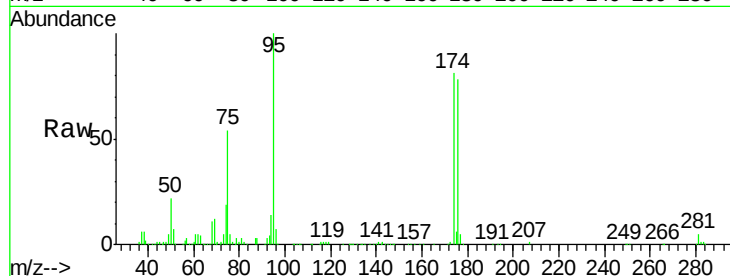

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

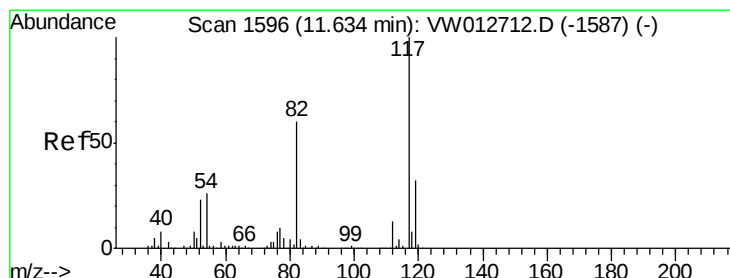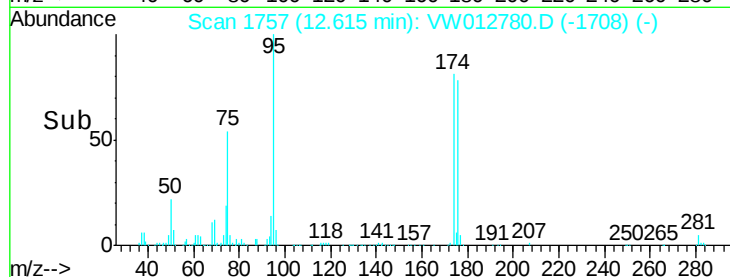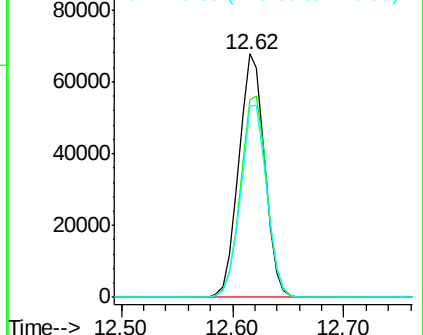

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1595

Delta R.T. -0.01 min

Lab File: VW012780.D

Acq: 08 Sep 2019 19:53


Tgt Ion: 117 Resp: 249742

Ion Ratio Lower Upper

117 100

82 59.0 48.2 72.4



119 31.4 25.8 38.6

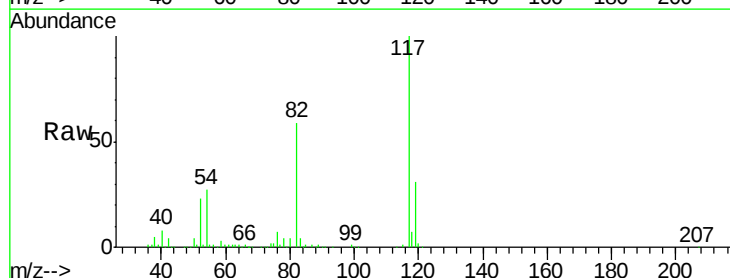


Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW

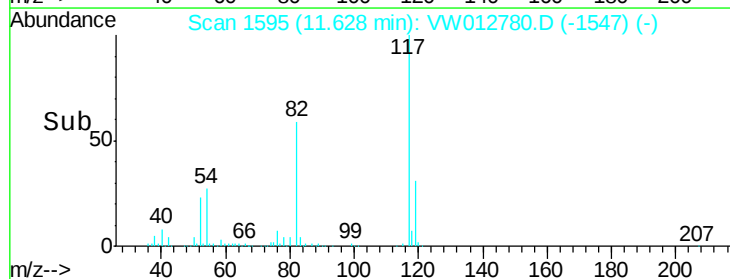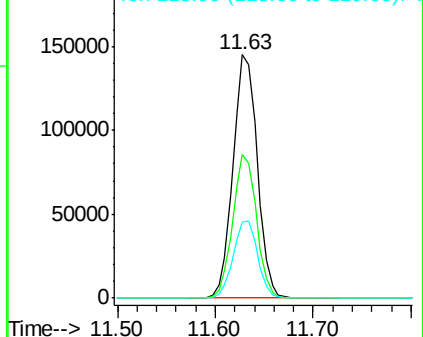

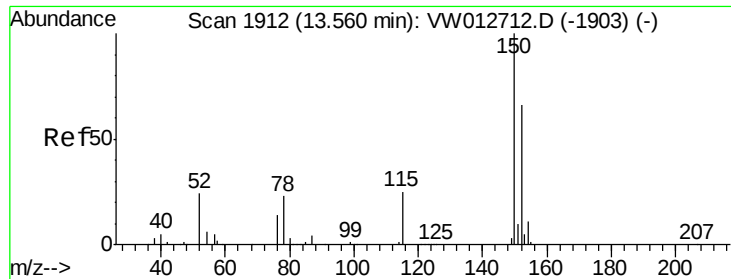

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.55 min Scan# 1911

Delta R.T. -0.01 min

Lab File: VW012780.D

Acq: 08 Sep 2019 19:53

Instrument :

MSVOA_W

ClientSampleId :

PAR-12-F3-(3.11)


Tot Ion:152 Resp: 96035

Ion Ratio Lower Upper

152 100

115 59.0 30.0 90.1

150 160.2 0.0 349.0

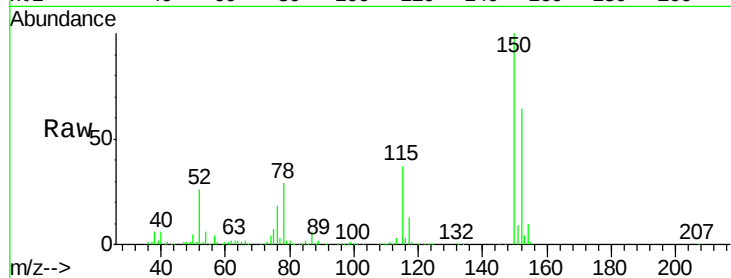

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

