
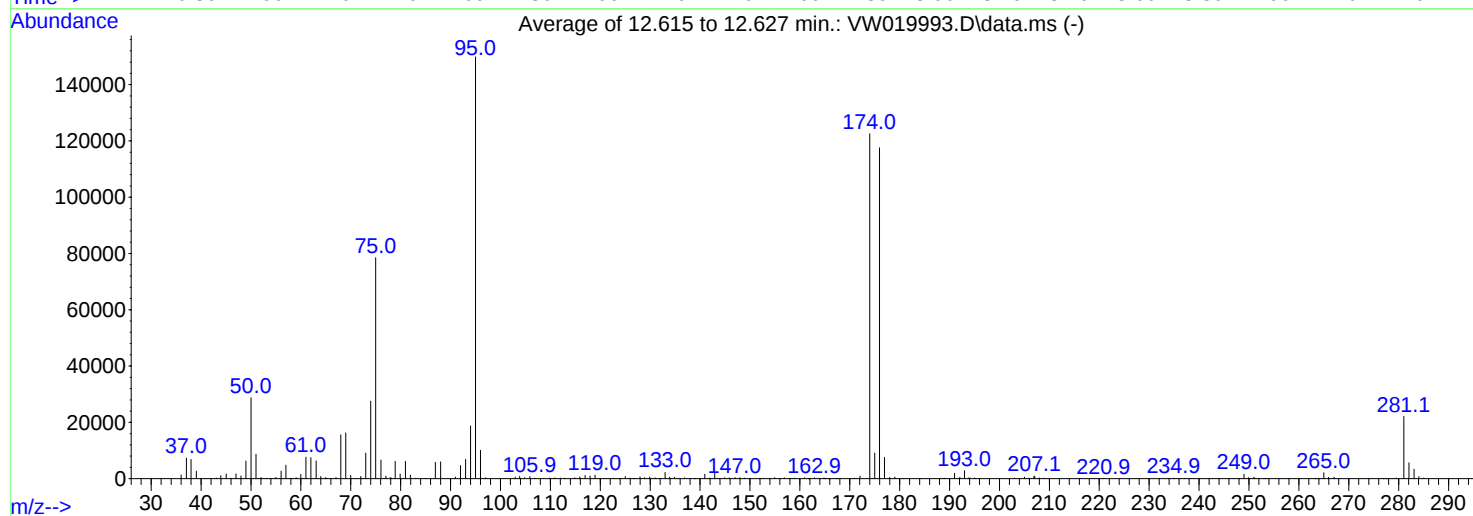


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090821\
 Data File : VW019993.D
 Acq On : 08 Sep 2021 08:38
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W090721S.M
 Title : SW846 8260
 Last Update : Wed Sep 08 12:18:21 2021

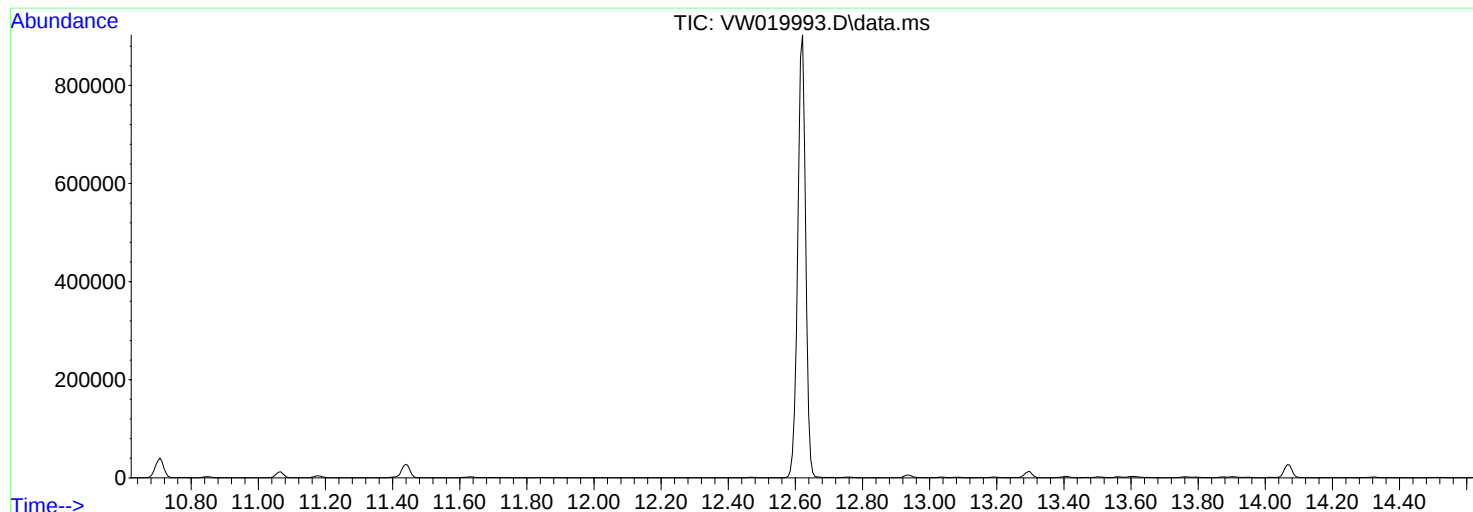

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	28771	PASS
75	95	30	60	52.4	78528	PASS
95	95	100	100	100.0	149867	PASS
96	95	5	9	6.7	10043	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.8	122584	PASS
175	174	5	9	7.4	9084	PASS
176	174	95	101	95.9	117571	PASS
177	176	5	9	6.4	7553	PASS