

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW090919\
 Data File : VW012847.D
 Acq On : 10 Sep 2019 03:13
 Operator : SY/VA
 Sample : K4644-06
 Misc : 6.40G/5ML/MSVOA W/SOIL
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 T11-D3-(4)

Quant Time: Sep 10 08:06:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090719S.M
 Quant Title : SW846 8260
 QLast Update : Sun Sep 08 05:04:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	263823	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	396328	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	305199	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.55	152	90914	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	140588	47.69	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.38%	
35) Dibromofluoromethane	7.88	113	115218	48.90	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.80%	
50) Toluene-d8	10.32	98	461343	49.98	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.96%	
62) 4-Bromofluorobenzene	12.62	95	121146	36.15	ug/l	0.00
Spiked Amount 50.000			Recovery	=	72.30%	
Target Compounds						
29) Tetrahydrofuran	7.54	42	5386	8.299	ug/l	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW090919\
Data File : VW012847.D
Acq On : 10 Sep 2019 03:13
Operator : SY/VA
Sample : K4644-06
Misc : 6.40G/5ML/MSVOA W/SOIL
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
T11-D3-(4)

Quant Time: Sep 10 08:06:24 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W090719S.M
Quant Title : SW846 8260
QLast Update : Sun Sep 08 05:04:40 2019
Response via : Initial Calibration

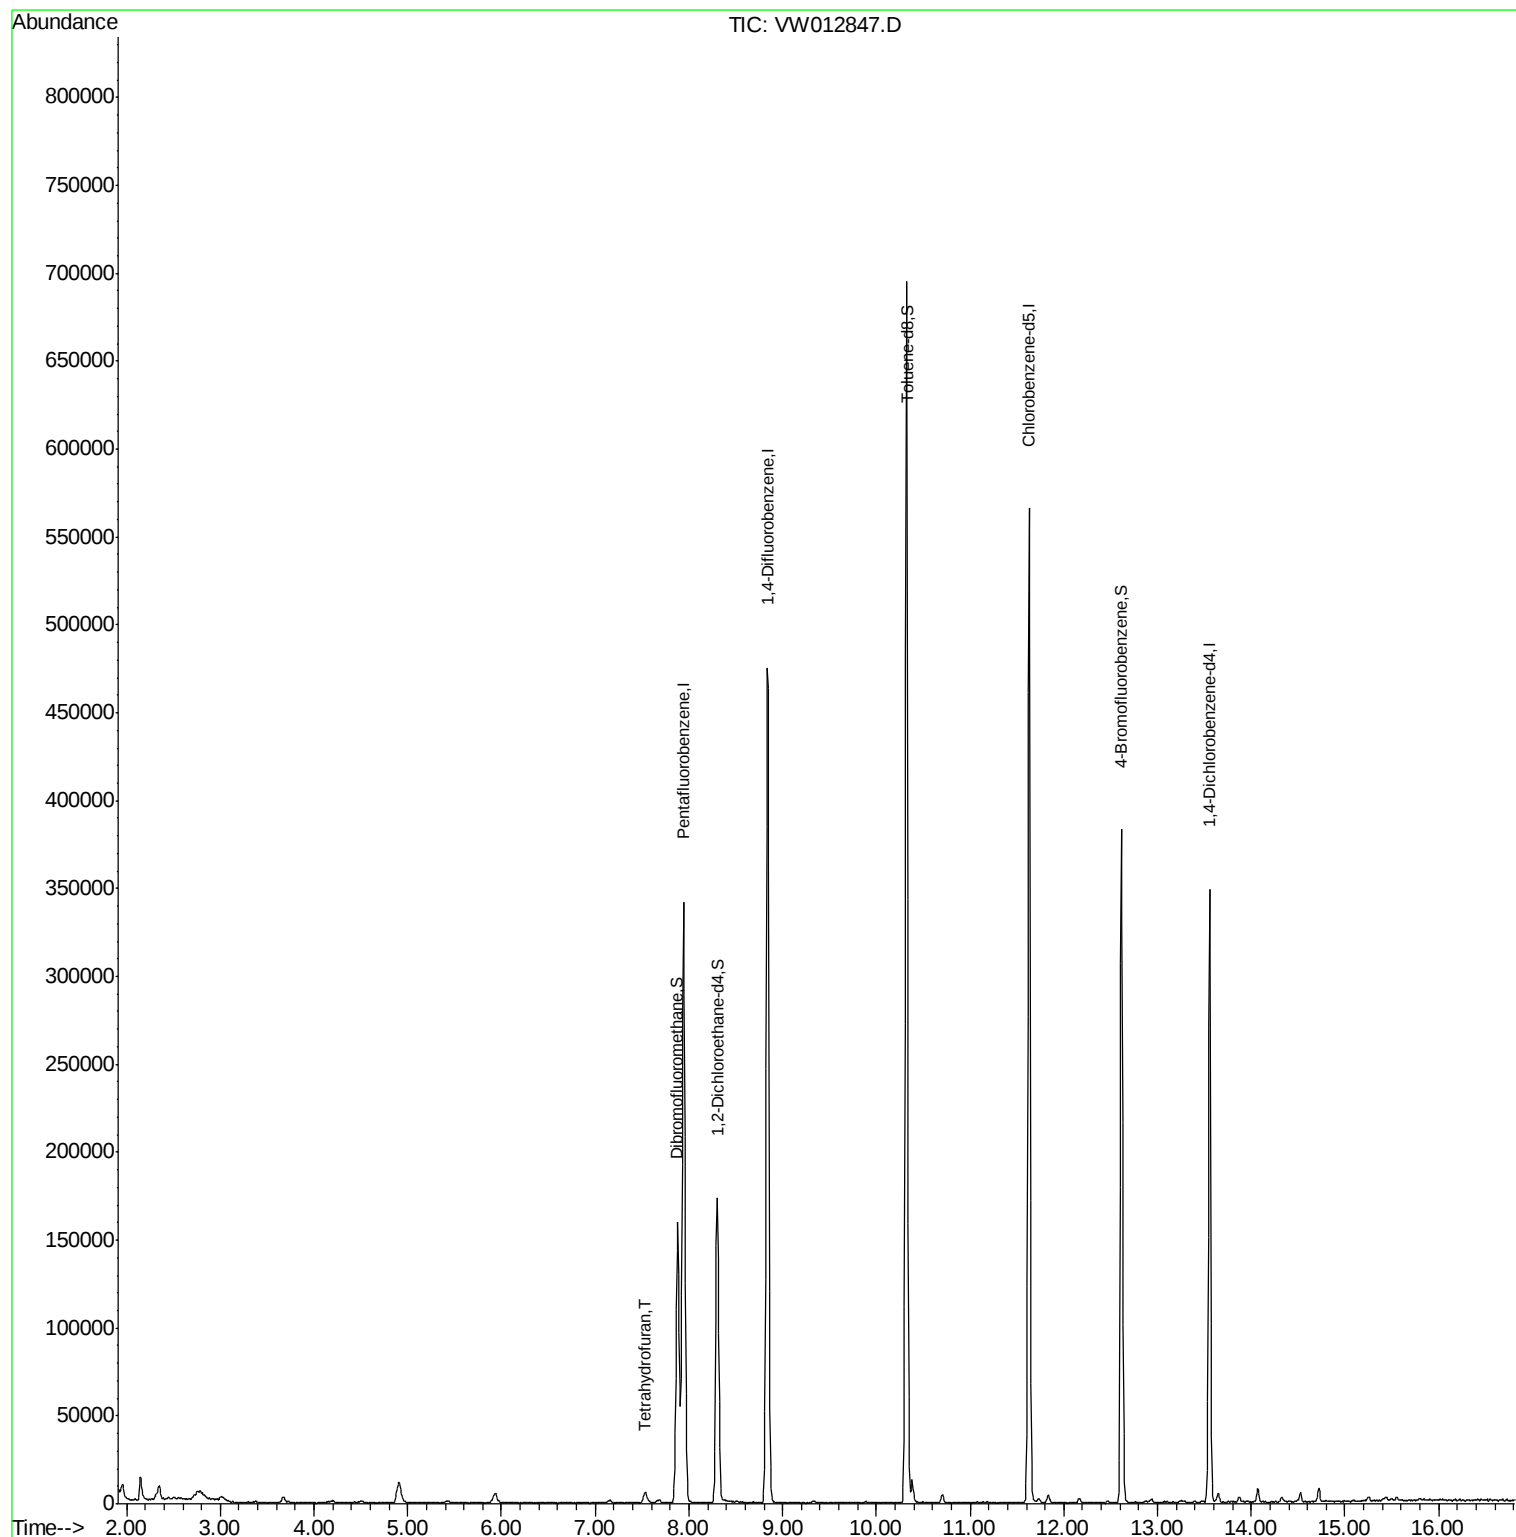

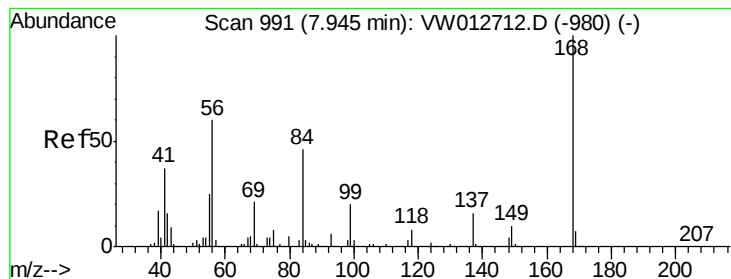

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW012847.D

Acq: 10 Sep 2019 03:13

Instrument :

MSVOA_W

ClientSampleId :


T11-D3-(4)

Tot Ion:168 Resp: 263823

Ion Ratio Lower Upper

168 100

99 56.1 47.8 71.6

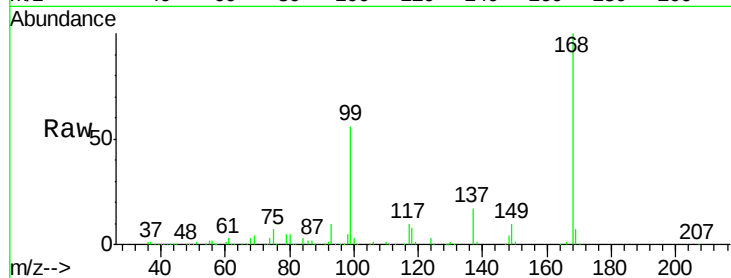

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW



7.95

100000

50000

0

Time-->

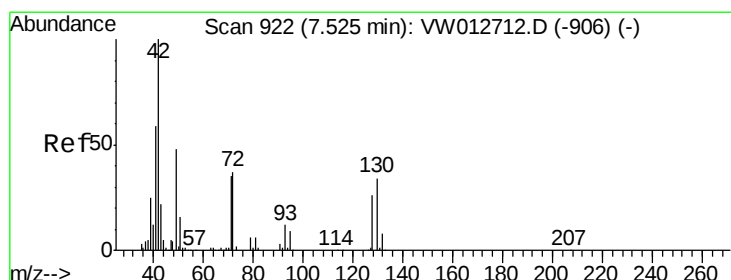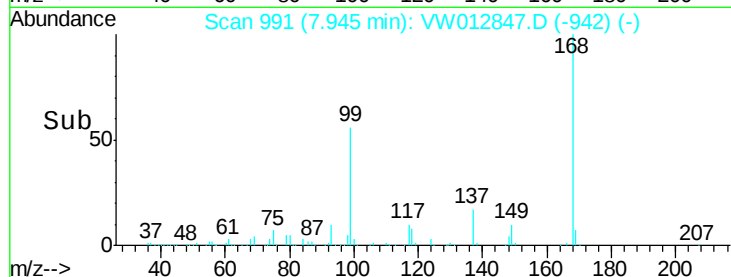

#29

Tetrahydrofuran

Concen: 8.299 ug/l

RT: 7.54 min Scan# 924

Delta R.T. 0.01 min

Lab File: VW012847.D

Acq: 10 Sep 2019 03:13


Tgt Ion: 42 Resp: 5386

Ion Ratio Lower Upper

42 100

72 38.8 28.4 42.6

71 37.3 27.1 40.7

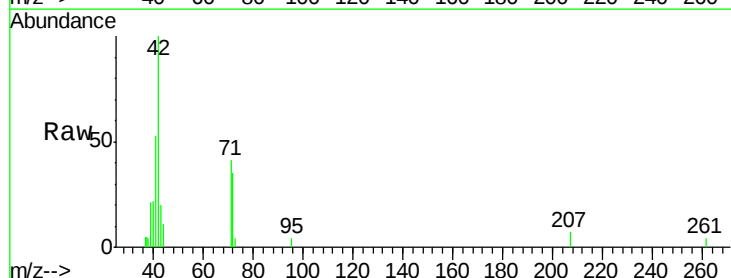

Abundance Ion 42.00 (41.70 to 42.70): VW

Ion 72.00 (71.70 to 72.70): VW

Ion 71.00 (70.70 to 71.70): VW

2500

2000


1500


1000

500

0

Time-->




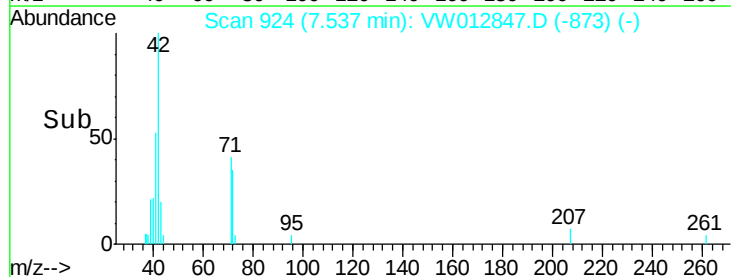


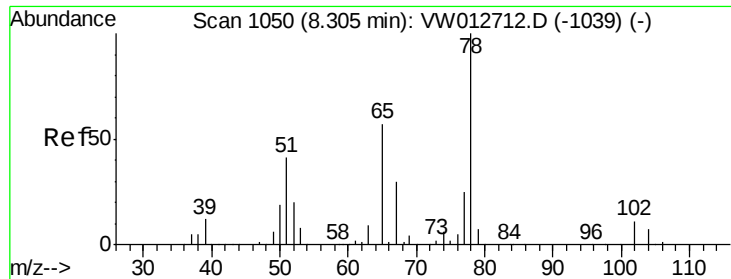

#33
 1,2-Dichloroethane-d4
 Concen: 47.693 ug/l
 RT: 8.30 min Scan# 1049
 Delta R.T. -0.01 min
 Lab File: VW012847.D
 Acq: 10 Sep 2019 03:13




Instrument :
 MSVOA_W
 ClientSampleId :
 T11-D3-(4)


Tot Ion: 65 Resp: 140588
 Ion Ratio Lower Upper
 65 100
 67 51.2 0.0 101.8

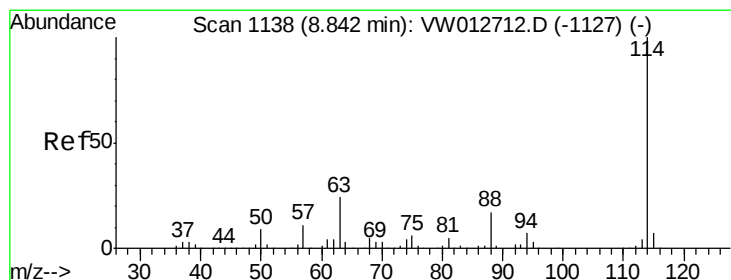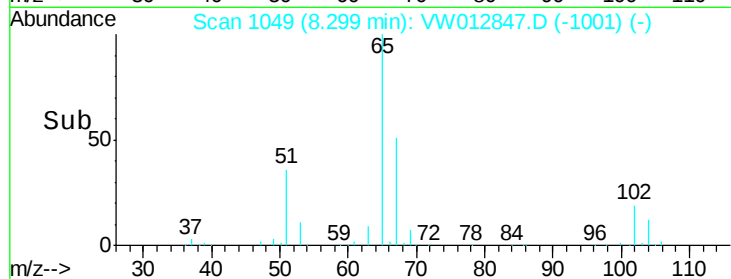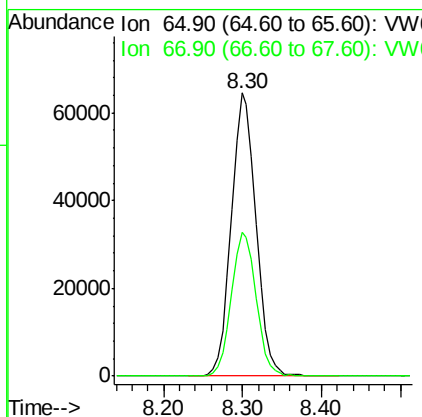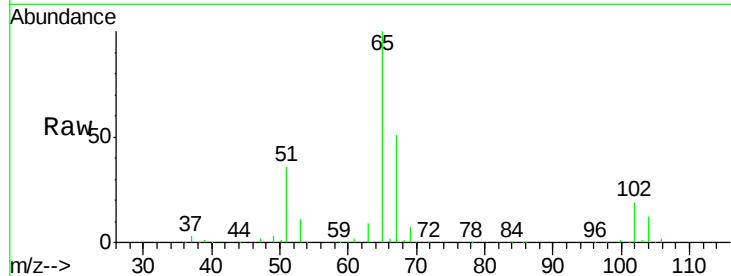

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW012847.D
 Acq: 10 Sep 2019 03:13

Tgt Ion: 114 Resp: 396328
 Ion Ratio Lower Upper
 114 100
 63 21.0 0.0 47.2
 88 16.0 0.0 34.0

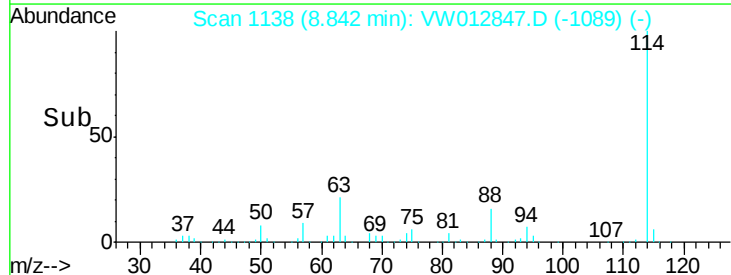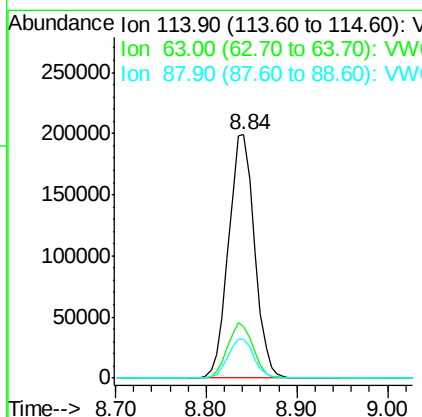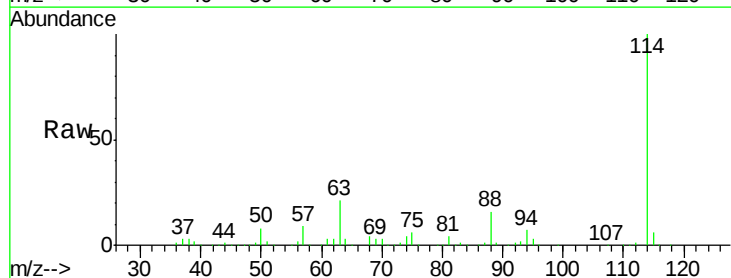

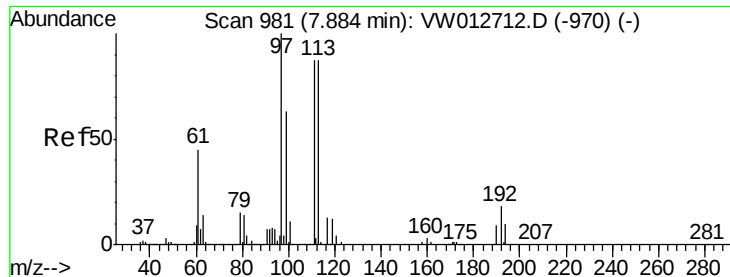

#35

Dibromofluoromethane

Concen: 48.898 ug/l

RT: 7.88 min Scan# 980

Delta R.T. -0.01 min

Lab File: VW012847.D

Acq: 10 Sep 2019 03:13

Instrument :

MSVOA_W

ClientSampleId :

T11-D3-(4)


Tot Ion:113 Resp: 115218

Ion Ratio Lower Upper

113 100

111 103.5 80.2 120.4




192 22.8 17.3 25.9

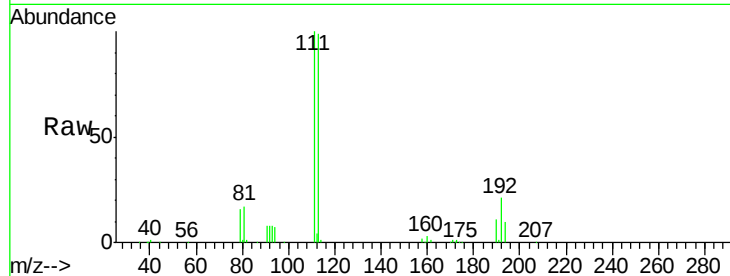

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

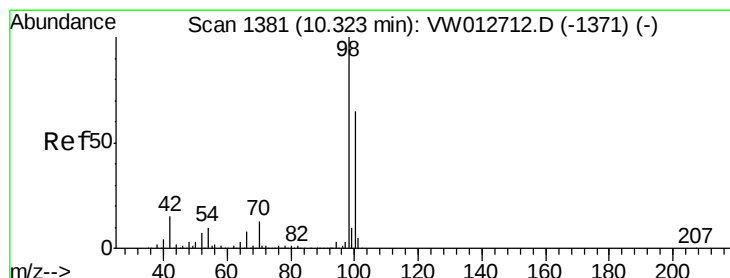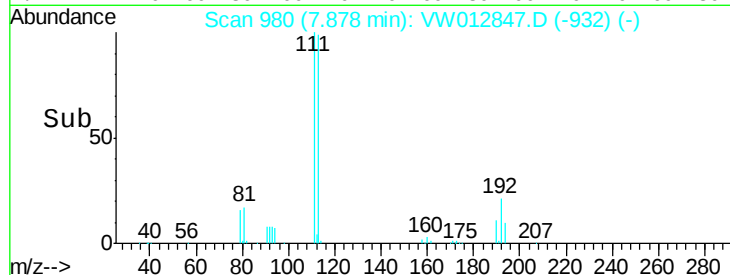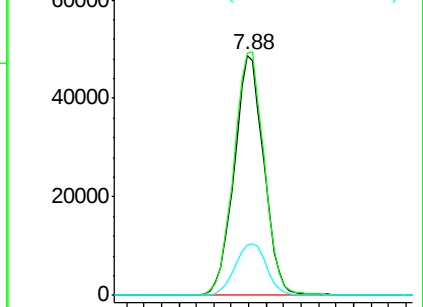

#50

Toluene-d8

Concen: 49.976 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW012847.D


Acq: 10 Sep 2019 03:13

Tgt Ion: 98 Resp: 461343

Ion Ratio Lower Upper



98 100


100 66.2 52.2 78.4

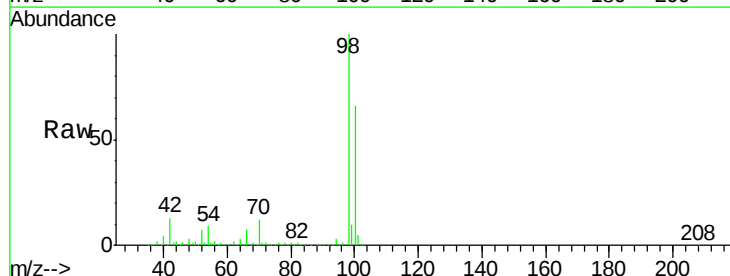

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW



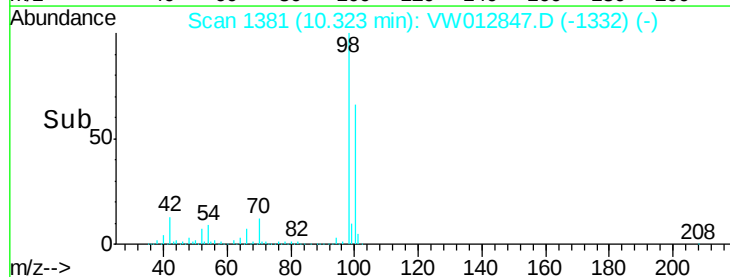
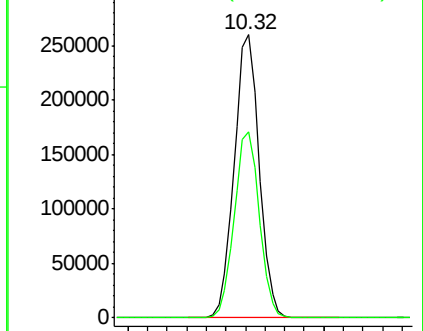


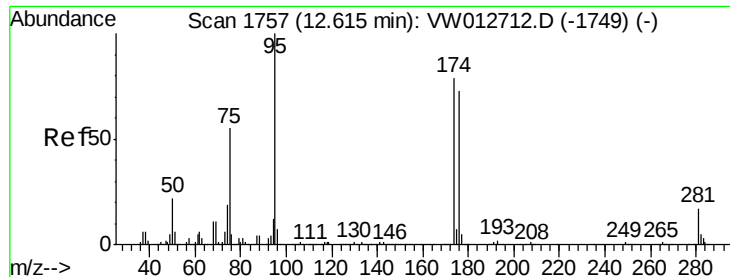

#62
4-Bromofluorobenzene
Concen: 36.149 ug/l
RT: 12.62 min Scan# 1757
Delta R.T. 0.00 min
Lab File: VW012847.D
Acq: 10 Sep 2019 03:13




Instrument :
MSVOA_W
ClientSampleId :
T11-D3-(4)




Tot Ion	95	174	176
Resp	121146	161.0	156.4
Ratio	100	84.3	80.9
Lower		0.0	0.0
Upper			

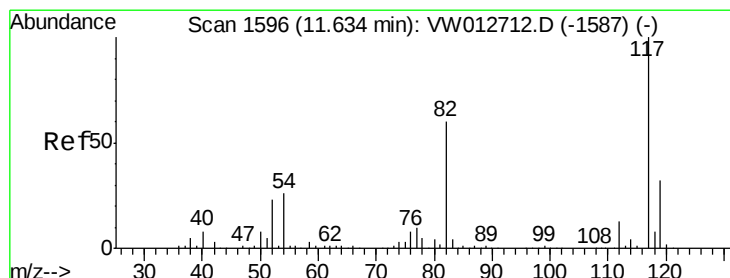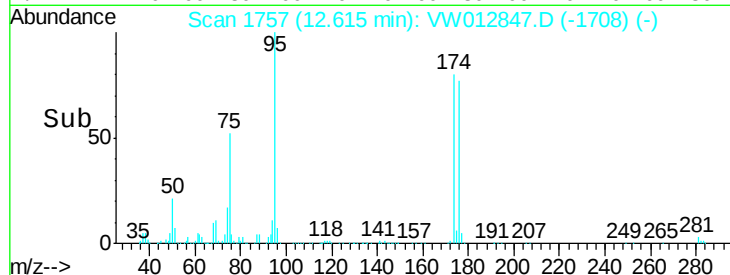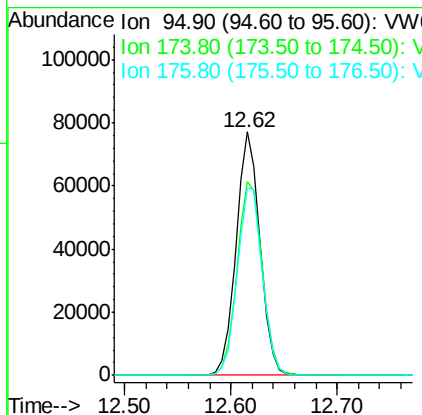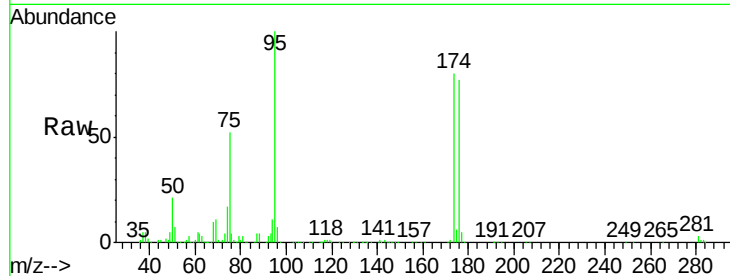

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1595
Delta R.T. -0.01 min
Lab File: VW012847.D
Acq: 10 Sep 2019 03:13

Tgt Ion	117	82	119
Resp	305199	72.4	38.6
Ratio	100	59.1	33.1
Lower		48.2	25.8
Upper			

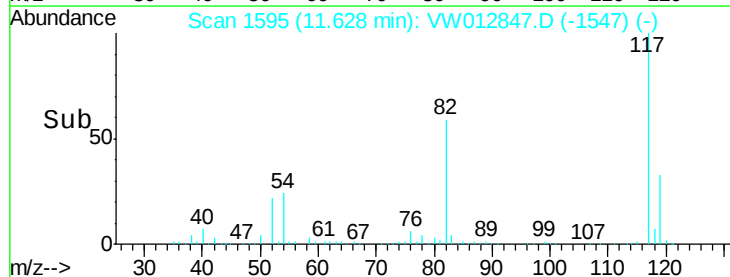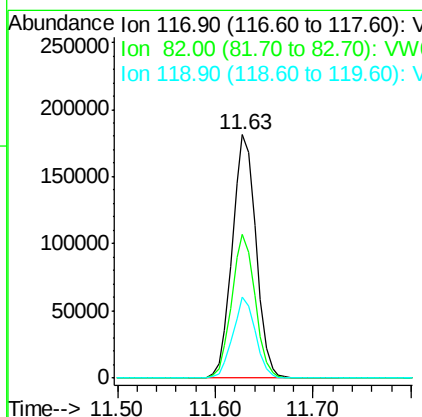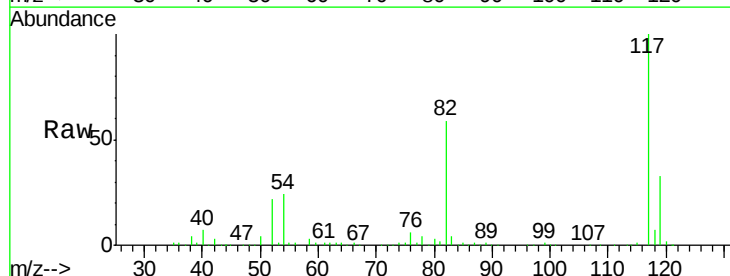

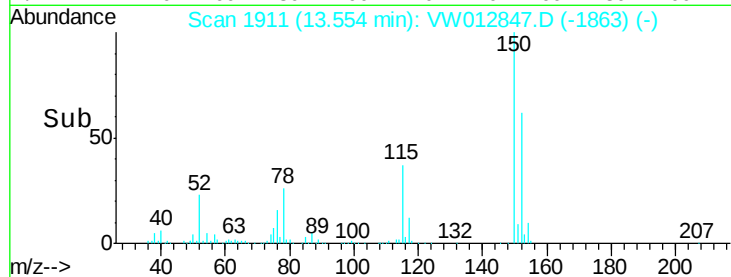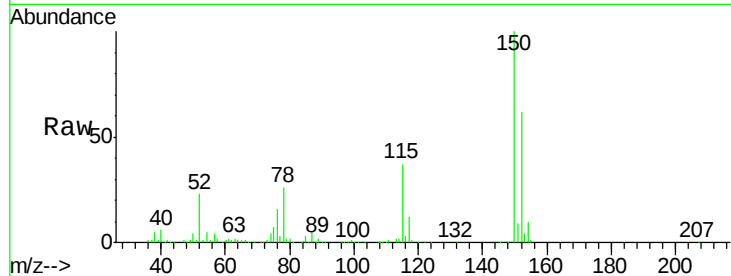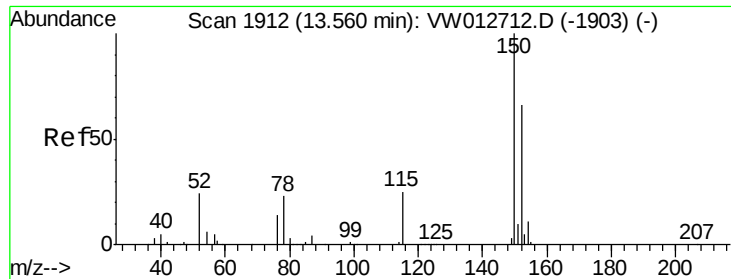

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.55 min Scan# 1911

Delta R.T. -0.01 min

Lab File: VW012847.D

Acq: 10 Sep 2019 03:13

Instrument :

MSVOA_W

ClientSampleId :

T11-D3-(4)

Tot Ion:152 Resp: 90914

Ion Ratio Lower Upper

152 100

115 58.3 30.0 90.1

150 158.0 0.0 349.0

