


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW090919\
Data File : VW012812.D
Acq On : 09 Sep 2019 10:16
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090719S.M
Title : SW846 8260
Last Update : Sun Sep 08 05:04:40 2019

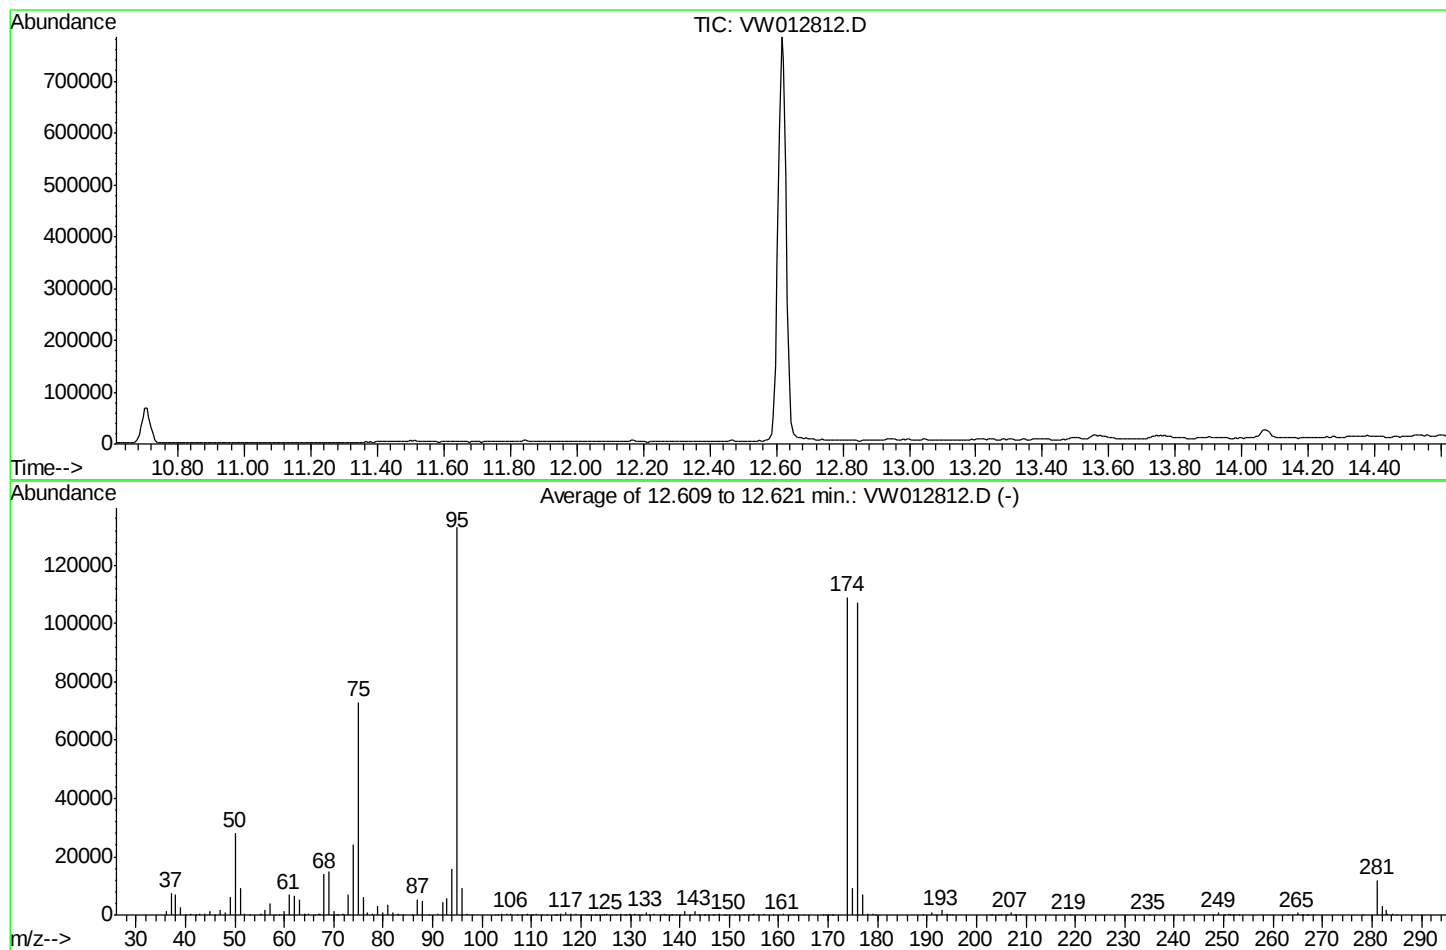

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	28216	PASS
75	95	30	60	54.9	73018	PASS
95	95	100	100	100.0	133067	PASS
96	95	5	9	7.0	9342	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.0	109120	PASS
175	174	5	9	8.6	9389	PASS
176	174	95	101	98.4	107341	PASS
177	176	5	9	6.7	7204	PASS