
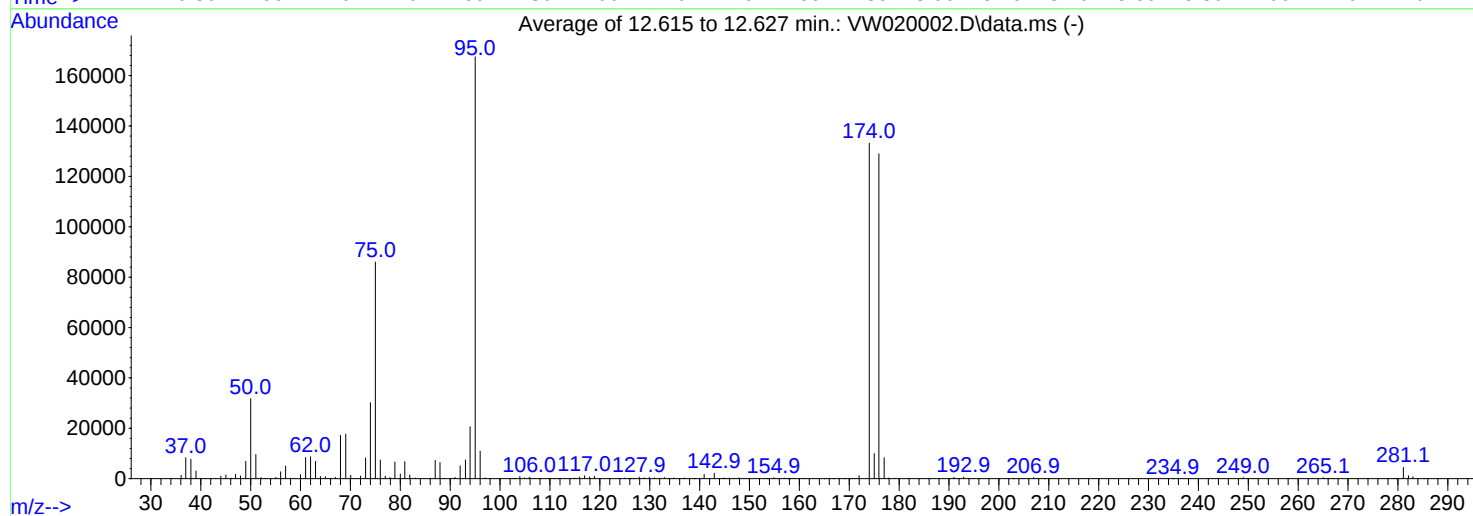


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW090921\
 Data File : VW020002.D
 Acq On : 09 Sep 2021 09:42
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W090721S.M
 Title : SW846 8260
 Last Update : Wed Sep 08 12:18:21 2021

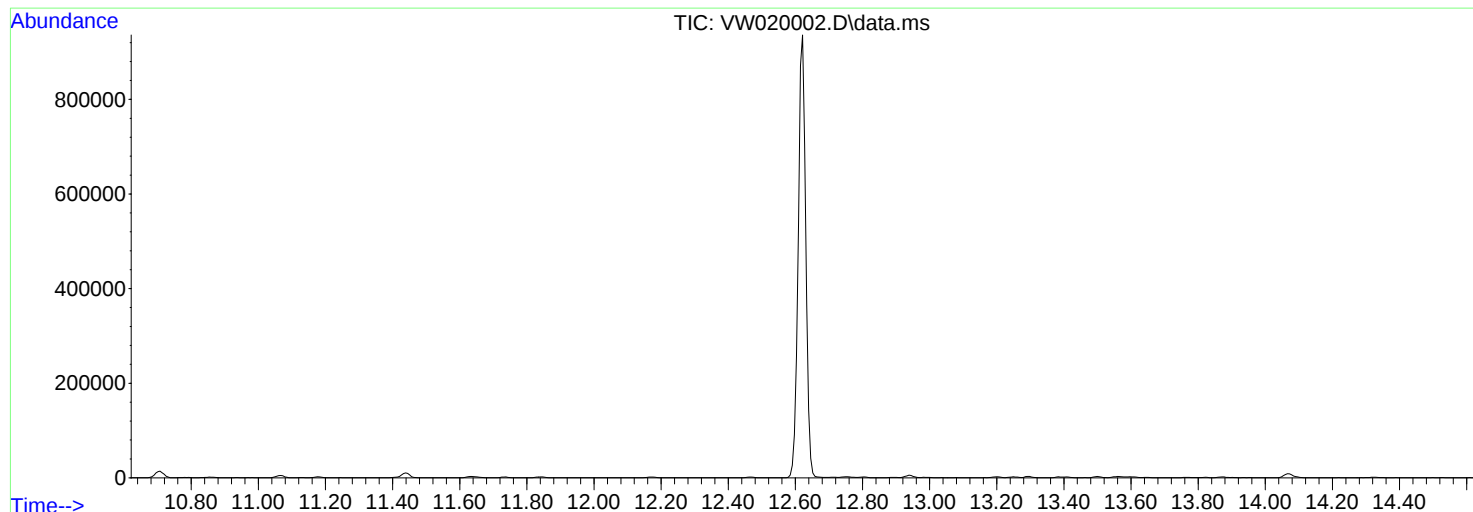

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	31736	PASS
75	95	30	60	51.4	86000	PASS
95	95	100	100	100.0	167467	PASS
96	95	5	9	6.5	10911	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.5	133205	PASS
175	174	5	9	7.5	9957	PASS
176	174	95	101	96.8	128960	PASS
177	176	5	9	6.4	8311	PASS