

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW091019\
 Data File : VW012878.D
 Acq On : 10 Sep 2019 18:33
 Operator : SY/VA
 Sample : K4692-13
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SB-26-7.5-8.0

Quant Time: Sep 11 08:38:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090719S.M
 Quant Title : SW846 8260
 QLast Update : Sun Sep 08 05:04:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	43586	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	62893	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	47221	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	12678	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	23279	47.80	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.60%	
35) Dibromofluoromethane	7.88	113	19241	51.46	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.92%	
50) Toluene-d8	10.32	98	70178	47.91	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.82%	
62) 4-Bromofluorobenzene	12.62	95	17435	32.78	ug/l	0.00
Spiked Amount 50.000			Recovery	=	65.56%	
Target Compounds						
20) Methylene Chloride	4.92	84	3418	8.229	ug/l	94
64) Tetrachloroethene	10.86	164	11272	39.340	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW091019\
Data File : VW012878.D
Acq On : 10 Sep 2019 18:33
Operator : SY/VA
Sample : K4692-13
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SB-26-7.5-8.0

Quant Time: Sep 11 08:38:12 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W090719S.M
Quant Title : SW846 8260
QLast Update : Sun Sep 08 05:04:40 2019
Response via : Initial Calibration

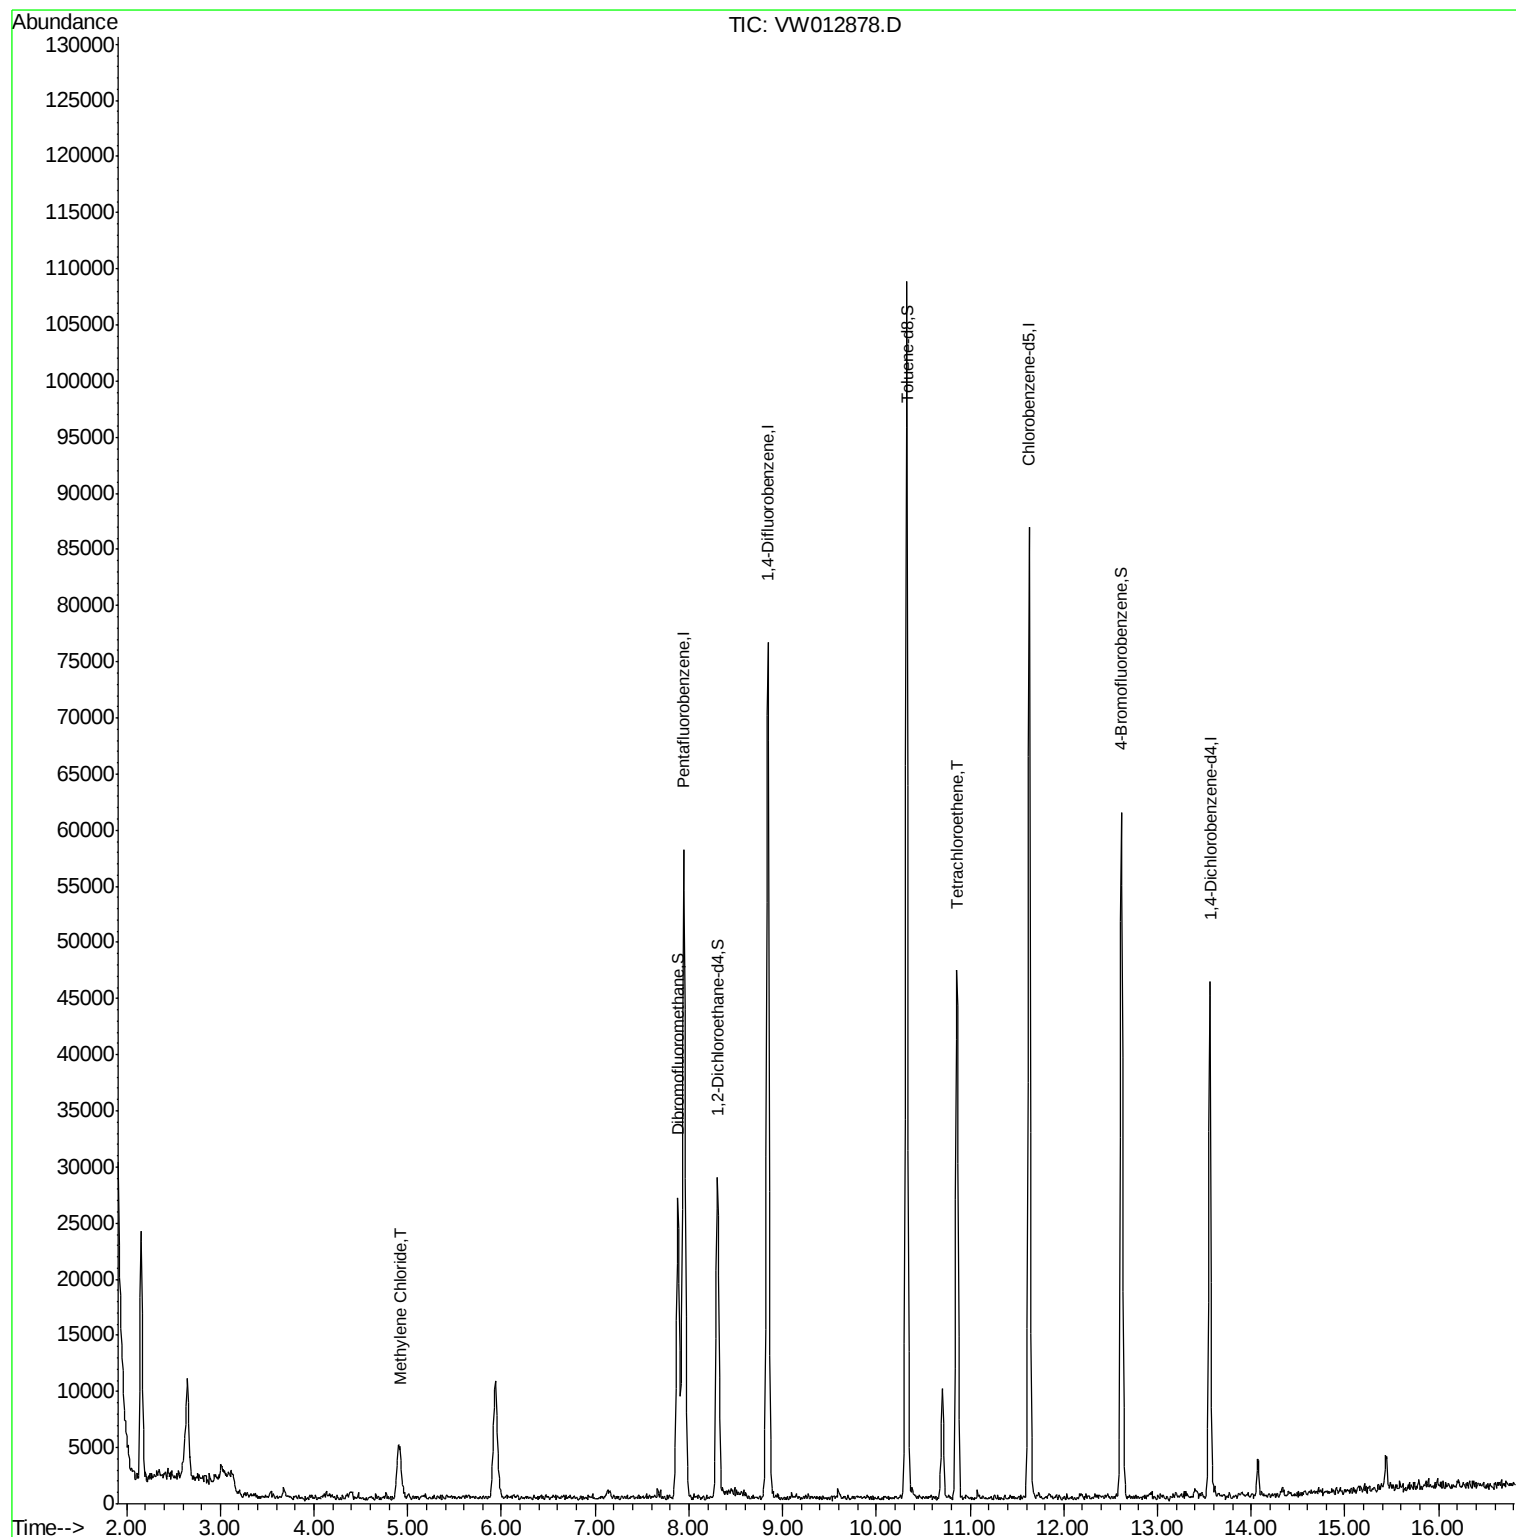

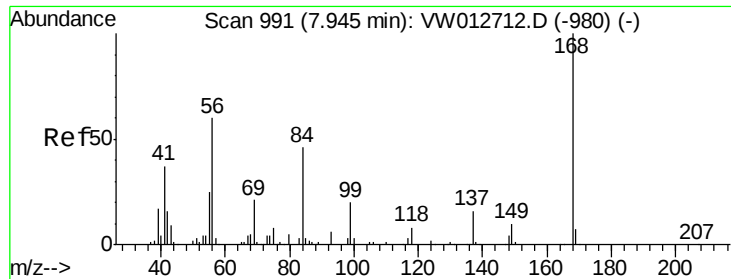

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW012878.D

Acq: 10 Sep 2019 18:33

Instrument :

MSVOA_W

ClientSampleId :


SB-26-7.5-8.0

Tot Ion:168 Resp: 43586

Ion Ratio Lower Upper




168 100

99 57.3 47.8 71.6

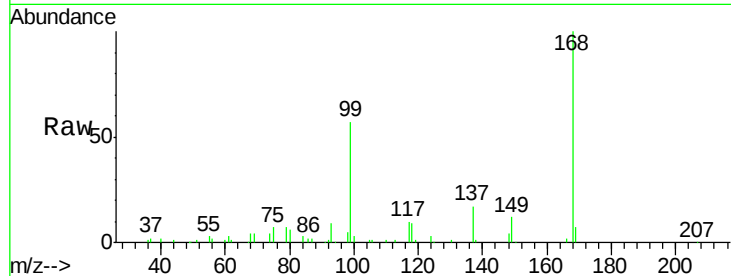

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

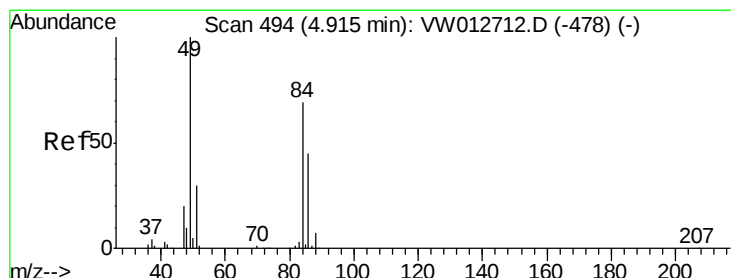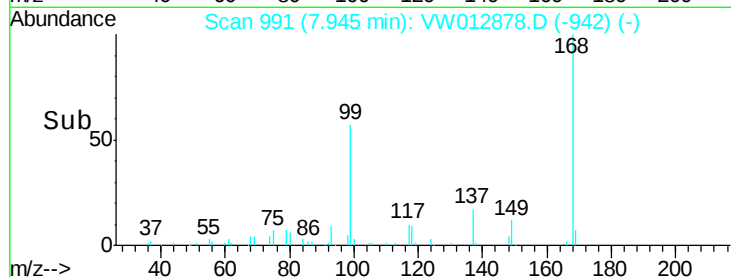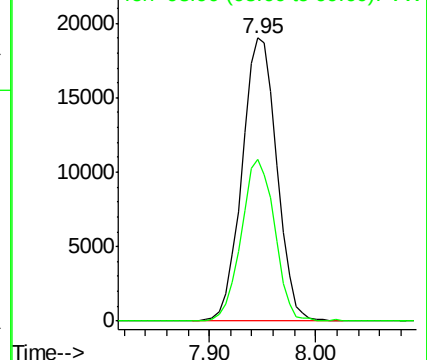

#20

Methylene Chloride

Concen: 8.229 ug/l

RT: 4.92 min Scan# 494

Delta R.T. 0.00 min

Lab File: VW012878.D

Acq: 10 Sep 2019 18:33

Tgt Ion: 84 Resp: 3418


Ion Ratio Lower Upper

84 100

49 140.6 115.4 173.0

51 38.3 34.9 52.3

86 75.1 52.2 78.4


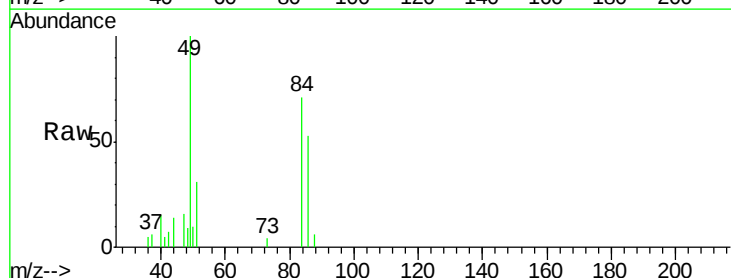



Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW



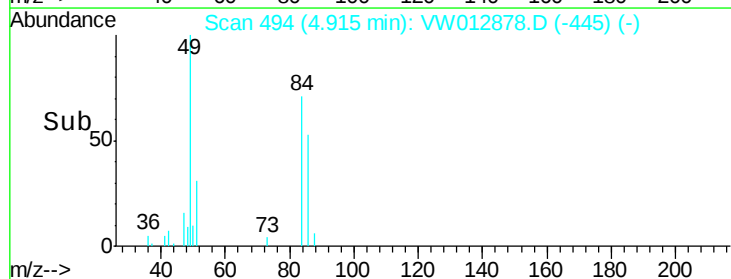
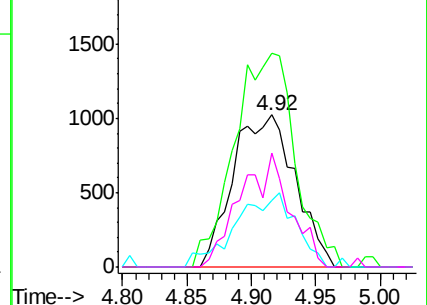


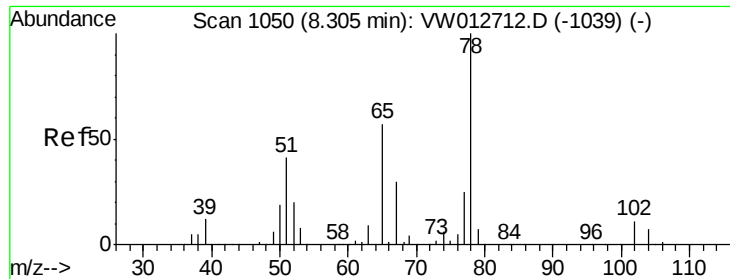

#33
 1,2-Dichloroethane-d4
 Concen: 47.801 ug/l
 RT: 8.31 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: VW012878.D
 Acq: 10 Sep 2019 18:33




Instrument :
 MSVOA_W
 ClientSampleId :
 SB-26-7.5-8.0


Tot Ion: 65 Resp: 23279
 Ion Ratio Lower Upper
 65 100
 67 51.1 0.0 101.8

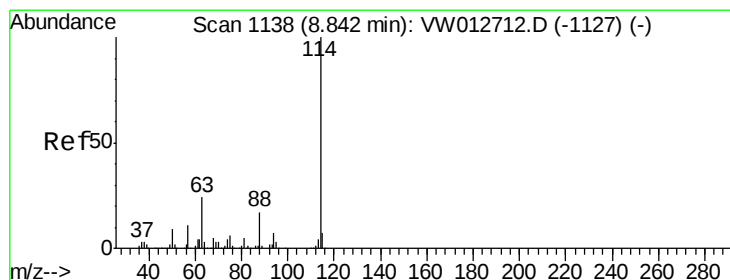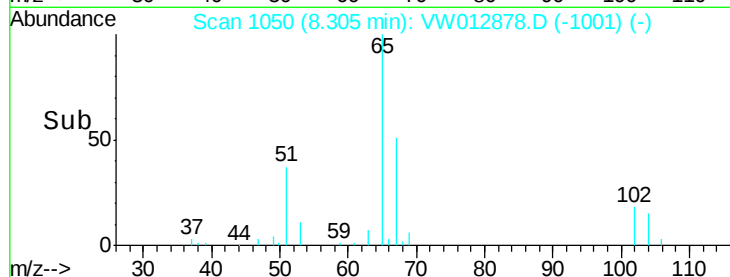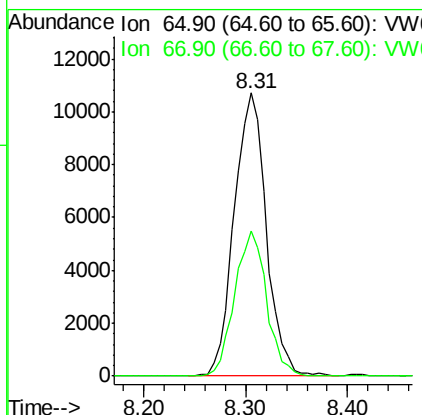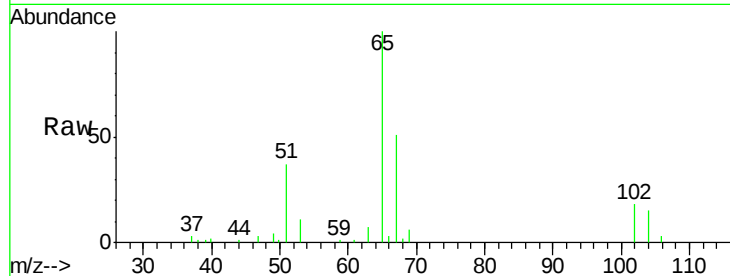

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW012878.D
 Acq: 10 Sep 2019 18:33

Tgt Ion: 114 Resp: 62893
 Ion Ratio Lower Upper
 114 100
 63 21.6 0.0 47.2
 88 16.5 0.0 34.0

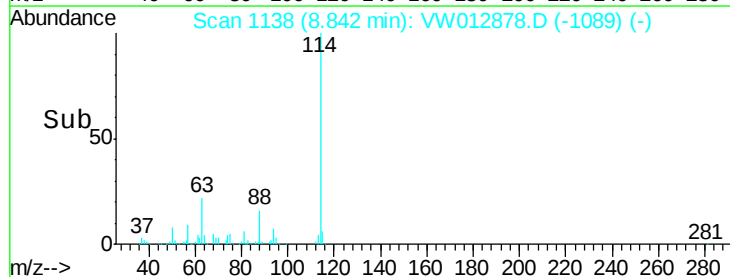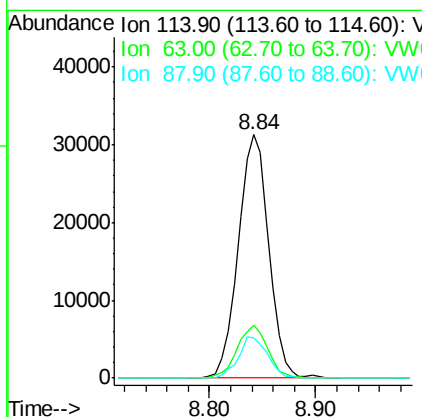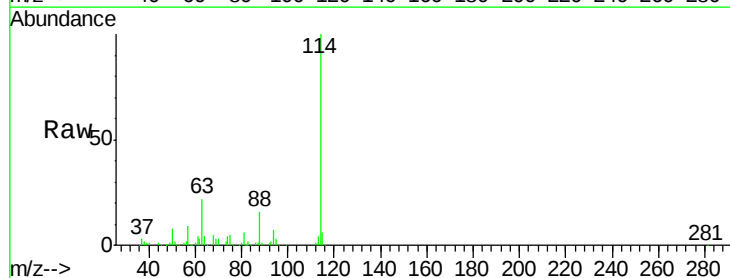

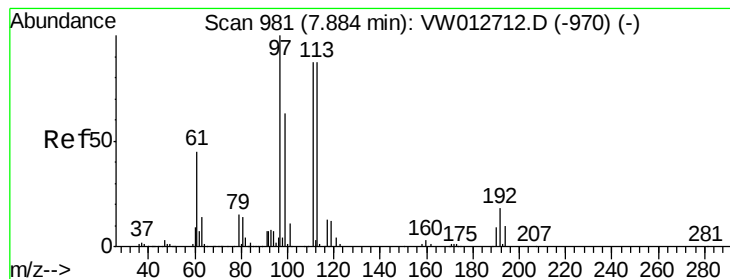

#35

Dibromofluoromethane

Concen: 51.458 ug/l

RT: 7.88 min Scan# 981

Delta R.T. 0.00 min

Lab File: VW012878.D

Acq: 10 Sep 2019 18:33

Instrument :

MSVOA_W

ClientSampleId :

SB-26-7.5-8.0


Tot Ion:113 Resp: 19241

Ion Ratio Lower Upper

113 100

111 101.7 80.2 120.4




192 22.4 17.3 25.9

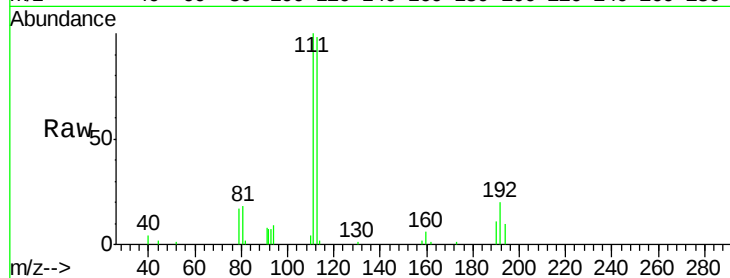

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

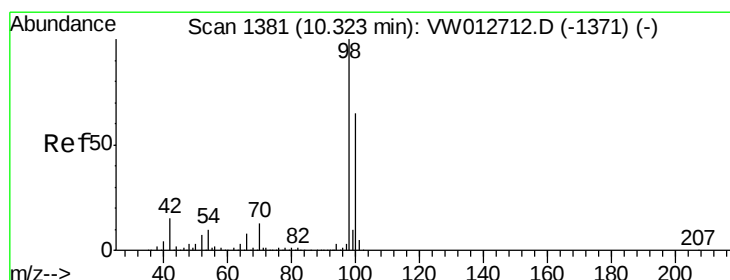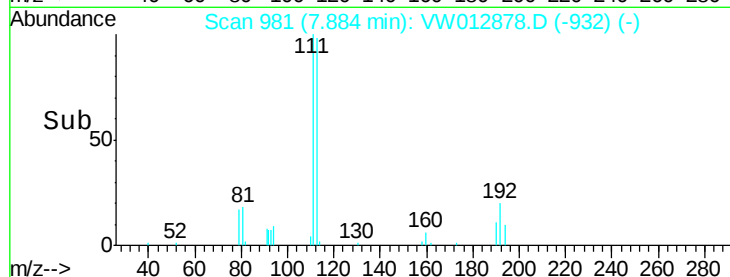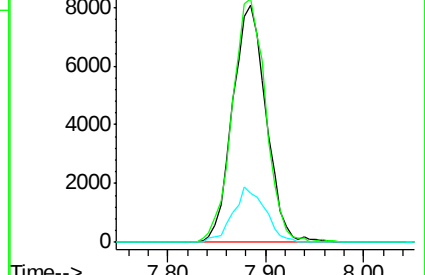

#50

Toluene-d8

Concen: 47.906 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW012878.D


Acq: 10 Sep 2019 18:33

Tgt Ion: 98 Resp: 70178

Ion Ratio Lower Upper



98 100


100 65.0 52.2 78.4

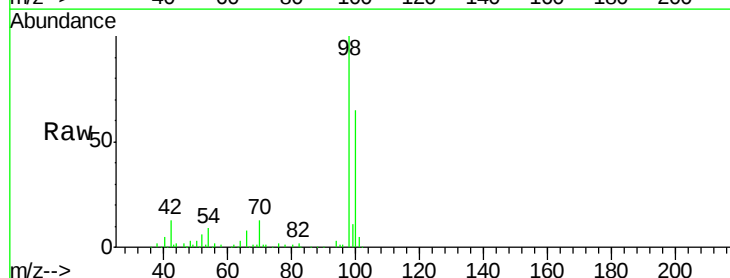

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW



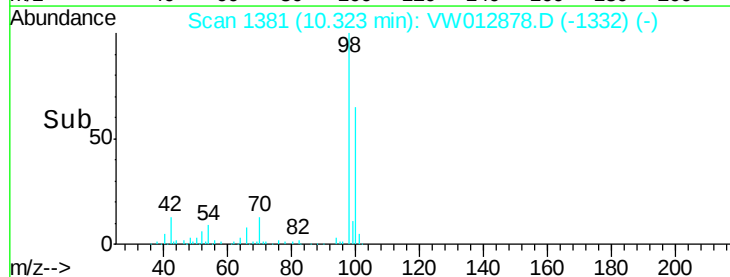
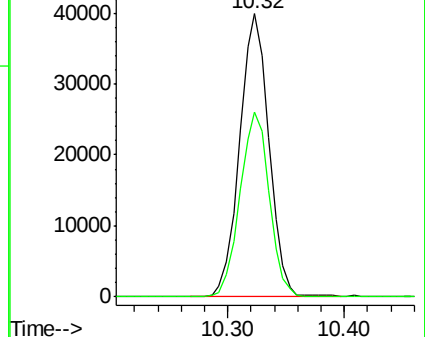


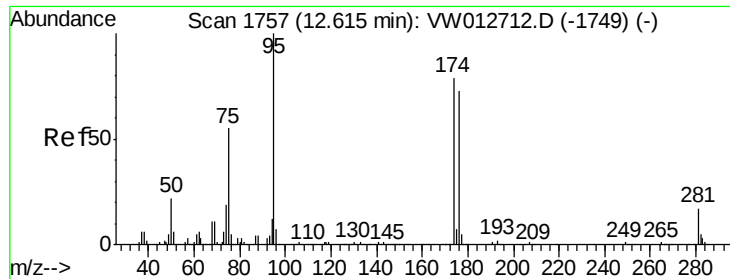

#62
4-Bromofluorobenzene
Concen: 32.784 ug/l
RT: 12.62 min Scan# 1757
Delta R.T. 0.00 min
Lab File: VW012878.D
Acq: 10 Sep 2019 18:33




Instrument :
MSVOA_W
ClientSampleId :
SB-26-7.5-8.0


Tot Ion: 95 Resp: 17435
Ion Ratio Lower Upper
95 100
174 89.2 0.0 161.0
176 82.1 0.0 156.4

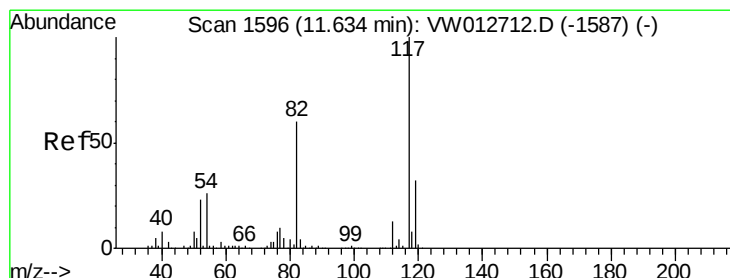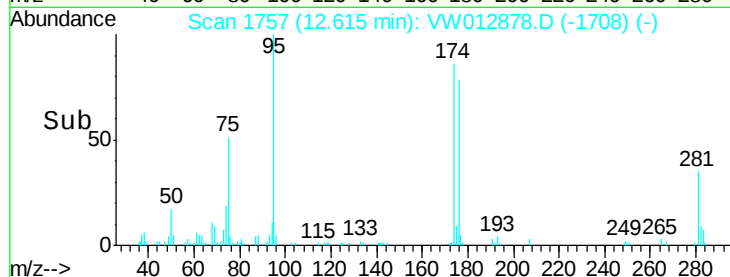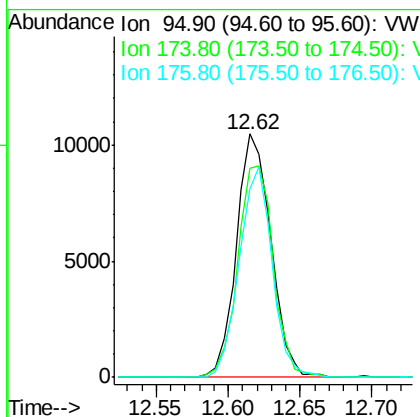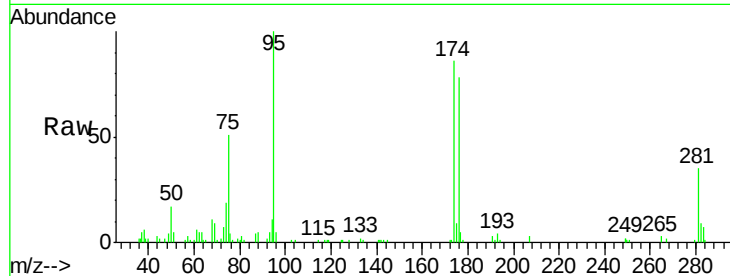

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW012878.D
Acq: 10 Sep 2019 18:33

Tgt Ion: 117 Resp: 47221
Ion Ratio Lower Upper
117 100
82 56.2 48.2 72.4
119 33.9 25.8 38.6

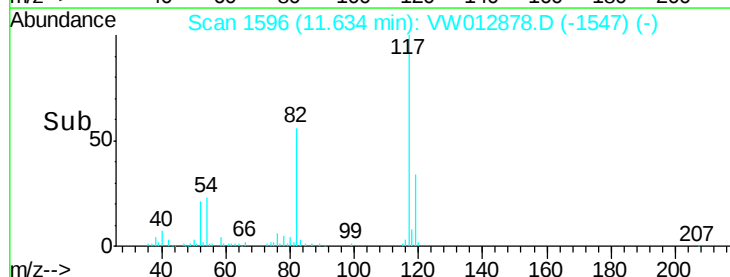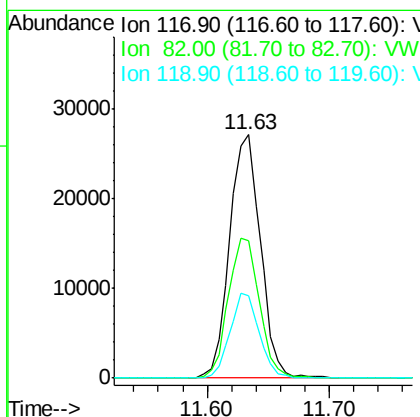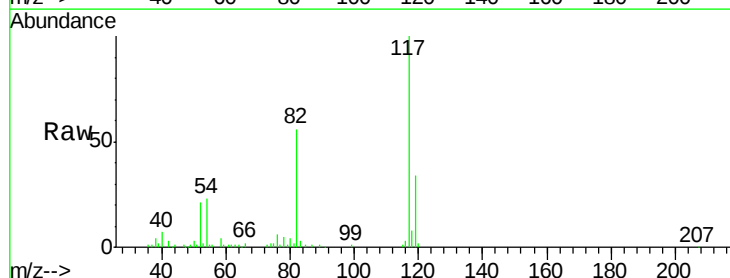

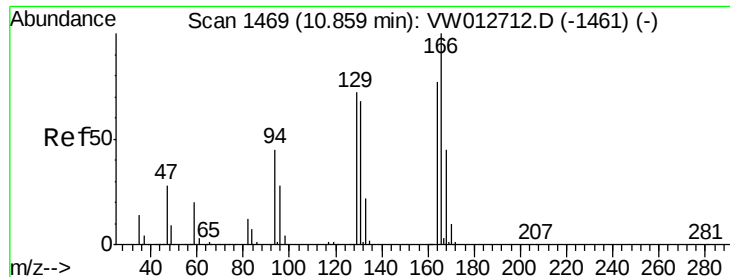

#64

Tetrachloroethene

Concen: 39.340 ug/l

RT: 10.86 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VW012878.D

Acq: 10 Sep 2019 18:33

Instrument :

MSVOA_W

ClientSampleId :

SB-26-7.5-8.0

Tot Ion:164 Resp: 11272


Ion Ratio Lower Upper

164 100

166 124.1 103.6 155.4

129 86.0 74.6 112.0

131 87.4 70.6 106.0



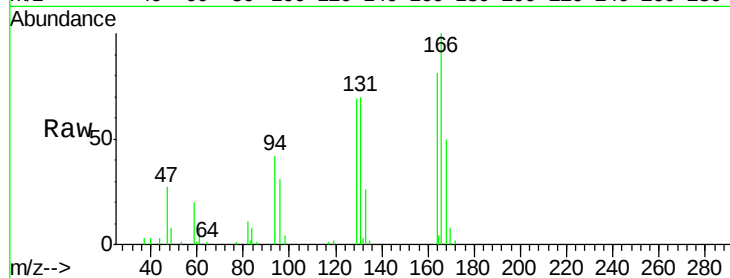


Abundance Ion 163.80 (163.50 to 164.50): V

Ion 165.80 (165.50 to 166.50): V

Ion 128.80 (128.50 to 129.50): V

Ion 130.80 (130.50 to 131.50): V

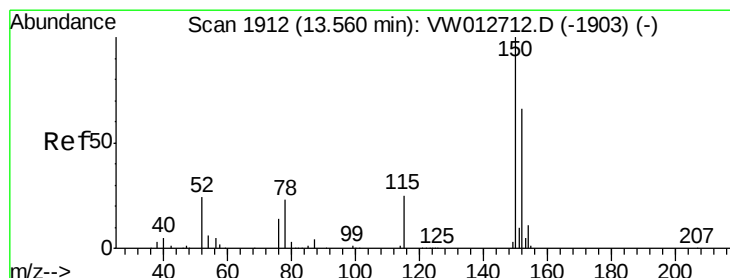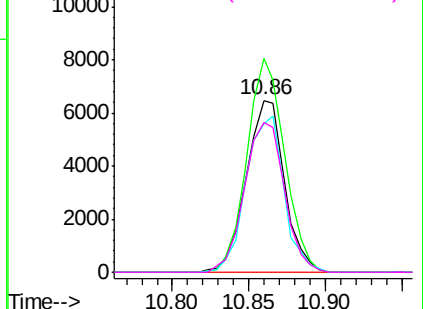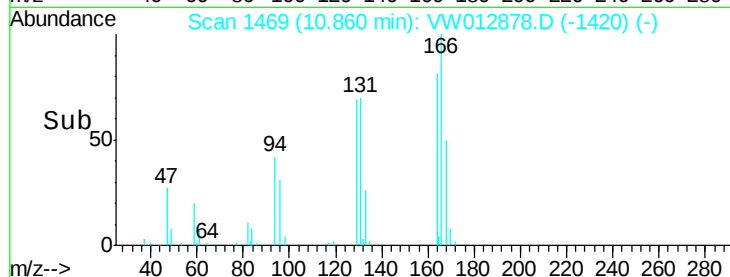

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. 0.00 min

Lab File: VW012878.D

Acq: 10 Sep 2019 18:33


Tgt Ion:152 Resp: 12678

Ion Ratio Lower Upper

152 100

115 55.6 30.0 90.1

150 152.2 0.0 349.0

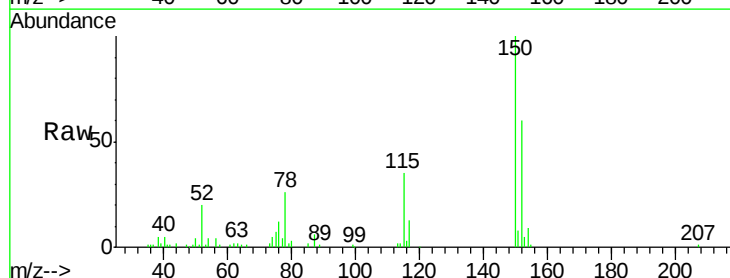

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

