

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW091020\
 Data File : VW016529.D
 Acq On : 10 Sep 2020 17:10
 Operator : SY/VA
 Sample : L3957-01
 Misc : 5.69G/10ML/MSVOA W/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFWP8

Quant Time: Sep 11 07:37:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 11 06:07:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	548112	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	406101	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	119795	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	113196	19.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.88%
7) Chloroethane-d5	2.90	69	118477	22.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.76%
10) 1,1-Dichloroethene-d2	4.03	63	156980	11.74	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.96%
20) 2-Butanone-d5	7.09	46	53141	25.59	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	51.18%
24) Chloroform-d	7.65	84	279735	21.79	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.16%
26) 1,2-Dichloroethane-d4	8.31	65	151975	21.65	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.60%
29) Benzene-d6	8.28	84	431594	20.91	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.64%
33) 1,2-Dichloropropane-d6	9.28	67	154726	25.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.04%
37) Toluene-d8	10.32	98	347608	17.71	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.84%
38) trans-1,3-Dichloropropene-	10.58	79	54905	17.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.76%
39) 2-Hexanone-d5	10.93	63	34958	28.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	56.40%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	111705	21.78	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.12%
61) 1,2-Dichlorobenzene-d4	13.86	152	93445	22.57	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.28%


Target Compounds				Ovalue
16) Methylene chloride	4.93	84	20095	2.349 ug/L 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW091020\
Data File : VW016529.D
Acq On : 10 Sep 2020 17:10
Operator : SY/VA
Sample : L3957-01
Misc : 5.69G/10ML/MSVOA W/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFWP8

Quant Time: Sep 11 07:37:01 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 11 06:07:14 2020
Response via : Initial Calibration

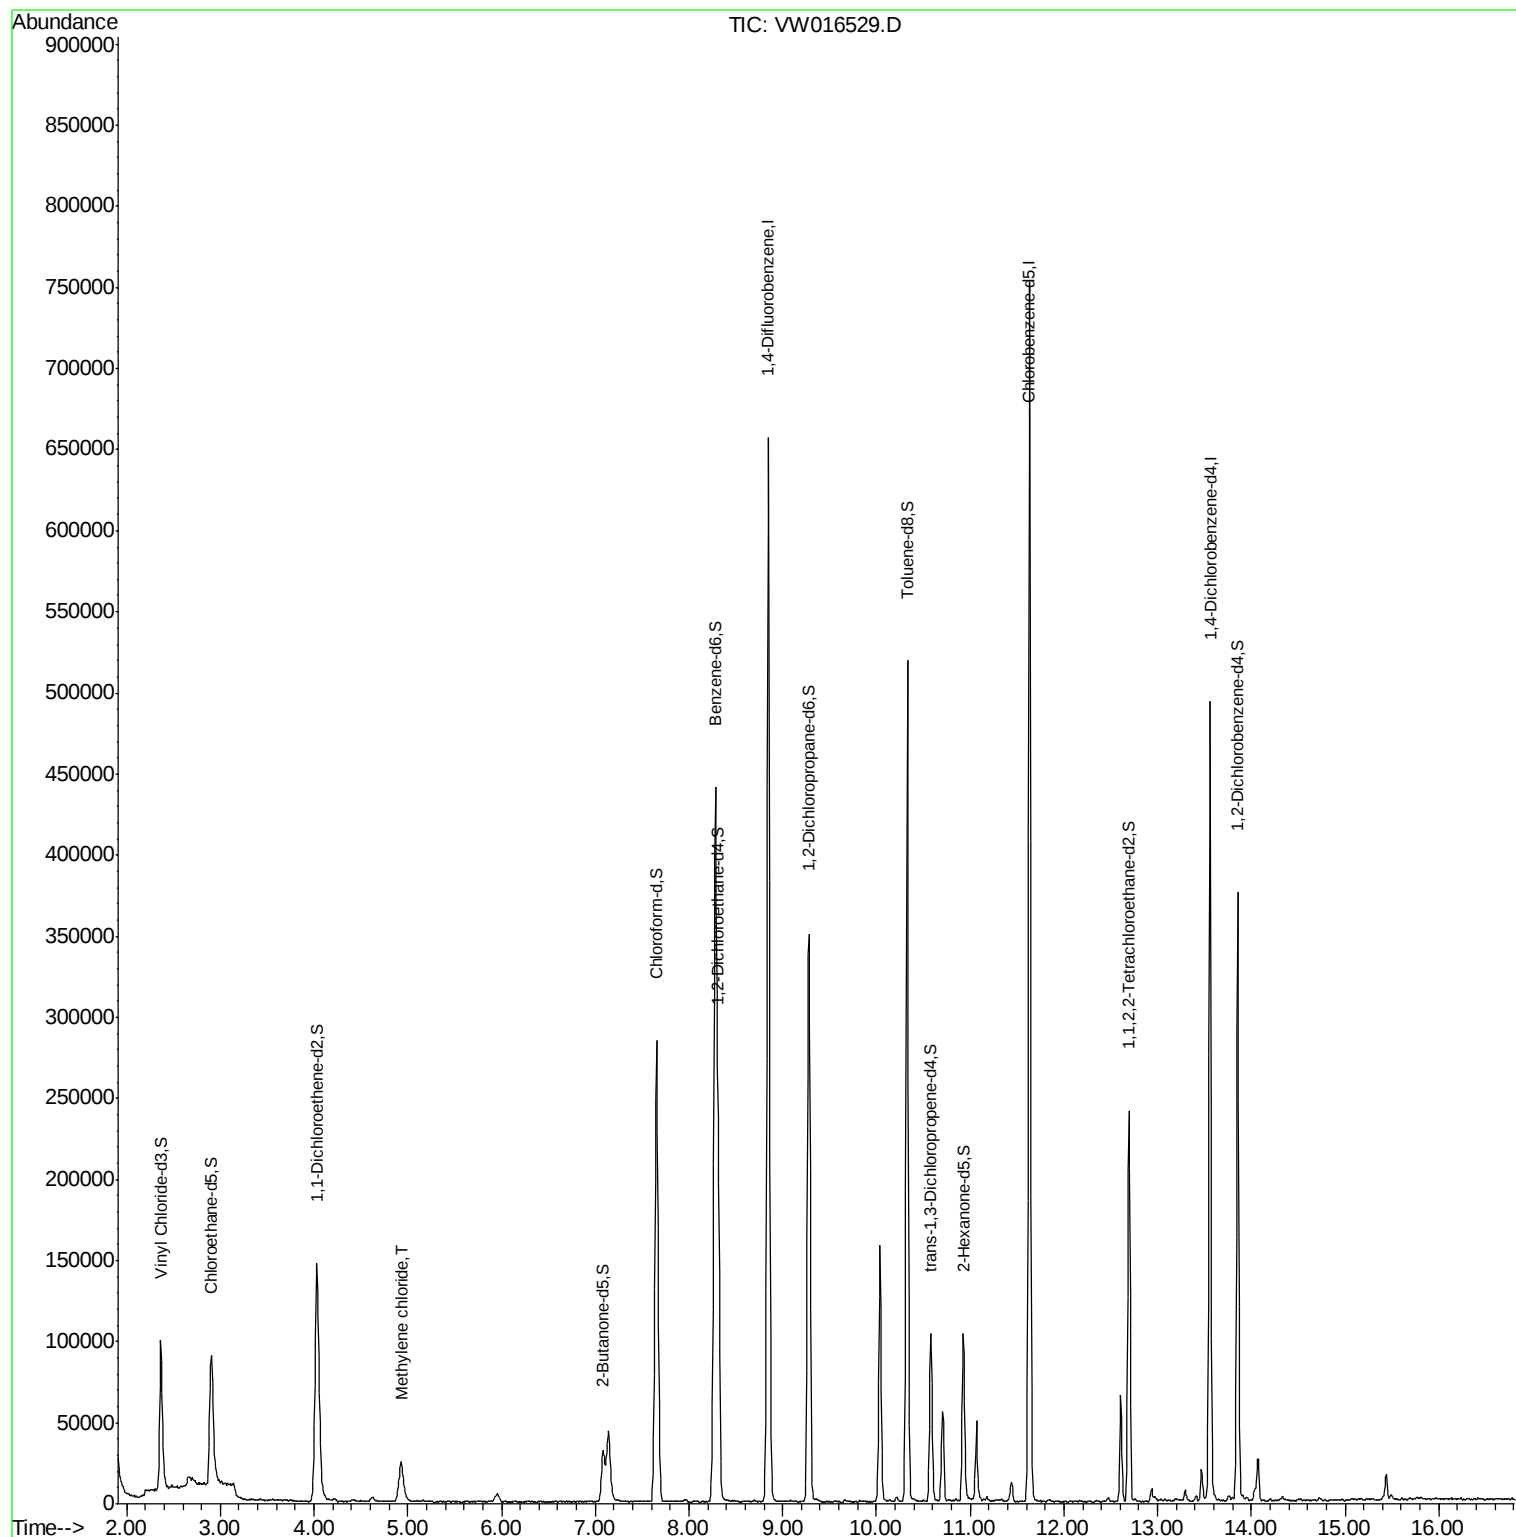

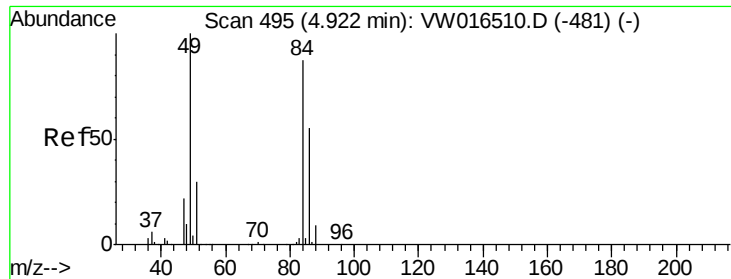

#16
 Methvlene chloride
 Concen: 2.349 ug/L
 RT: 4.93 min Scan# 497
 Delta R.T. 0.01 min
 Lab File: VW016529.D
 Acq: 10 Sep 2020 17:10

Instrument :
 MSVOA_W
 ClientSampleId :
 BFWP8

Tot Ion: 84 Resp: 20095
 Ion Ratio Lower Upper
 84 100
 49 120.6 86.7 160.9
 86 69.5 44.9 83.5

