


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW091119\
 Data File : VW012905.D
 Acq On : 11 Sep 2019 09:33
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W090719S.M
 Title : SW846 8260
 Last Update : Sun Sep 08 05:04:40 2019

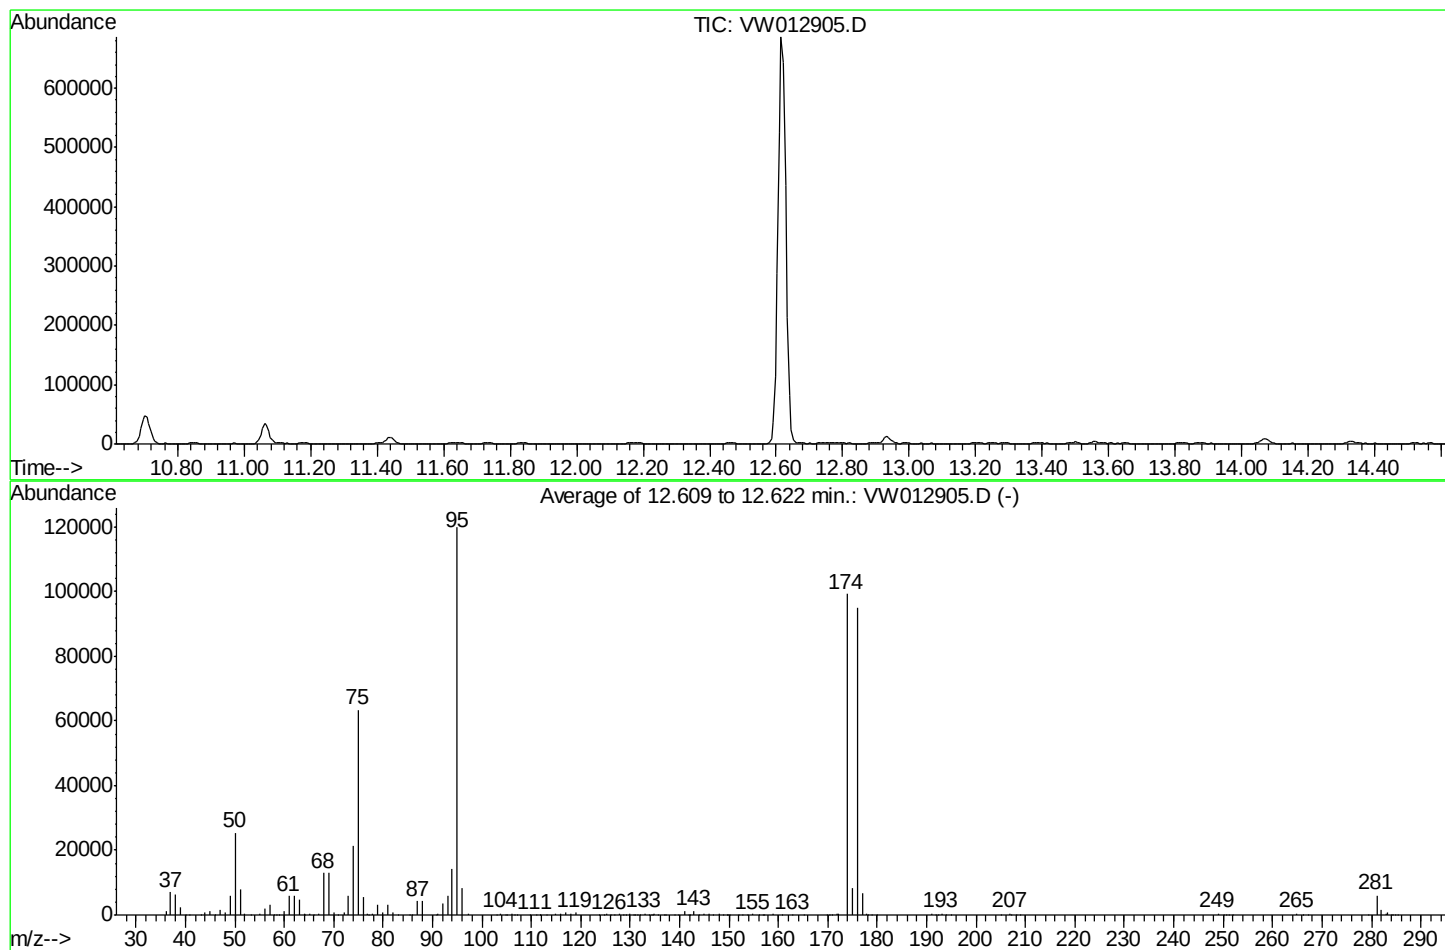

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	25458	PASS
75	95	30	60	52.8	63333	PASS
95	95	100	100	100.0	119856	PASS
96	95	5	9	6.9	8293	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.8	99285	PASS
175	174	5	9	8.4	8347	PASS
176	174	95	101	95.6	94920	PASS
177	176	5	9	7.1	6705	PASS