

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW091120\
 Data File : VW016538.D
 Acq On : 11 Sep 2020 10:19
 Operator : SY/VA
 Sample : L3949-04
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 9/14/2020 9:47:58 AM

Quant Time: Sep 12 07:22:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 12 07:12:32 2020
 Response via : Initial Calibration

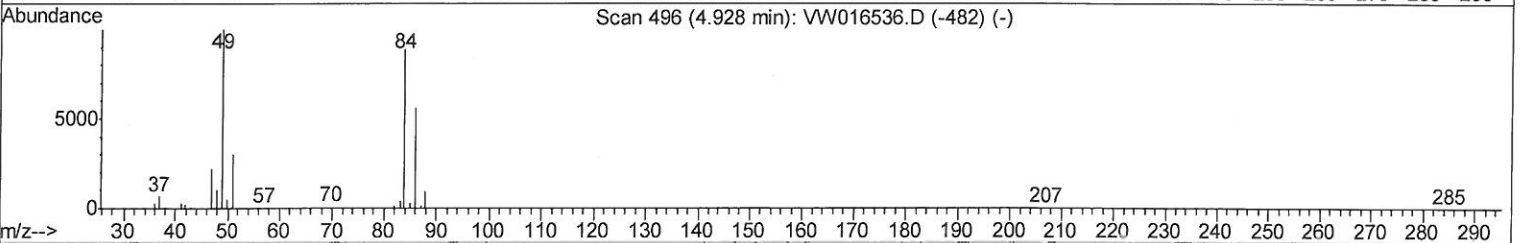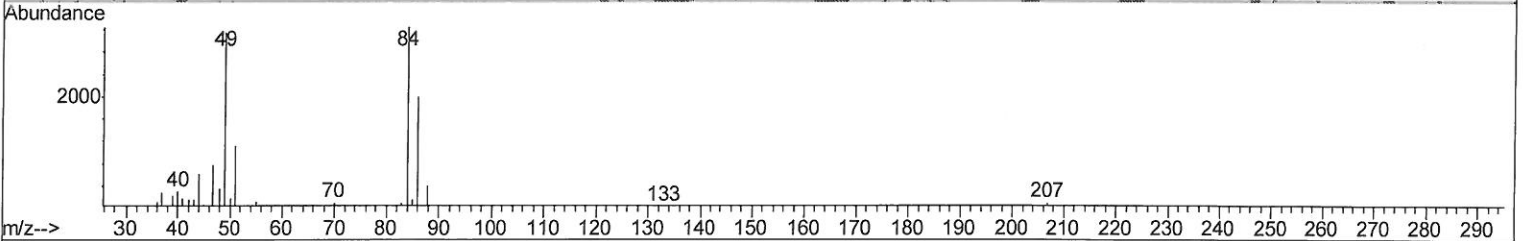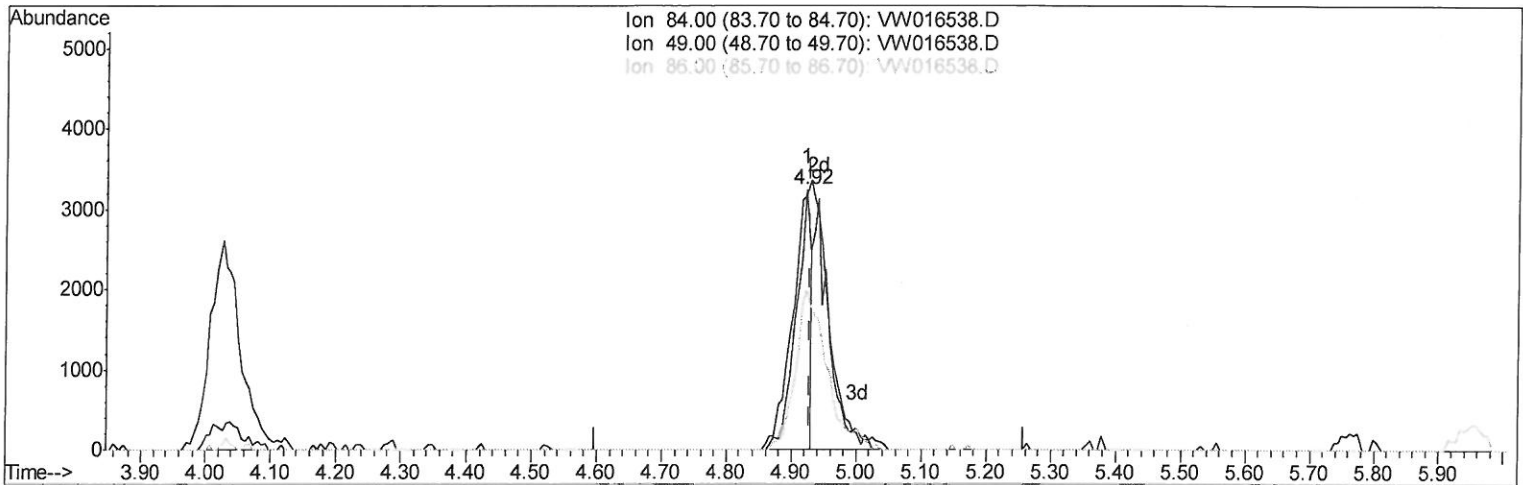

TIC: VW016538.D

(16) Methylene chloride (T)

4.922min (-0.006) 0.57ug/L

response 5075

Ion	Exp%	Act%
84.00	100	100
49.00	123.80	97.35
86.00	64.20	61.28
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW091120\
 Data File : VW016538.D
 Acq On : 11 Sep 2020 10:19
 Operator : SY/VA
 Sample : L3949-04
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 9/14/2020 9:47:58 AM

Quant Time: Sep 12 07:22:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Sep 12 07:12:32 2020
 Response via : Initial Calibration

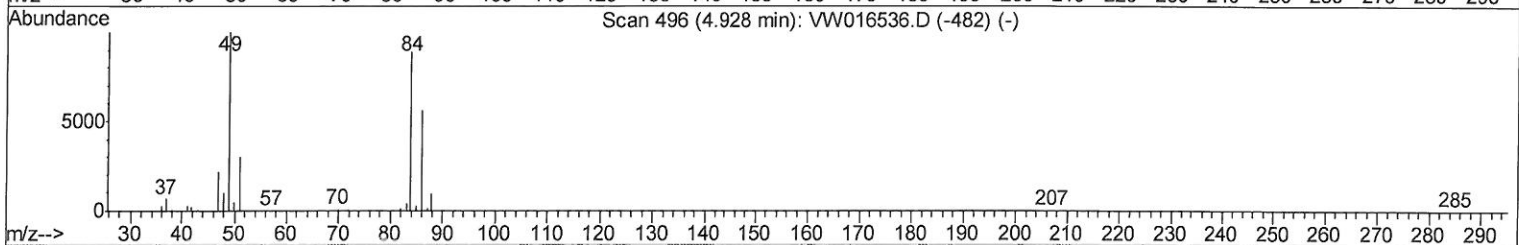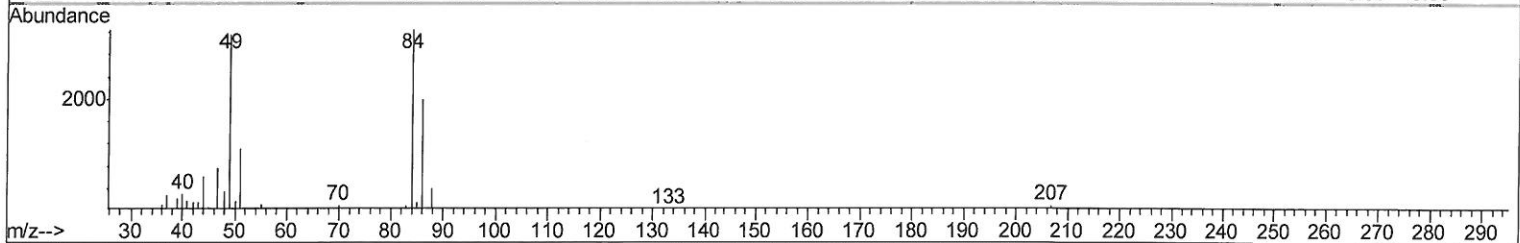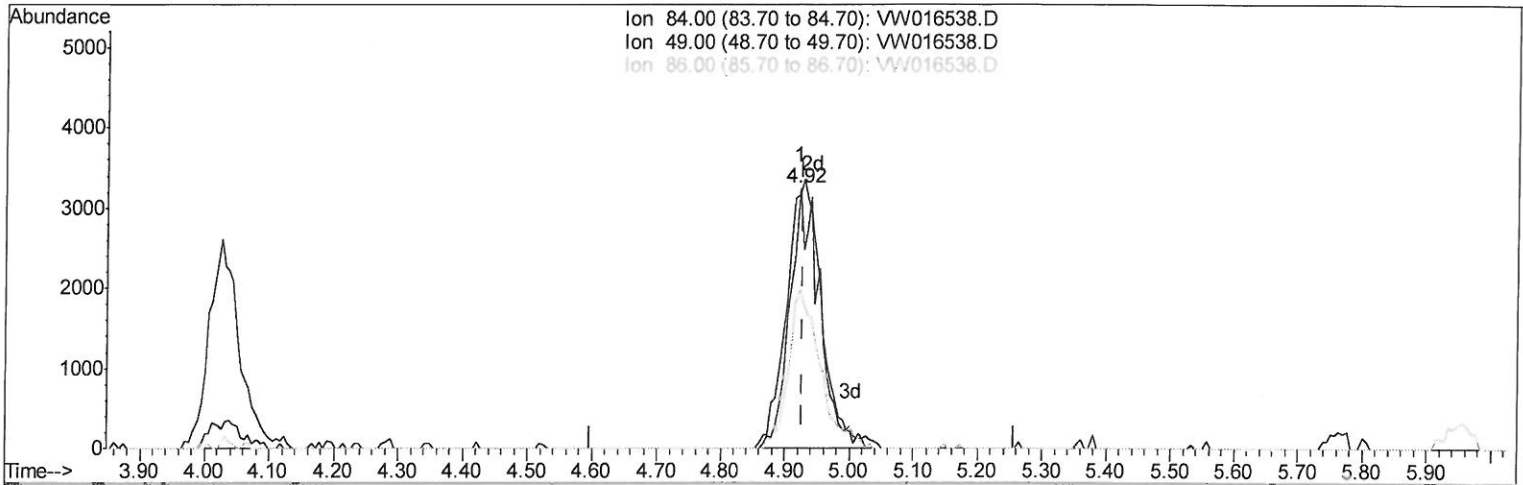

TIC: VW016538.D

(16) Methylene chloride (T)

4.922min (-0.006) 1.18ug/L m

response 10483

Ion	Exp%	Act%
84.00	100	100
49.00	123.80	97.35
86.00	64.20	61.28
0.00	0.00	0.00

509/14/20 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091120\
Quantitation Report (LSC Reviewed)

Data File : VW016538.D
Acq On : 11 Sep 2020 10:19
Operator : SY/VA
Sample : L3949-04
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

MMDadoda
9/14/2020 9:47:58 AM

Quant Time: Sep 14 09:22:38 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 12 07:12:32 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	571085	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	499269	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	217126	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	126897	20.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.76%
7) Chloroethane-d5	2.90	69	130349	23.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.84%
10) 1,1-Dichloroethene-d2	4.03	63	213847	15.35	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.40%
20) 2-Butanone-d5	7.09	46	84615	39.10	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.20%
24) Chloroform-d	7.65	84	314184	23.49	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.96%
26) 1,2-Dichloroethane-d4	8.31	65	174293	23.83	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.32%
29) Benzene-d6	8.28	84	608348	23.97	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.88%
33) 1,2-Dichloropropane-d6	9.28	67	177970	23.87	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.48%
37) Toluene-d8	10.33	98	579583	24.02	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.08%
38) trans-1,3-Dichloropropene-	10.58	79	82209	21.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.40%
39) 2-Hexanone-d5	10.93	63	67824	44.50	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.00%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	147806	23.44	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.76%
61) 1,2-Dichlorobenzene-d4	13.86	152	184192	24.55	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.20%

Target Compounds

16) Methylene chloride	4.92	84	10483m	1.176	ug/L	Qvalue
------------------------	------	----	--------	-------	------	--------

09/14/2020

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091120\
Quantitation Report (LSC Reviewed)

Data File : VW016538.D
Acq On : 11 Sep 2020 10:19
Operator : SY/VA
Sample : L3949-04
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

MMDadoda
9/14/2020 9:47:58 AM

Quant Time: Sep 14 09:22:38 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM090320S.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 12 07:12:32 2020
Response via : Initial Calibration

