




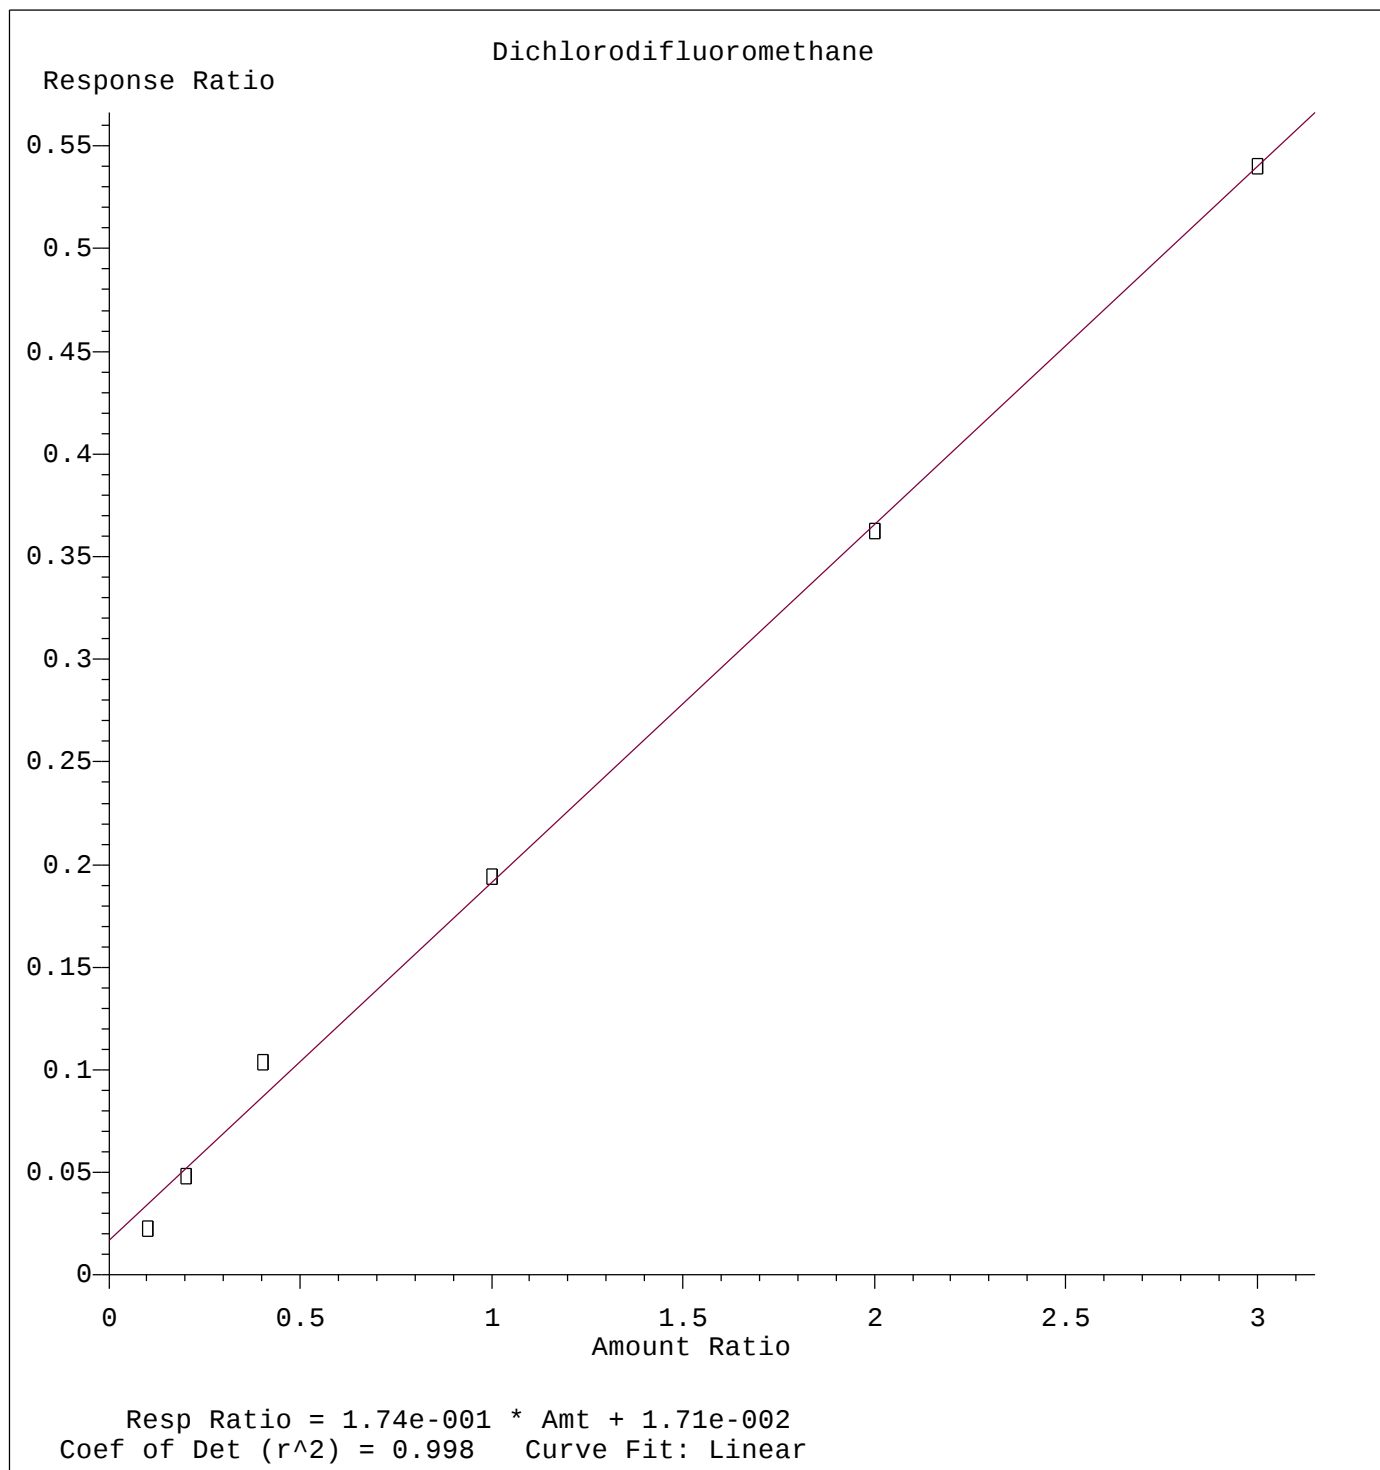


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Calibration Table Last Updated: Fri Sep 13 17:26:01 2019

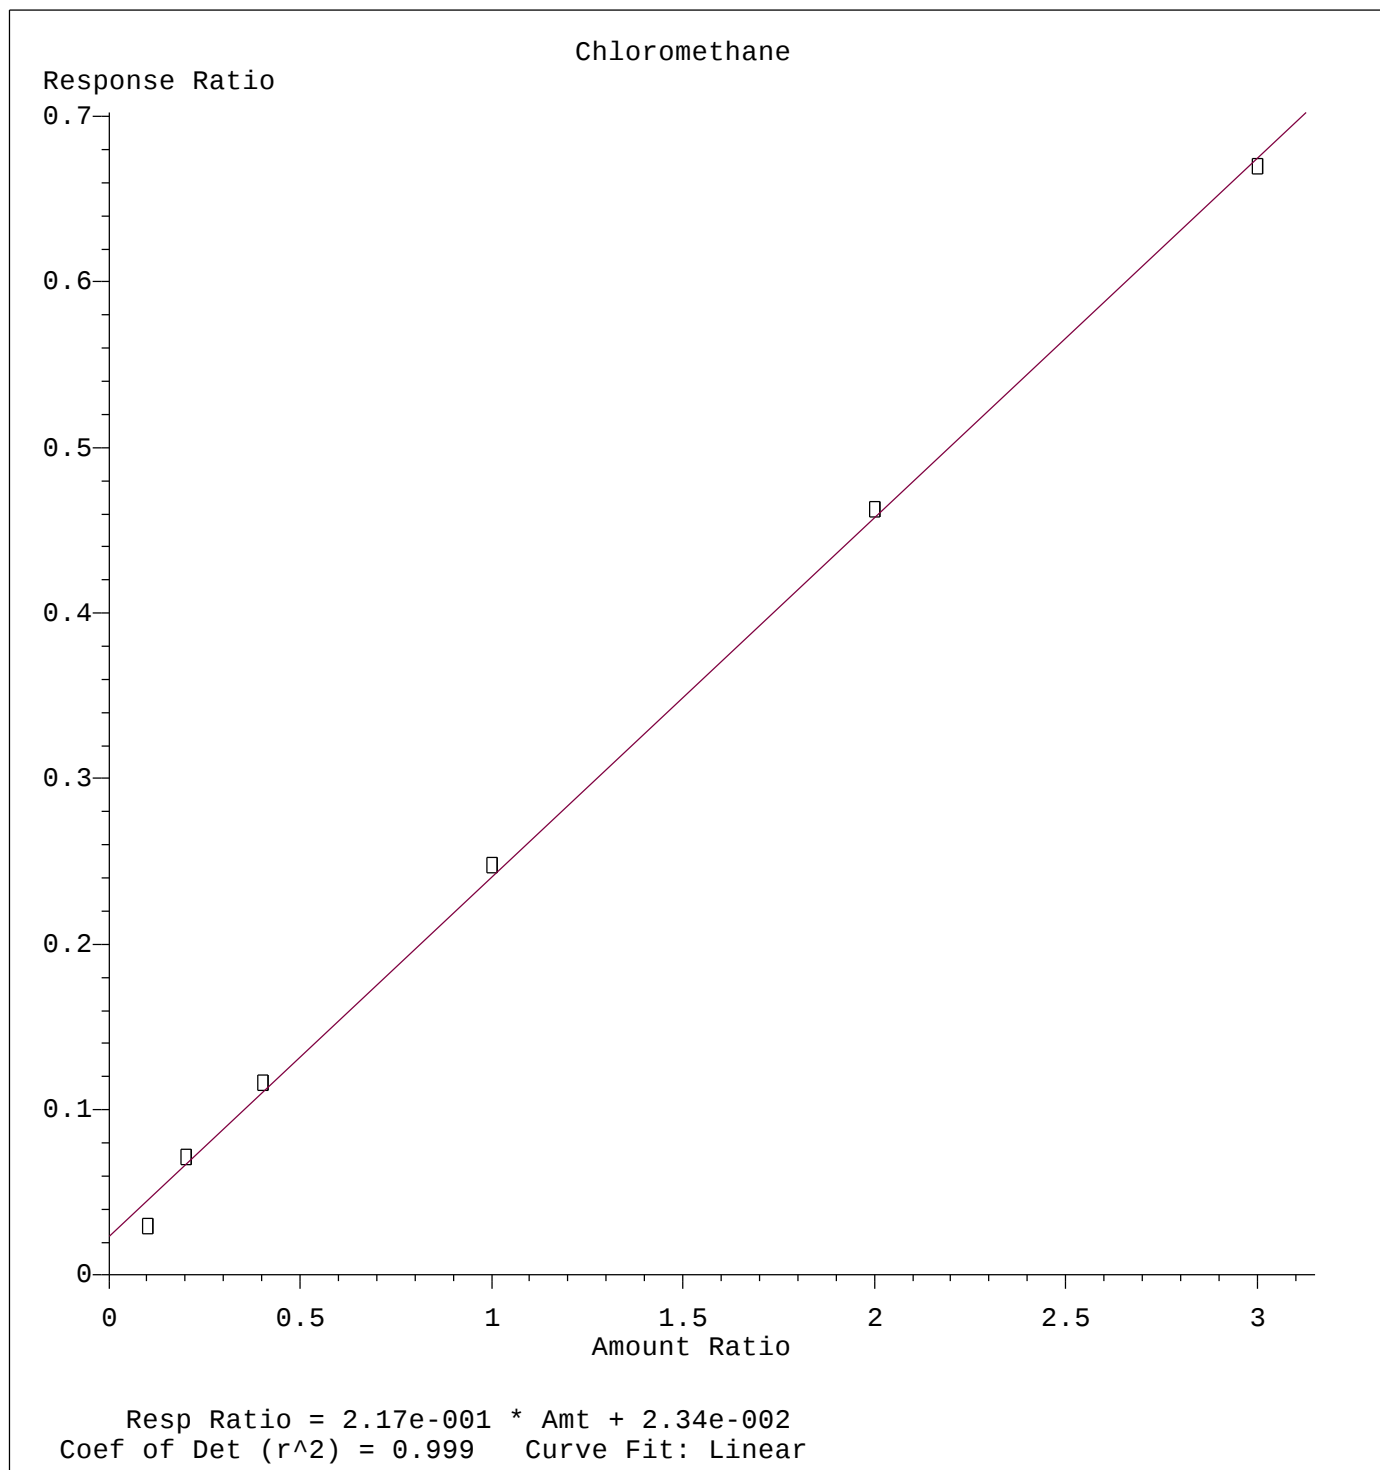


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Calibration Table Last Updated: Fri Sep 13 17:26:01 2019

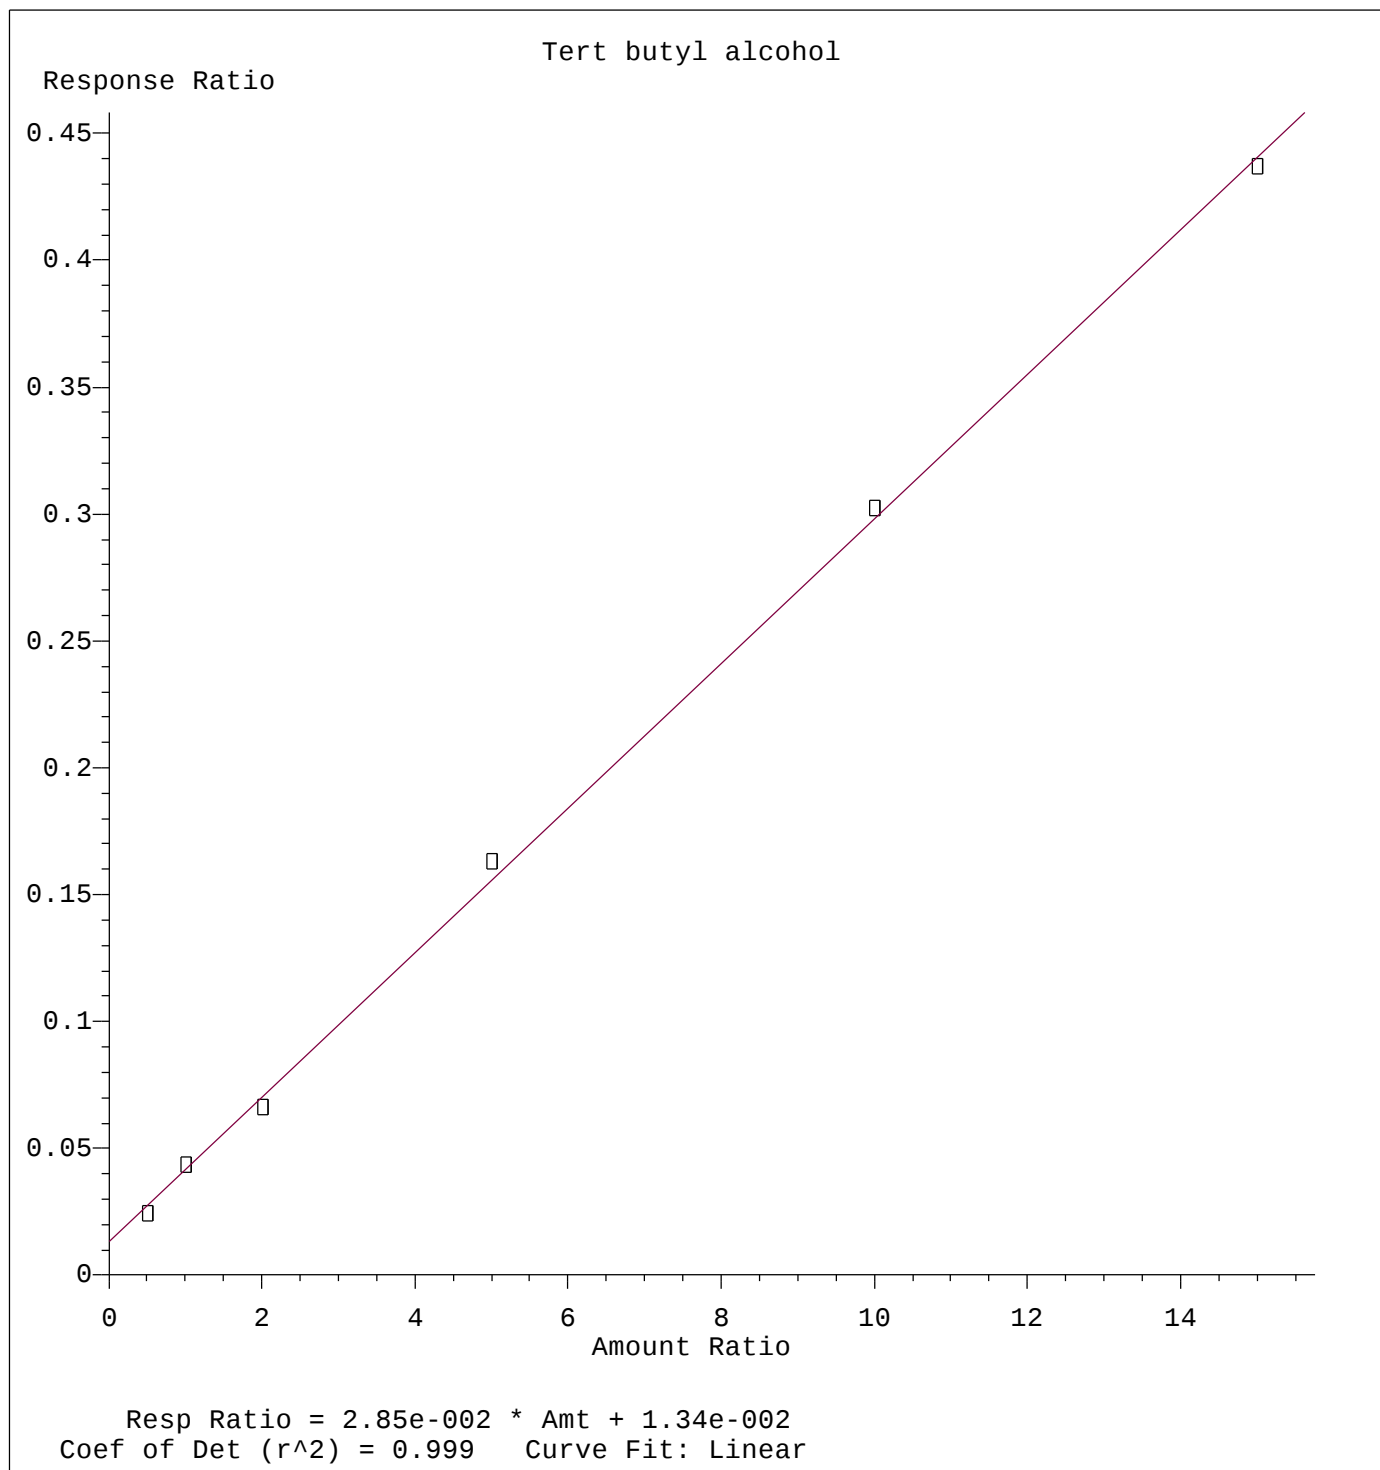

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Calibration Table Last Updated: Fri Sep 13 17:26:01 2019

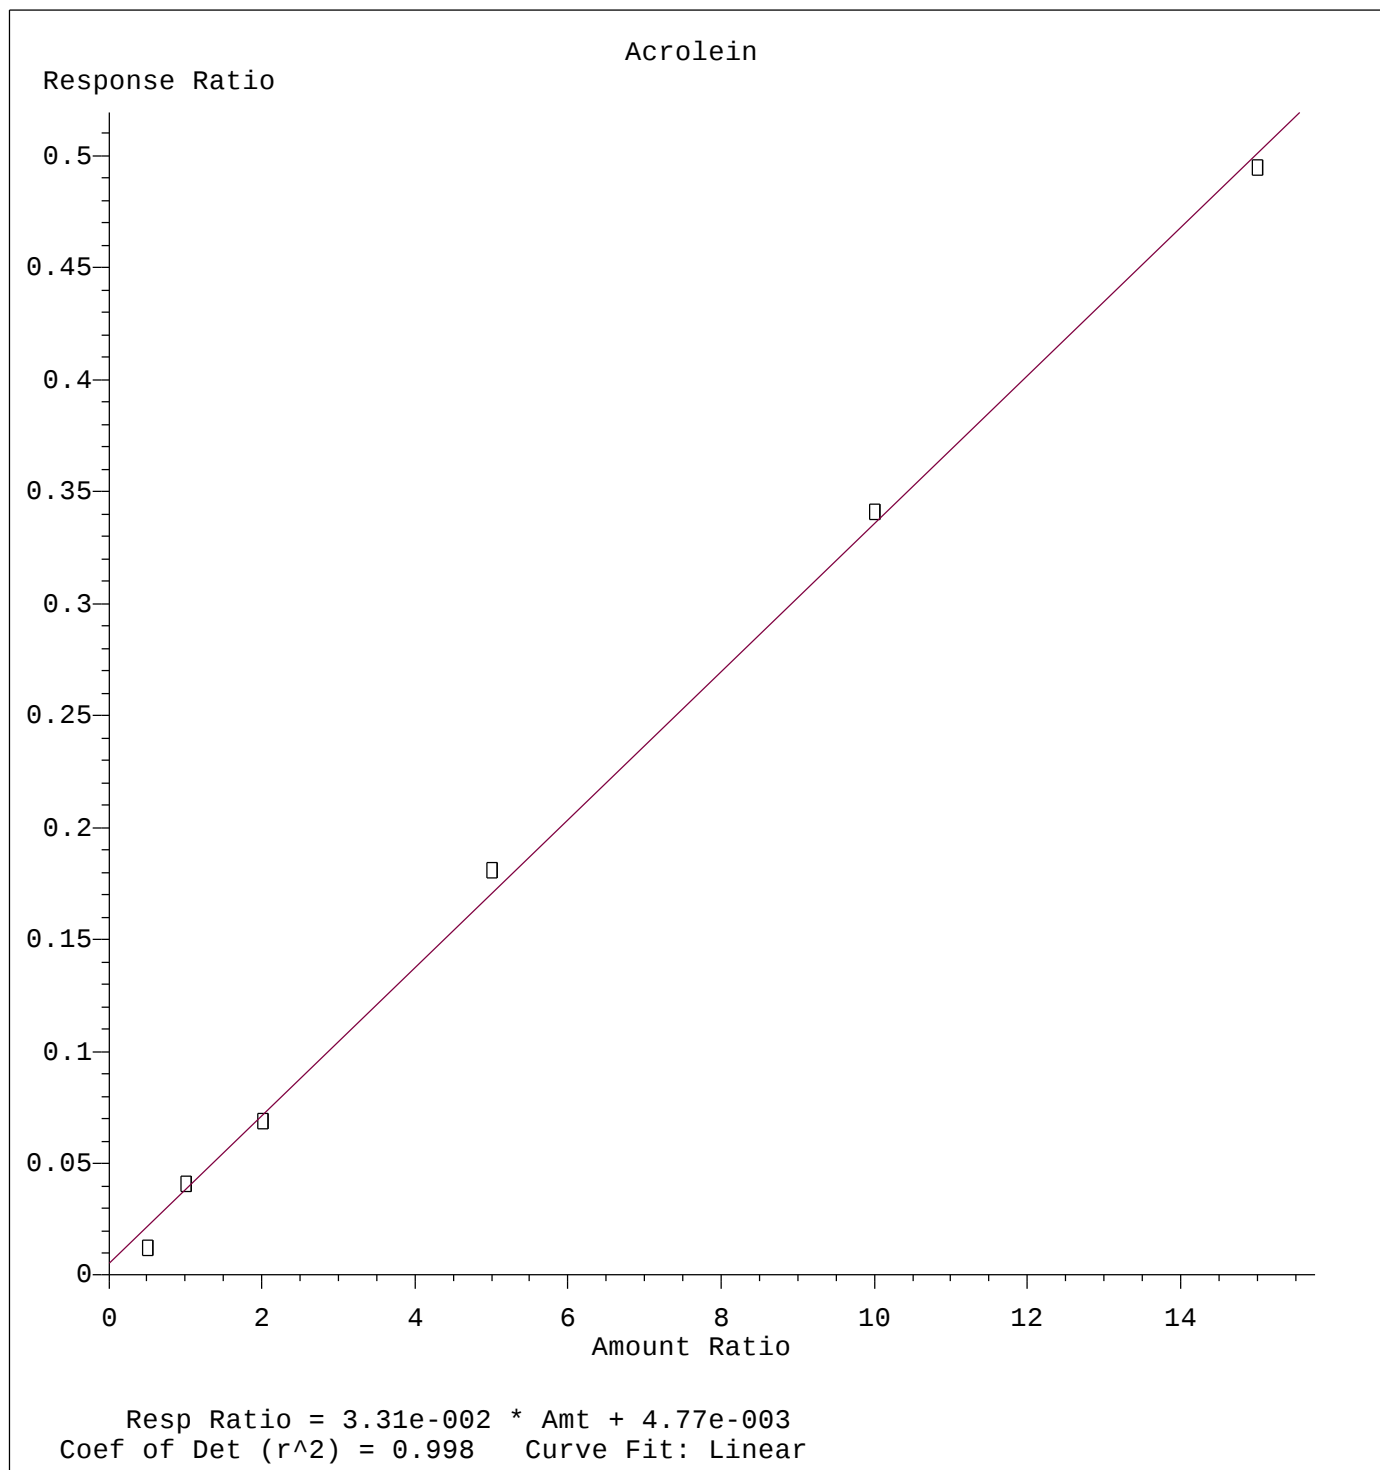


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Calibration Table Last Updated: Fri Sep 13 17:26:01 2019

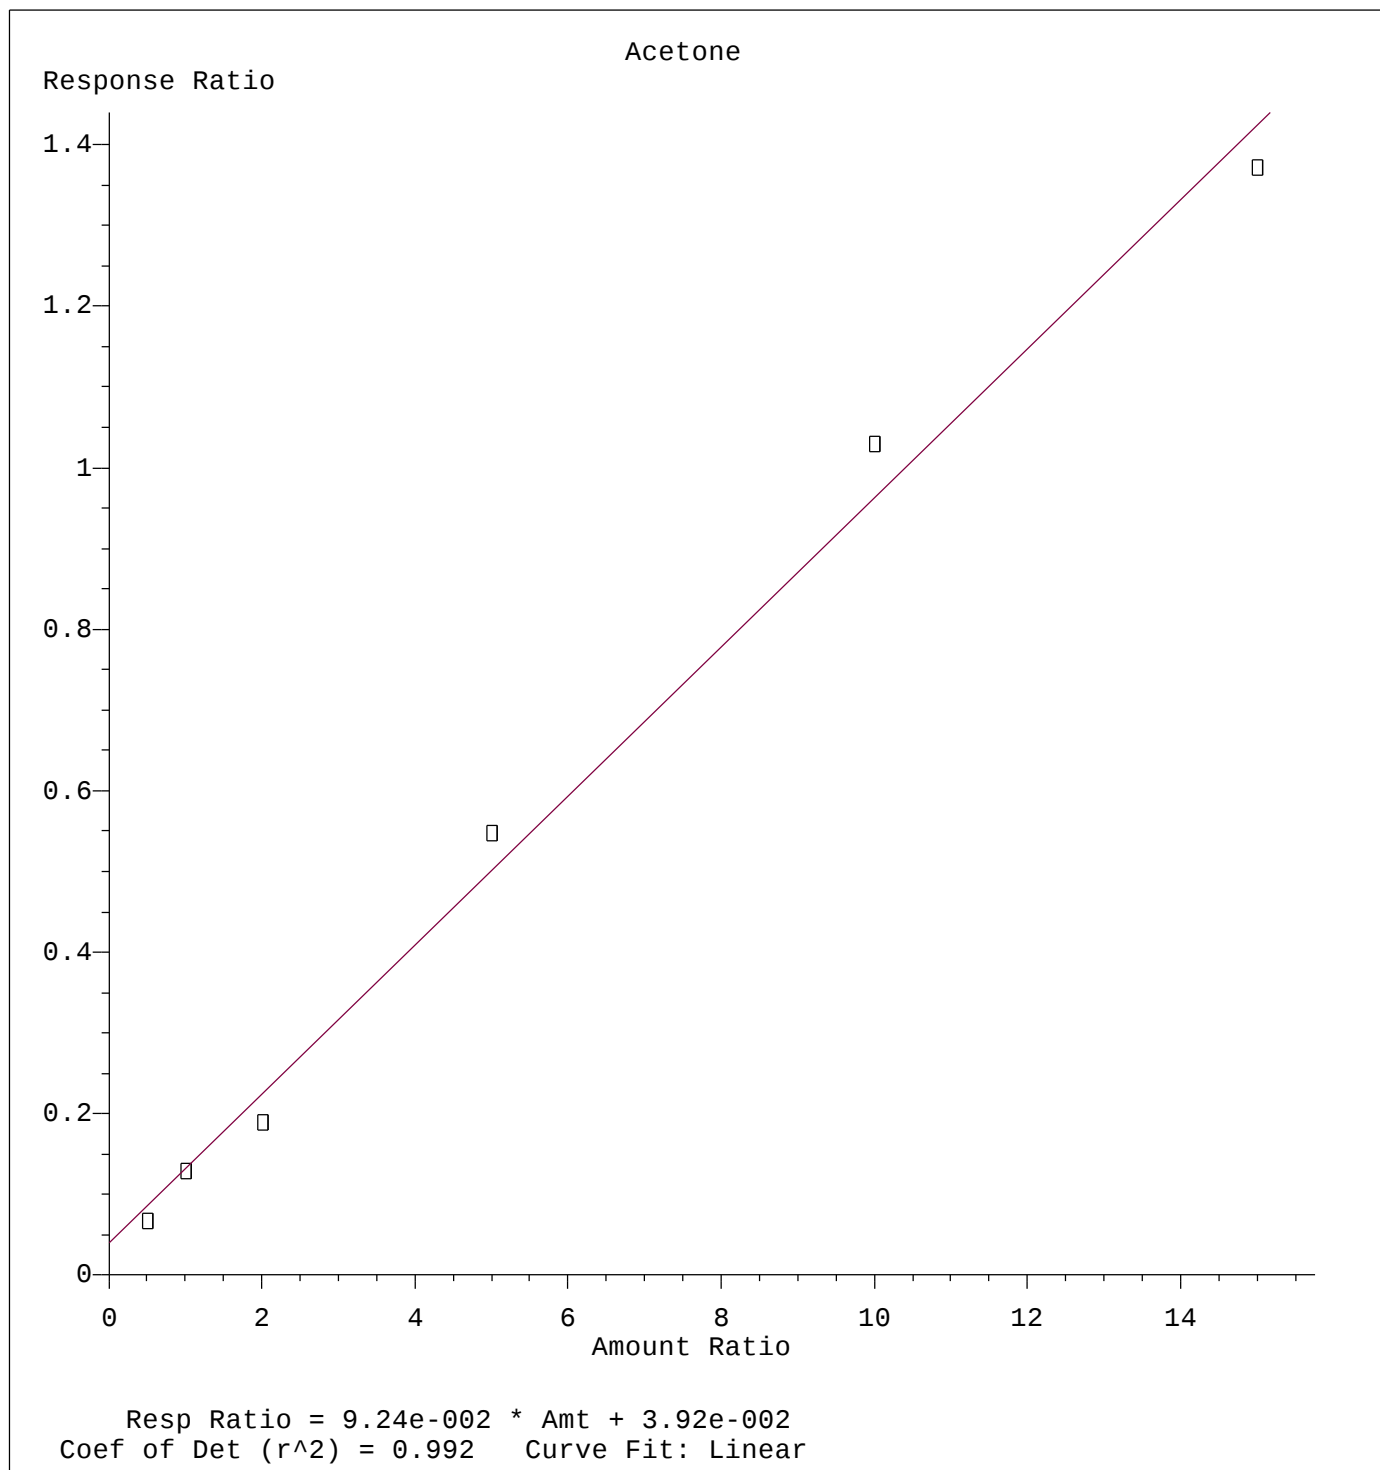

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Calibration Table Last Updated: Fri Sep 13 17:26:01 2019

Methylene Chloride

Response Ratio

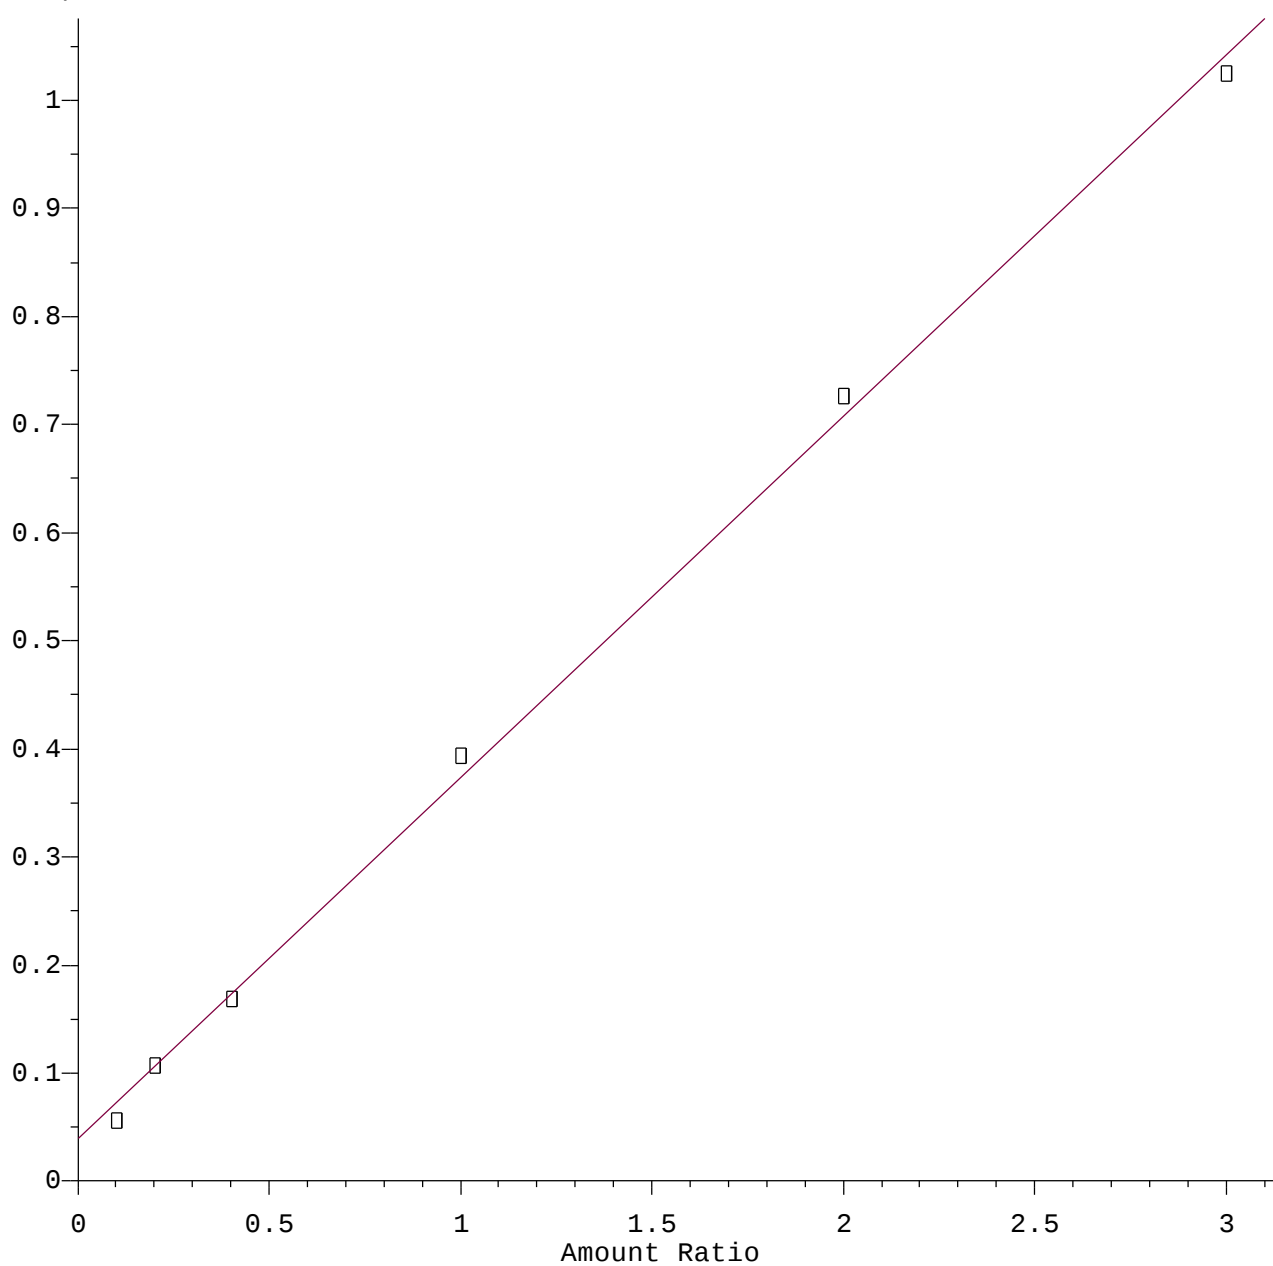


Resp Ratio = $3.34 \times 10^{-1} \times \text{Amt} + 3.87 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Calibration Table Last Updated: Fri Sep 13 17:26:01 2019


2,2-Dichloropropane

Response Ratio

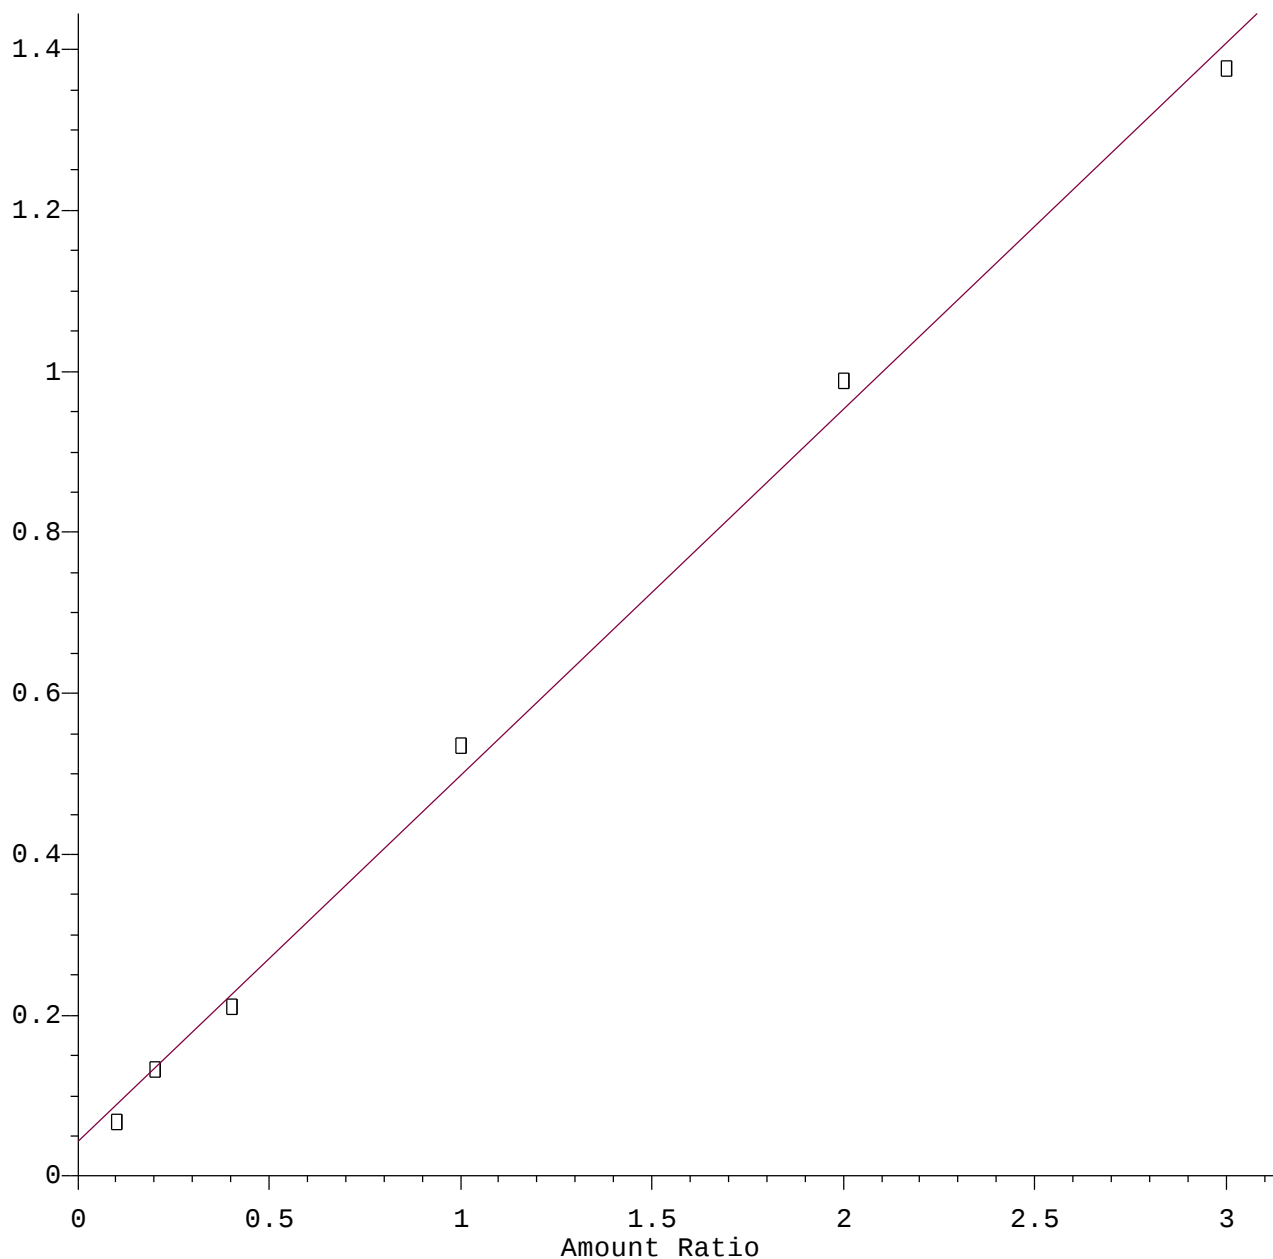

Resp Ratio = $4.55 \times 10^{-1} \times \text{Amt} + 4.32 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Calibration Table Last Updated: Fri Sep 13 17:26:01 2019

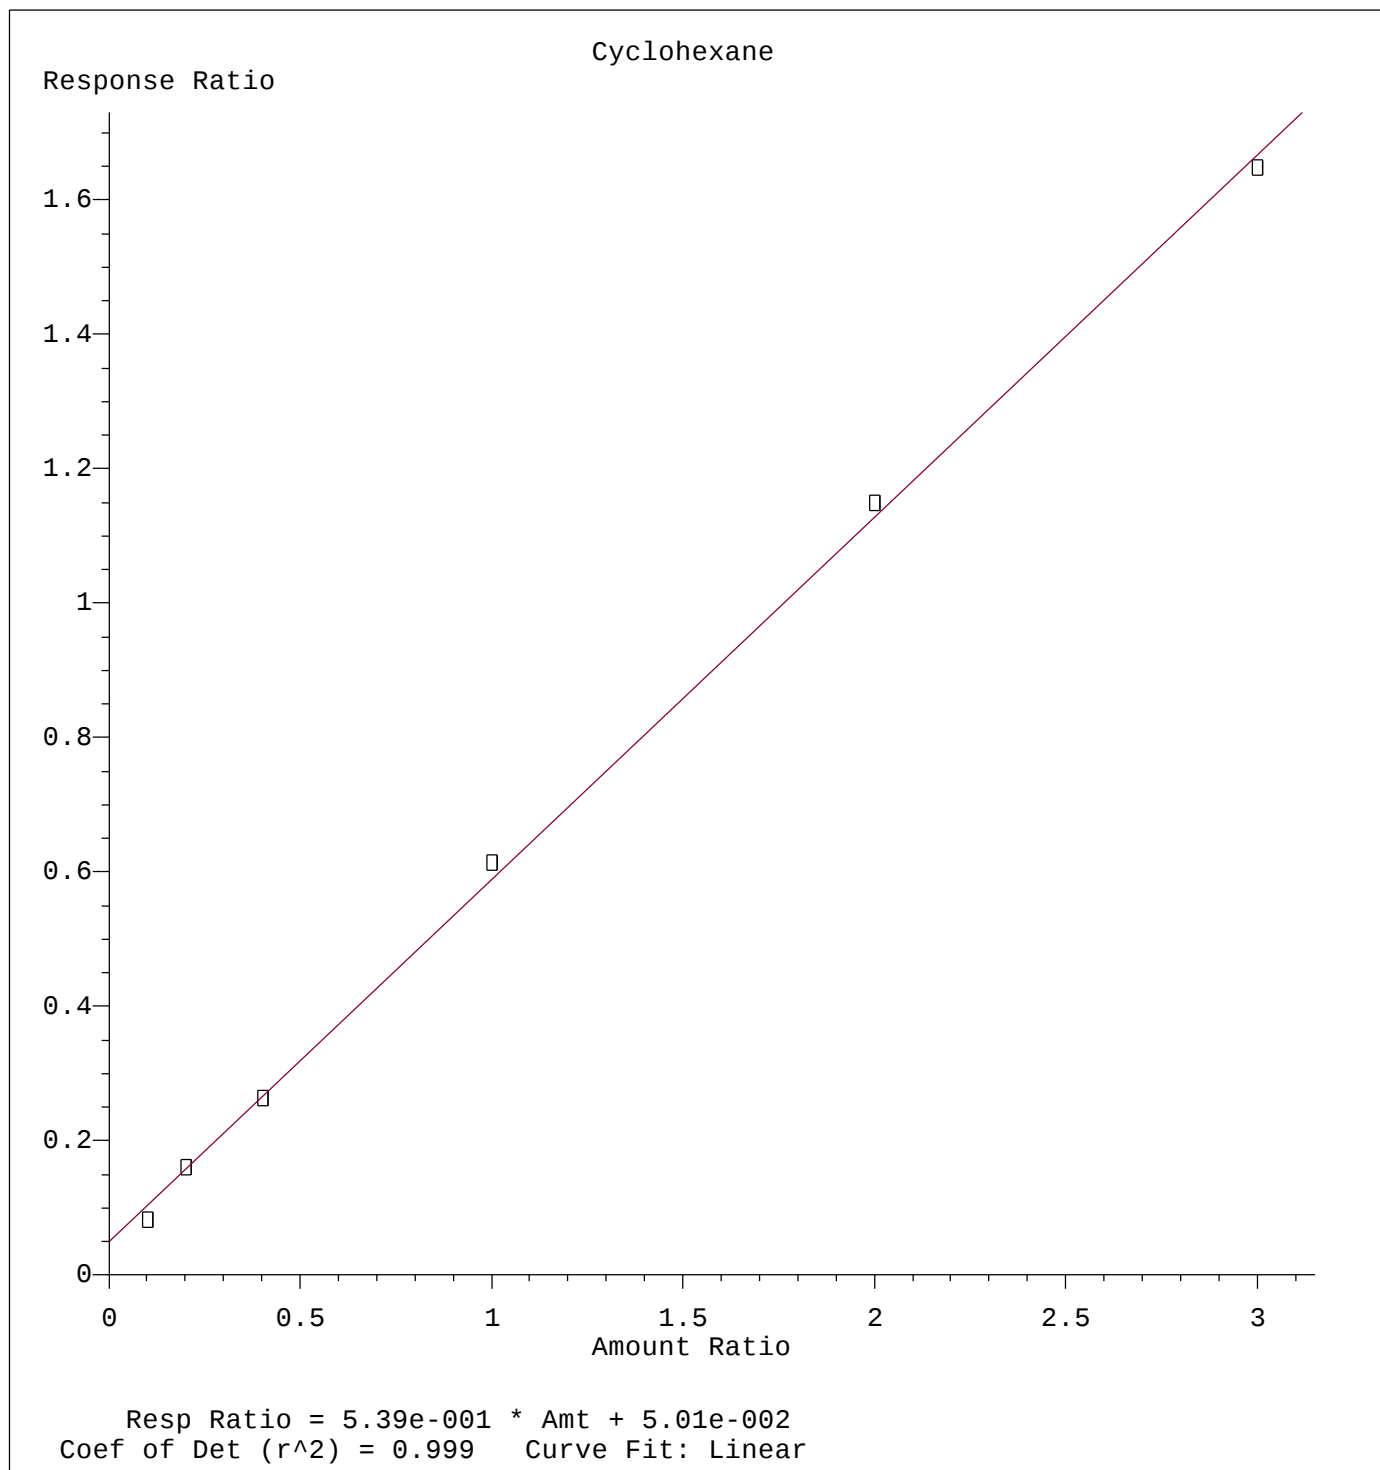

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Calibration Table Last Updated: Fri Sep 13 17:26:01 2019