


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW091419\
 Data File : VW012950.D
 Acq On : 13 Sep 2019 12:28
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
 Title : SW846 8260
 Last Update : Fri Sep 13 17:26:01 2019

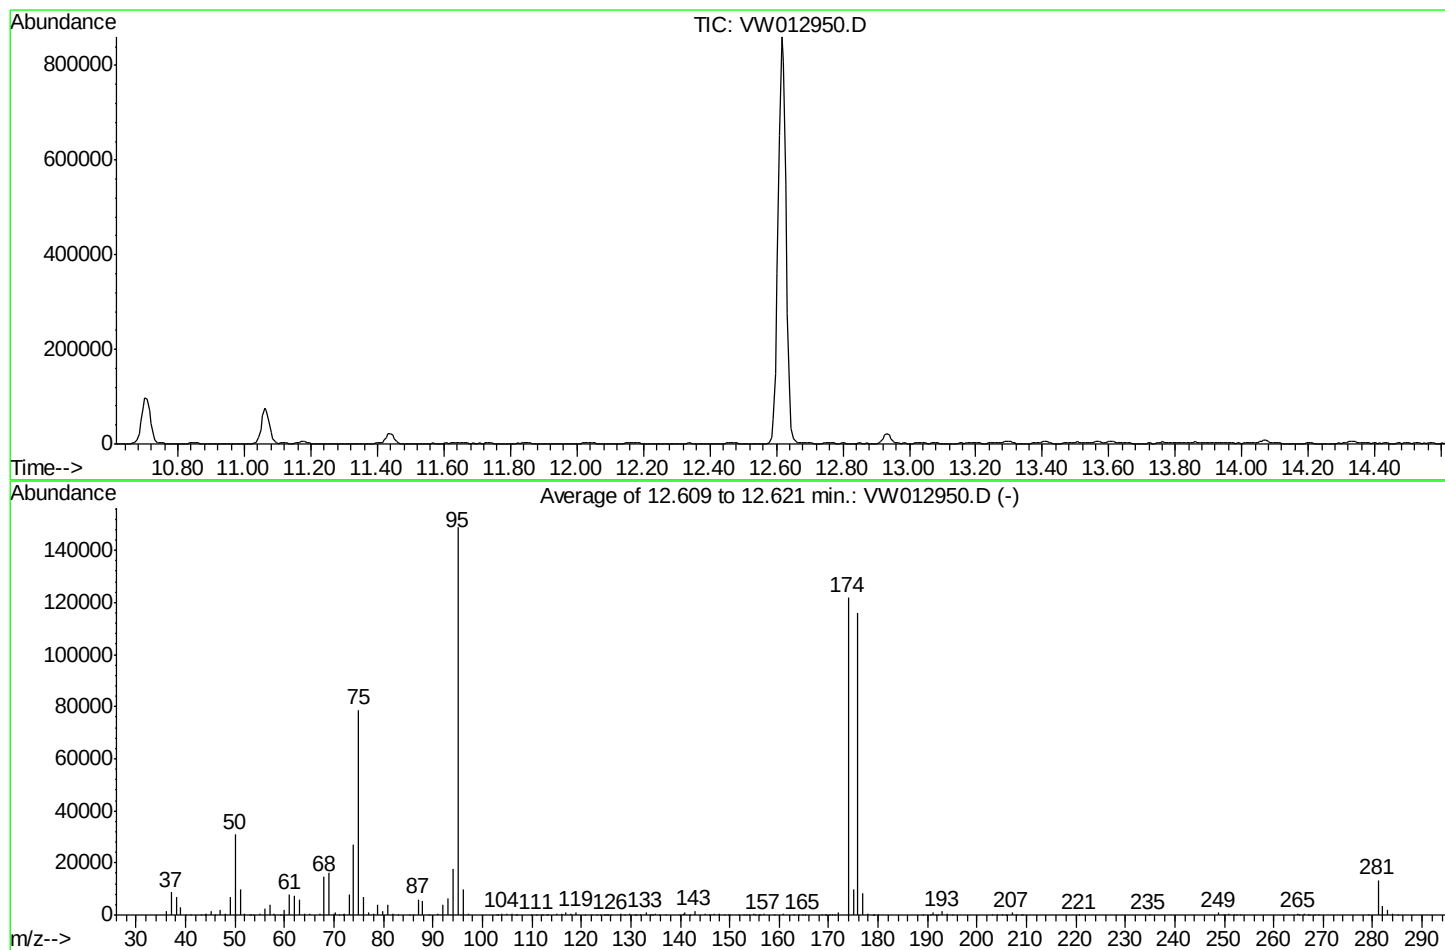

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	30938	PASS
75	95	30	60	53.0	78832	PASS
95	95	100	100	100.0	148848	PASS
96	95	5	9	6.6	9836	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.8	121816	PASS
175	174	5	9	8.2	10046	PASS
176	174	95	101	95.1	115810	PASS
177	176	5	9	7.1	8221	PASS