


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091419\
 Data File : VW012959.D
 Acq On : 13 Sep 2019 17:56
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
 Title : SW846 8260
 Last Update : Fri Sep 13 17:26:01 2019

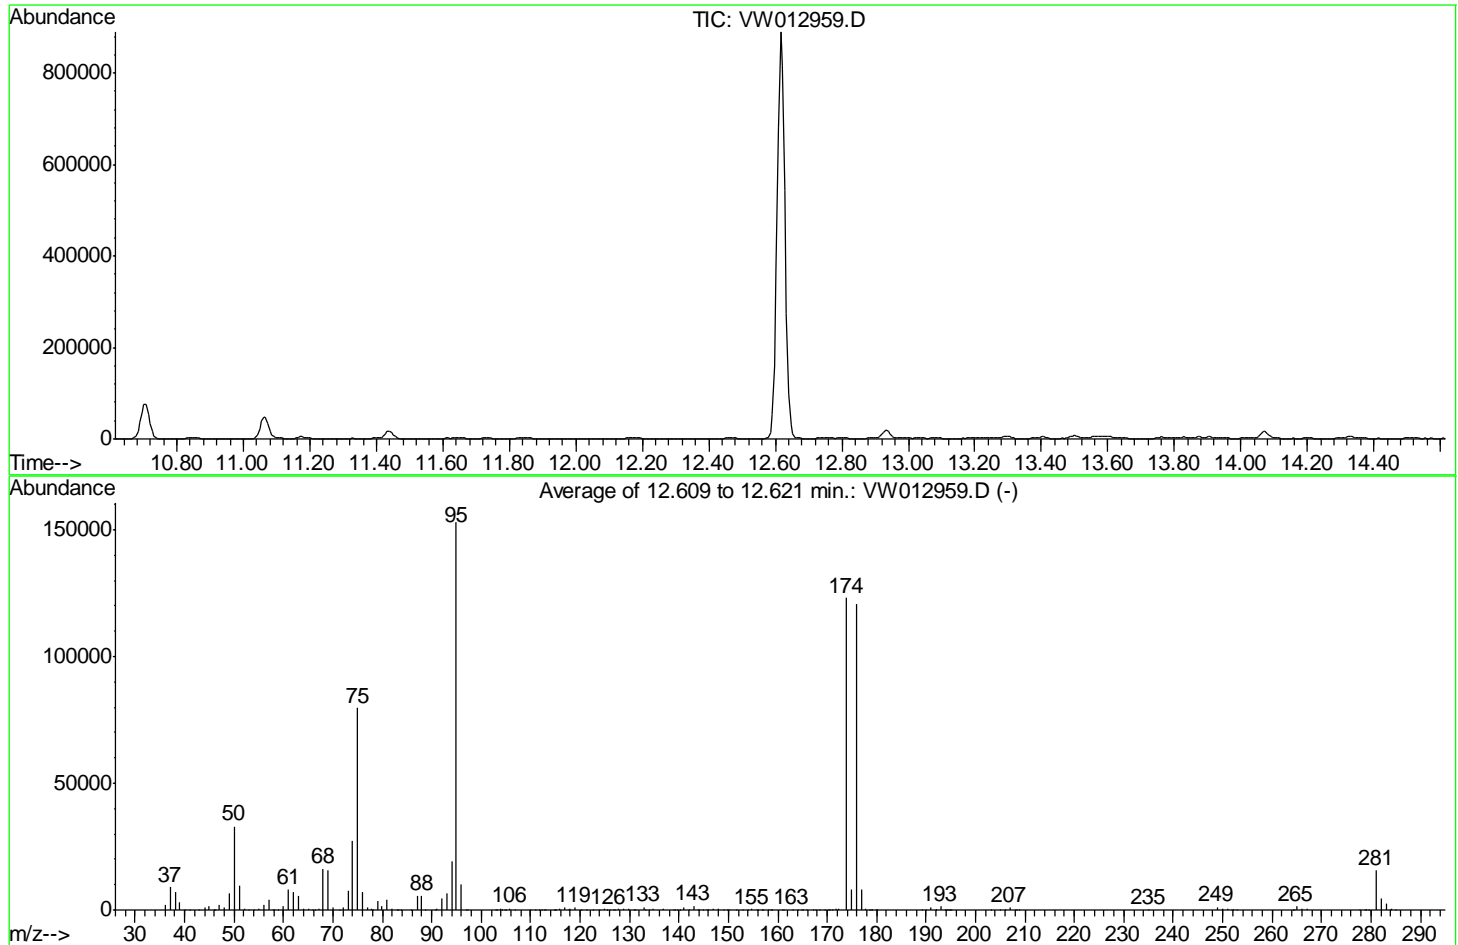

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	32882	PASS
75	95	30	60	52.1	79706	PASS
95	95	100	100	100.0	152938	PASS
96	95	5	9	6.5	9913	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.6	123192	PASS
175	174	5	9	6.5	8028	PASS
176	174	95	101	97.8	120520	PASS
177	176	5	9	6.8	8203	PASS