

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091520\
 Data File : VW016557.D
 Acq On : 15 Sep 2020 14:17
 Operator : SY/VA
 Sample : VSTD00505
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD00505

Manual Integrations
 APPROVED

MMDadoda
 9/16/2020 11:46:00 AM

Quant Time: Sep 15 15:15:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 15 15:13:12 2020
 Response via : Initial Calibration

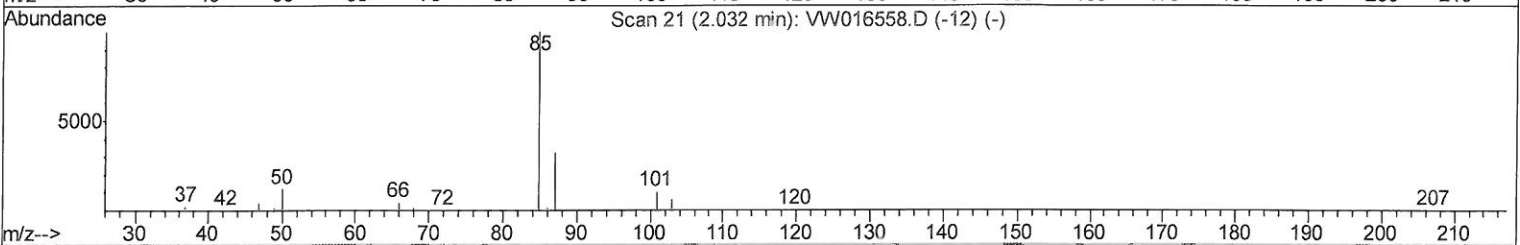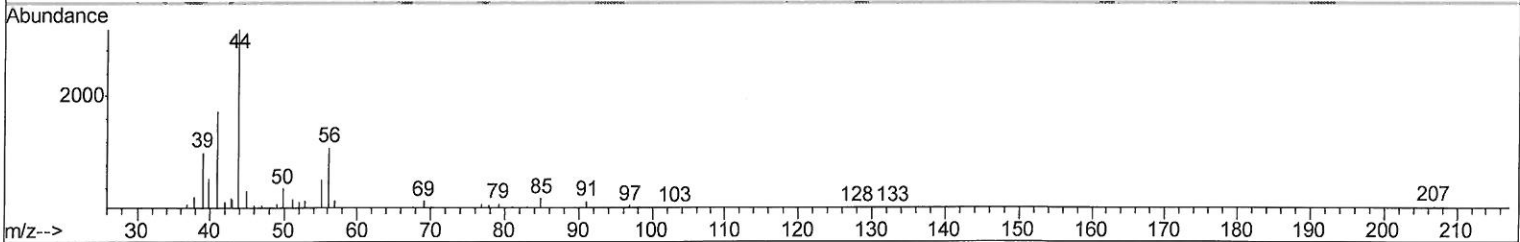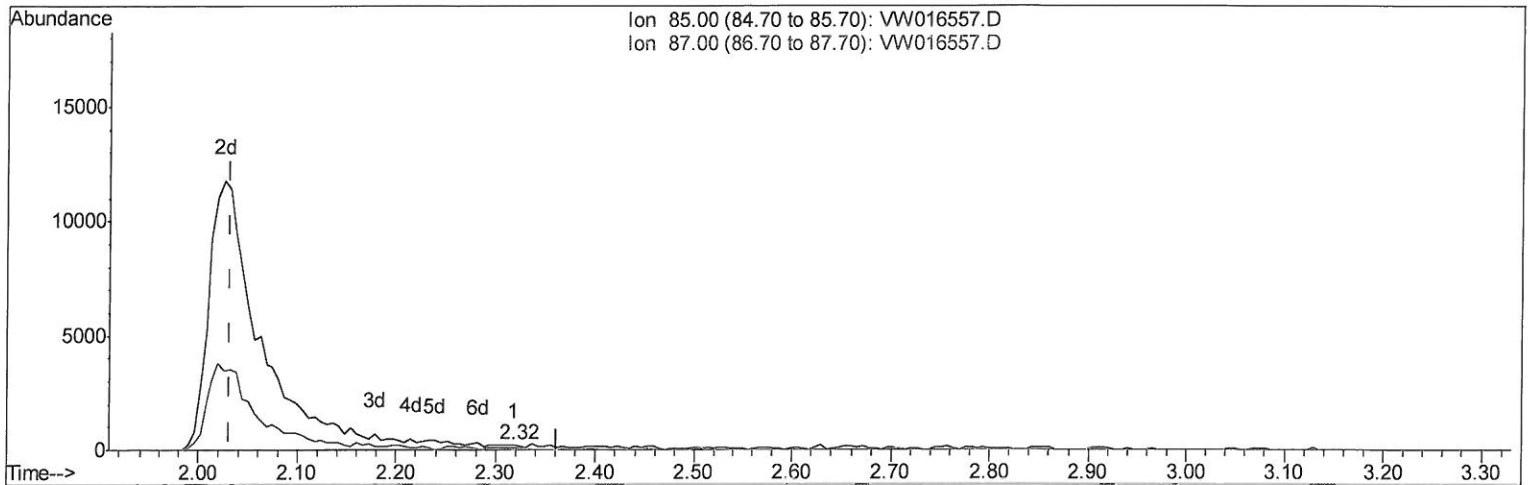

TIC: VW016557.D

(2) Dichlorodifluoromethane (T)

2.318min (+0.287) 0.02ug/L

response 165

Ion	Exp%	Act%
85.00	100	100
87.00	31.70	33.94
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091520\
 Data File : VW016557.D
 Acq On : 15 Sep 2020 14:17
 Operator : SY/VA
 Sample : VSTD00505
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD00505

Manual Integrations
 APPROVED

MMDadoda
 9/16/2020 11:46:00 AM

Quant Time: Sep 15 15:15:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 15 15:13:12 2020
 Response via : Initial Calibration

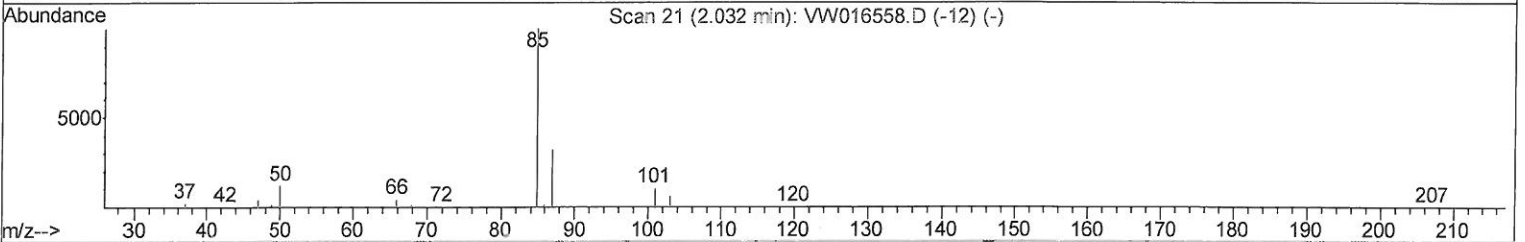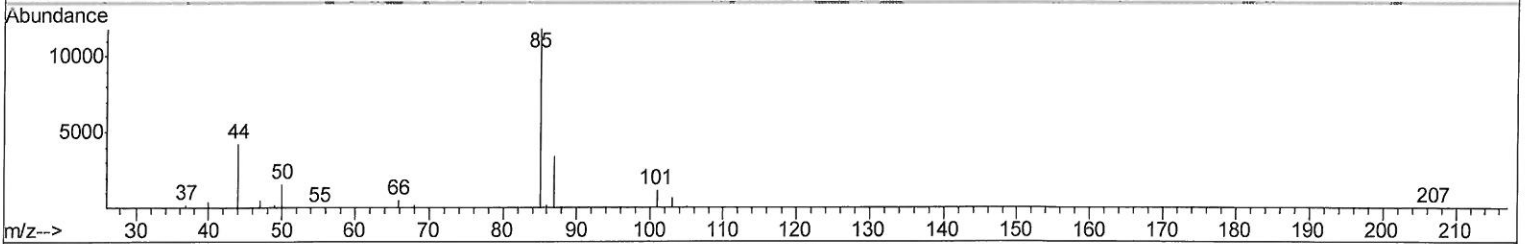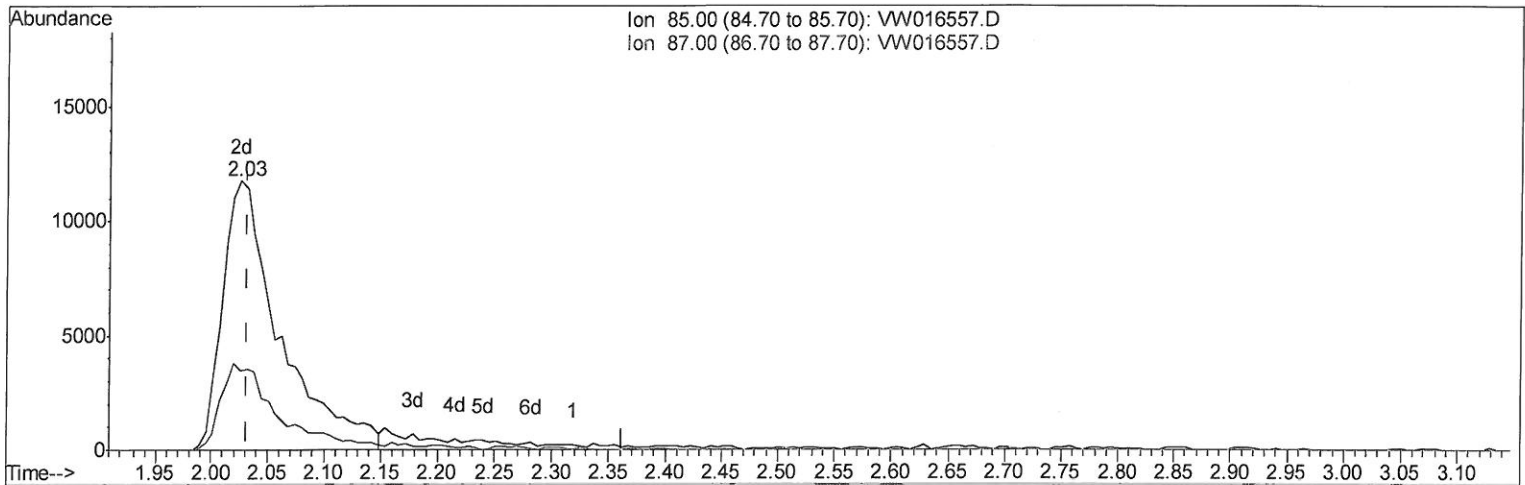

TIC: VW016557.D

(2) Dichlorodifluoromethane (T)

2.026min (-0.006) 5.80ug/L m

09/24/2024

response 41243

Ion	Exp%	Act%
85.00	100	100
87.00	31.70	0.14#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091520\
 Data File : VW016557.D
 Acq On : 15 Sep 2020 14:17
 Operator : SY/VA
 Sample : VSTD00505
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD00505

Manual Integrations
 APPROVED

MMDadoda
 9/16/2020 11:46:00 AM

Quant Time: Sep 15 15:20:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 15 15:13:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	624739	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	545019	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	270318	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	33257	5.15	ug/L	0.00
7) Chloroethane-d5	2.90	69	26926	4.79	ug/L	0.00
10) 1,1-Dichloroethene-d2	4.04	63	72672	4.94	ug/L	0.00
20) 2-Butanone-d5	7.09	46	18539	8.54	ug/L	0.00
24) Chloroform-d	7.66	84	72159	5.20	ug/L	0.00
26) 1,2-Dichloroethane-d4	8.31	65	37284	4.96	ug/L	0.00
29) Benzene-d6	8.28	84	139774	5.34	ug/L	0.00
33) 1,2-Dichloropropane-d6	9.28	67	37391	4.93	ug/L	0.00
37) Toluene-d8	10.33	98	136017	5.43	ug/L	0.00
38) trans-1,3-Dichloropropene-	10.59	79	18034	4.72	ug/L	0.00
39) 2-Hexanone-d5	10.93	63	12838	8.50	ug/L	0.00
48) 1,1,2,2-Tetrachloroethane-	12.69	84	31316	4.90	ug/L	0.00
61) 1,2-Dichlorobenzene-d4	13.85	152	50079	5.59	ug/L	0.00

Target Compounds

					Qvalue
2) Dichlorodifluoromethane	2.03	85	41243m	5.799 ug/L	98
3) Chloromethane	2.23	50	27607	4.613 ug/L	98
5) Vinyl chloride	2.37	62	43758	5.580 ug/L	97
6) Bromomethane	2.79	94	32053	5.460 ug/L	99
8) Chloroethane	2.94	64	25470	5.338 ug/L	97
9) Trichlorofluoromethane	3.28	101	40805	6.010 ug/L	99
11) 1,1,2-Trichloro-1,2,2-trif	4.09	101	42121	5.533 ug/L	97
12) 1,1-Dichloroethene	4.06	96	40984	5.356 ug/L	92
13) Acetone	4.14	43	12738	8.509 ug/L	98
14) Carbon disulfide	4.40	76	122691	5.257 ug/L	99
15) Methyl Acetate	4.68	43	15091	4.273 ug/L	98
16) Methylene chloride	4.93	84	55793	5.767 ug/L	97
17) Methyl tert-butyl Ether	5.44	73	56847	5.029 ug/L	99
18) trans-1,2-Dichloroethene	5.44	96	42132	5.200 ug/L	97
19) 1,1-Dichloroethane	6.23	63	66435	4.885 ug/L	96
21) 2-Butanone	7.18	43	23361	9.522 ug/L	85
22) cis-1,2-Dichloroethene	7.18	96	43497	5.170 ug/L	98
23) Bromochloromethane	7.52	128	21164	5.368 ug/L	95
25) Chloroform	7.68	83	74072	5.214 ug/L	98
27) 1,2-Dichloroethane	8.41	62	46617	4.969 ug/L	99
30) Cyclohexane	7.96	56	63278	5.009 ug/L	98
31) 1,1,1-Trichloroethane	7.88	97	67594	5.699 ug/L	99
32) Carbon tetrachloride	8.07	117	64464	5.703 ug/L	99
34) Benzene	8.33	78	154411	5.291 ug/L	100
35) Trichloroethene	9.10	95	44313	5.428 ug/L	99
36) Methylcyclohexane	9.34	83	75615	5.317 ug/L	99
40) 1,2-Dichloropropane	9.37	63	35385	4.963 ug/L	100
41) Bromodichloromethane	9.65	83	52232	5.181 ug/L	95
42) cis-1,3-Dichloropropene	10.08	75	59805	4.917 ug/L	99
43) 4-Methyl-2-pentanone	10.21	43	44862	9.078 ug/L	99

9/24/20 57

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091520\
 Data File : VW016557.D
 Acq On : 15 Sep 2020 14:17
 Operator : SY/VA
 Sample : VSTD00505
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD00505

Manual Integrations
 APPROVED

MMDadoda
 9/16/2020 11:46:00 AM

Quant Time: Sep 15 15:20:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 15 15:13:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) Toluene	10.40	91	175208	5.366	ug/L	98
45) trans-1,3-Dichloropropene	10.61	75	51095	4.733	ug/L	98
46) 1,1,2-Trichloroethane	10.79	97	29814	5.211	ug/L	97
47) Tetrachloroethene	10.87	164	39300	5.834	ug/L	91
49) 2-Hexanone	10.98	43	26469	7.722	ug/L	98
50) Dibromochloromethane	11.13	129	37310	5.111	ug/L	95
51) 1,2-Dibromoethane	11.24	107	29933	5.236	ug/L	99
52) Chlorobenzene	11.66	112	116321	5.545	ug/L	99
53) Ethylbenzene	11.74	91	196126	5.317	ug/L	100
54) m,p-Xylene	11.84	106	76322	5.377	ug/L	98
55) o-xylene	12.17	106	72638	5.371	ug/L	98
56) Styrene	12.18	104	120597	5.220	ug/L	100
57) Isopropylbenzene	12.47	105	199635	5.372	ug/L	99
58) 1,1,2,2-Tetrachloroethane	12.72	83	32358	4.781	ug/L	96
59) 1,2,3-Trichloropropane	12.77	75	24328	4.811	ug/L	99
62) Bromoform	12.35	173	22242	4.939	ug/L	99
63) 1,3-Dichlorobenzene	13.50	146	90846	5.338	ug/L	96
64) 1,4-Dichlorobenzene	13.58	146	91446	5.442	ug/L	99
65) 1,2-Dichlorobenzene	13.87	146	83790	5.554	ug/L	99
66) 1,2-Dibromo-3-chloropropan	14.49	75	5643	4.163	ug/L	91
67) 1,3,5-Trichlorobenzene	14.63	180	65976	5.528	ug/L	97
68) 1,2,4-trichlorobenzene	15.14	180	52480	5.085	ug/L	98
69) Naphthalene	15.37	128	84974	4.064	ug/L	99
70) 1,2,3-Trichlorobenzene	15.56	180	44130	4.985	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

(QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091520\
Data File : VW016557.D
Acq On : 15 Sep 2020 14:17
Operator : SY/VA
Sample : VSTD00505
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD00505

Manual Integrations

MMDadoda
9/16/2020 11:46:00 AM

Quant Time: Sep 15 15:20:19 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 15 15:13:12 2020
Response via : Initial Calibration

