

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW091520\
 Data File : VW016563.D
 Acq On : 15 Sep 2020 19:12
 Operator : SY/VA
 Sample : L4024-01
 Misc : 5.45G/10ML/MSVOA W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3H1

Manual Integrations
 APPROVED

MMDadoda
 9/16/2020 11:46:02 AM

Quant Time: Sep 16 04:53:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 16 04:36:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	691114	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	603832	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	284595	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	174401	26.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.28%
7) Chloroethane-d5	2.90	69	141792	25.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.84%
10) 1,1-Dichloroethene-d2	4.03	63	277390	18.55	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.20%
20) 2-Butanone-d5	7.09	46	64380	35.30	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.60%
24) Chloroform-d	7.65	84	356566	24.66	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.64%
26) 1,2-Dichloroethane-d4	8.31	65	178604	24.07	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.28%
29) Benzene-d6	8.28	84	712055	26.29	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.16%
33) 1,2-Dichloropropane-d6	9.28	67	190924	26.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.08%
37) Toluene-d8	10.33	98	687204	25.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.16%
38) trans-1,3-Dichloropropene-	10.58	79	86483	23.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.52%
39) 2-Hexanone-d5	10.93	63	53618	40.17	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.34%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	129392	20.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.88%
61) 1,2-Dichlorobenzene-d4	13.86	152	237808	26.15	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.60%

Target Compounds				Ovalue
13) Acetone	4.14	43	3356m	2.349 ug/L
16) Methylene chloride	4.93	84	15420m	1.447 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW091520\
Data File : VW016563.D
Acq On : 15 Sep 2020 19:12
Operator : SY/VA
Sample : L4024-01
Misc : 5.45G/10ML/MSVOA W/SOIL
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BG3H1

Manual Integrations
APPROVED

MMDadoda
9/16/2020 11:46:02 AM

Quant Time: Sep 16 04:53:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 16 04:36:48 2020
Response via : Initial Calibration

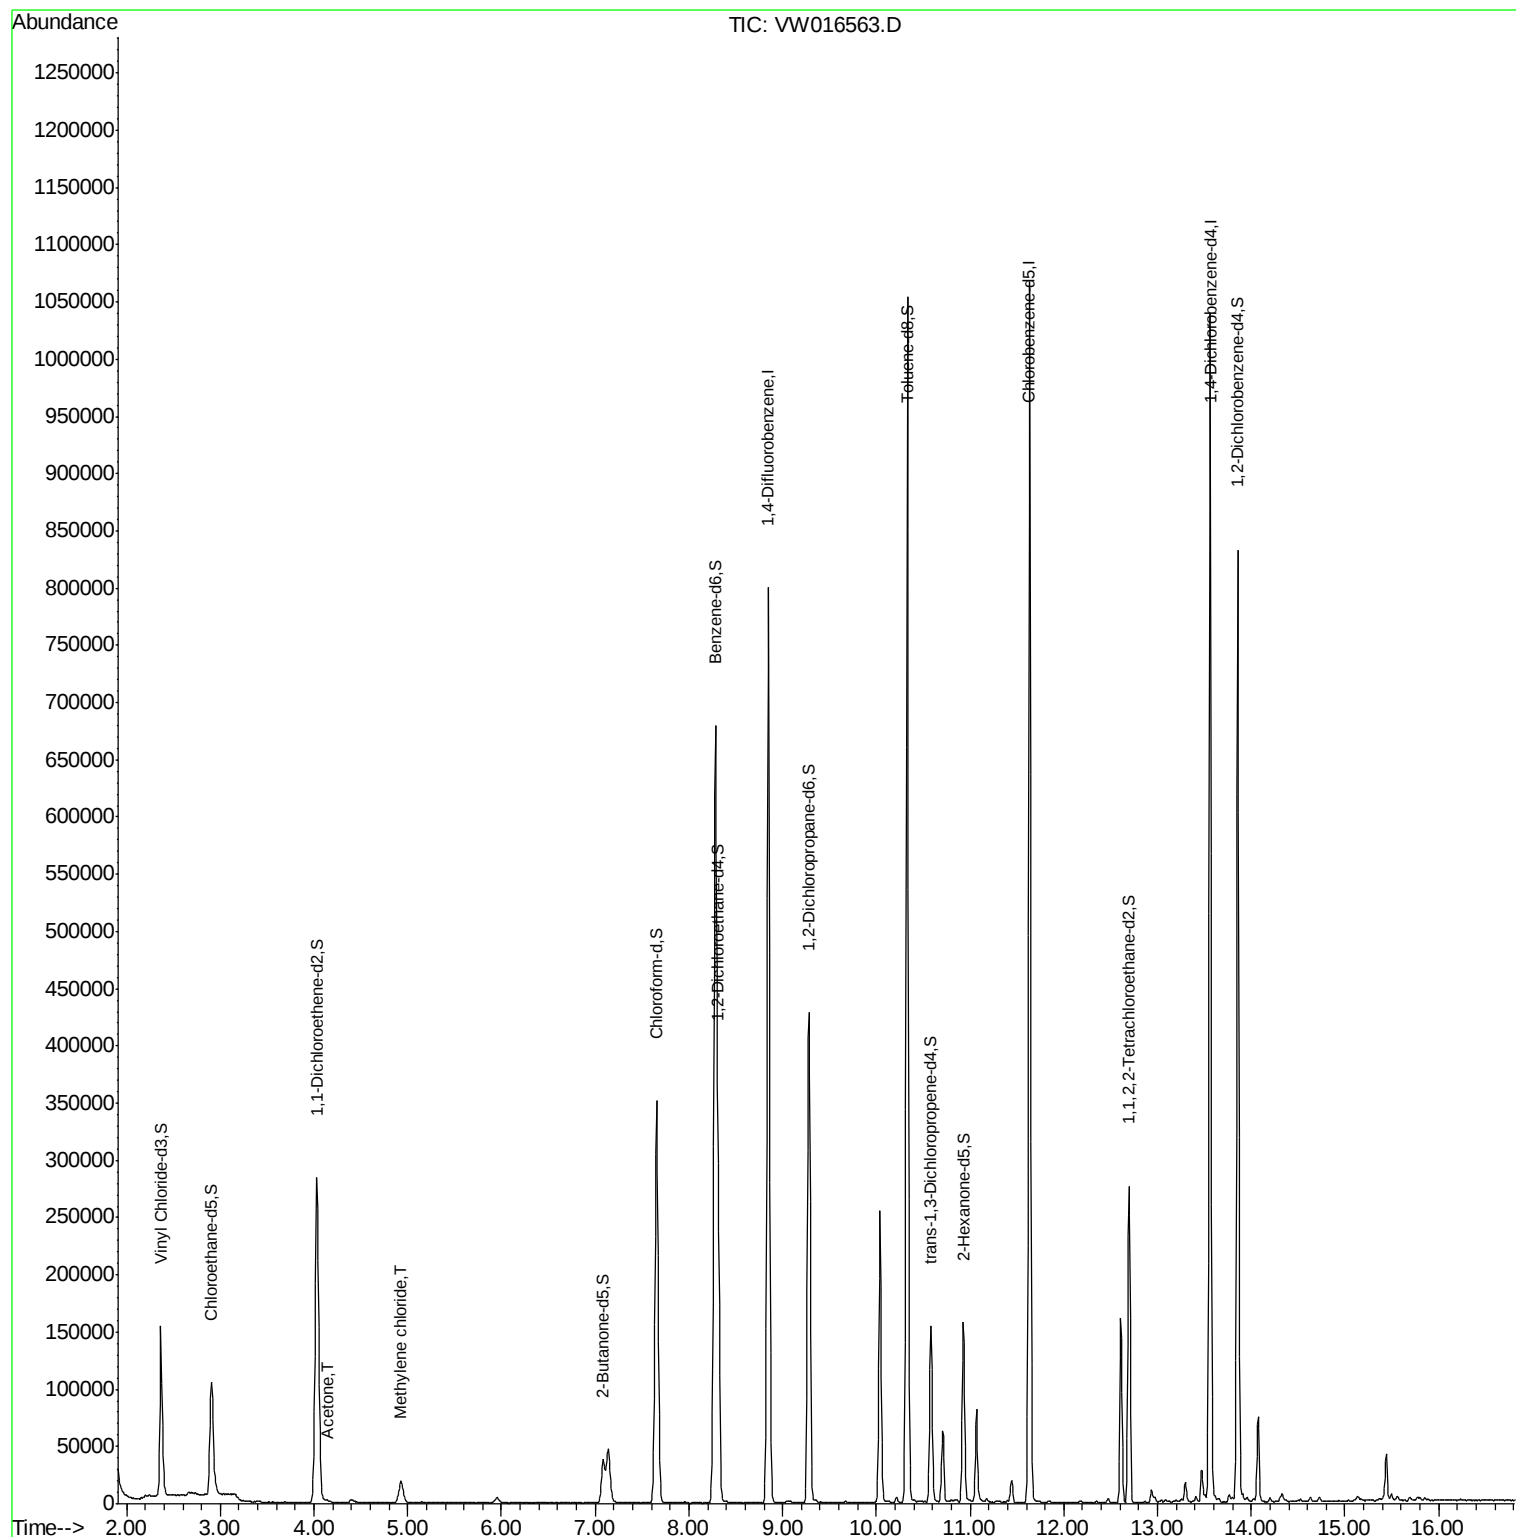

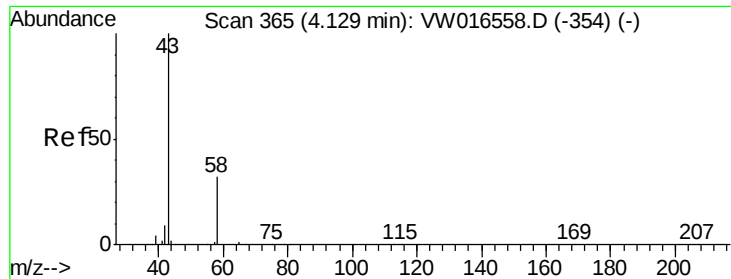

#13

Acetone

Concen: 2.349 ug/L m

RT: 4.14 min Scan# 367

Delta R.T. 0.01 min

Lab File: VW016563.D

Acq: 15 Sep 2020 19:12

Instrument :

MSVOA_W

ClientSampled :

BG3H1

Tot Ion: 43 Resp: 3356

Ion Ratio Lower Upper

43 100





58 12.2 0.0 60.2

Manual Integrations

APPROVED

MMDadoda

9/16/2020 11:46:02 AM

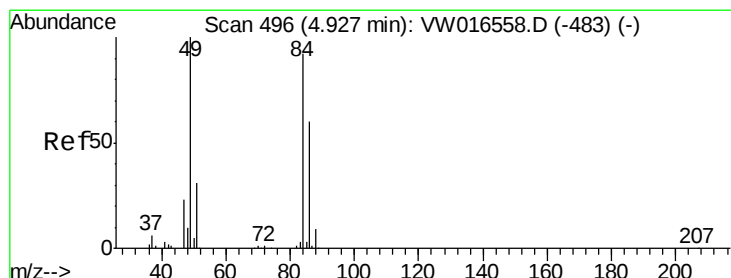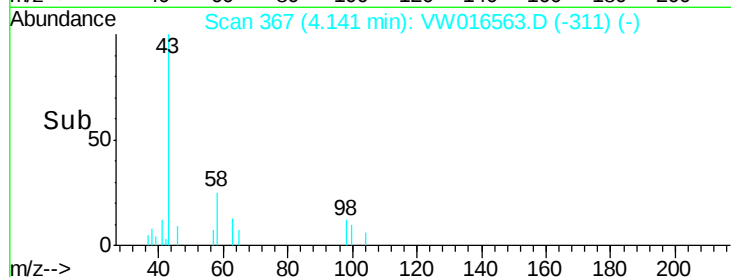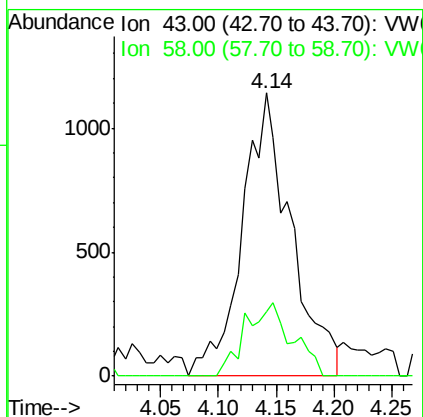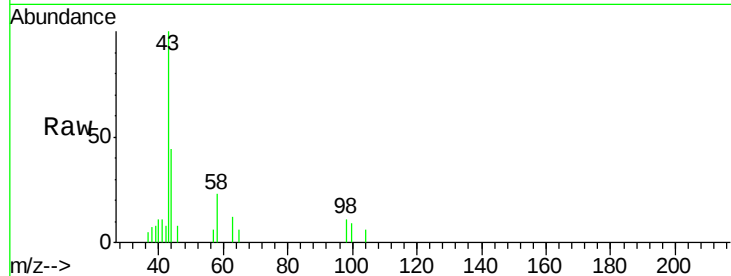

#16

Methylene chloride

Concen: 1.447 ug/L m

RT: 4.93 min Scan# 496

Delta R.T. 0.00 min

Lab File: VW016563.D

Acq: 15 Sep 2020 19:12

Tgt Ion: 84 Resp: 15420

Ion Ratio Lower Upper

84 100

49 120.5 76.0 141.2

86 74.2 45.6 84.6

