


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW091520\
 Data File : VW016555.D
 Acq On : 15 Sep 2020 12:54
 Operator : SY/VA
 Sample : BFB25
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB25

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Title : VOC Analysis
 Last Update : Wed Sep 16 08:47:42 2020

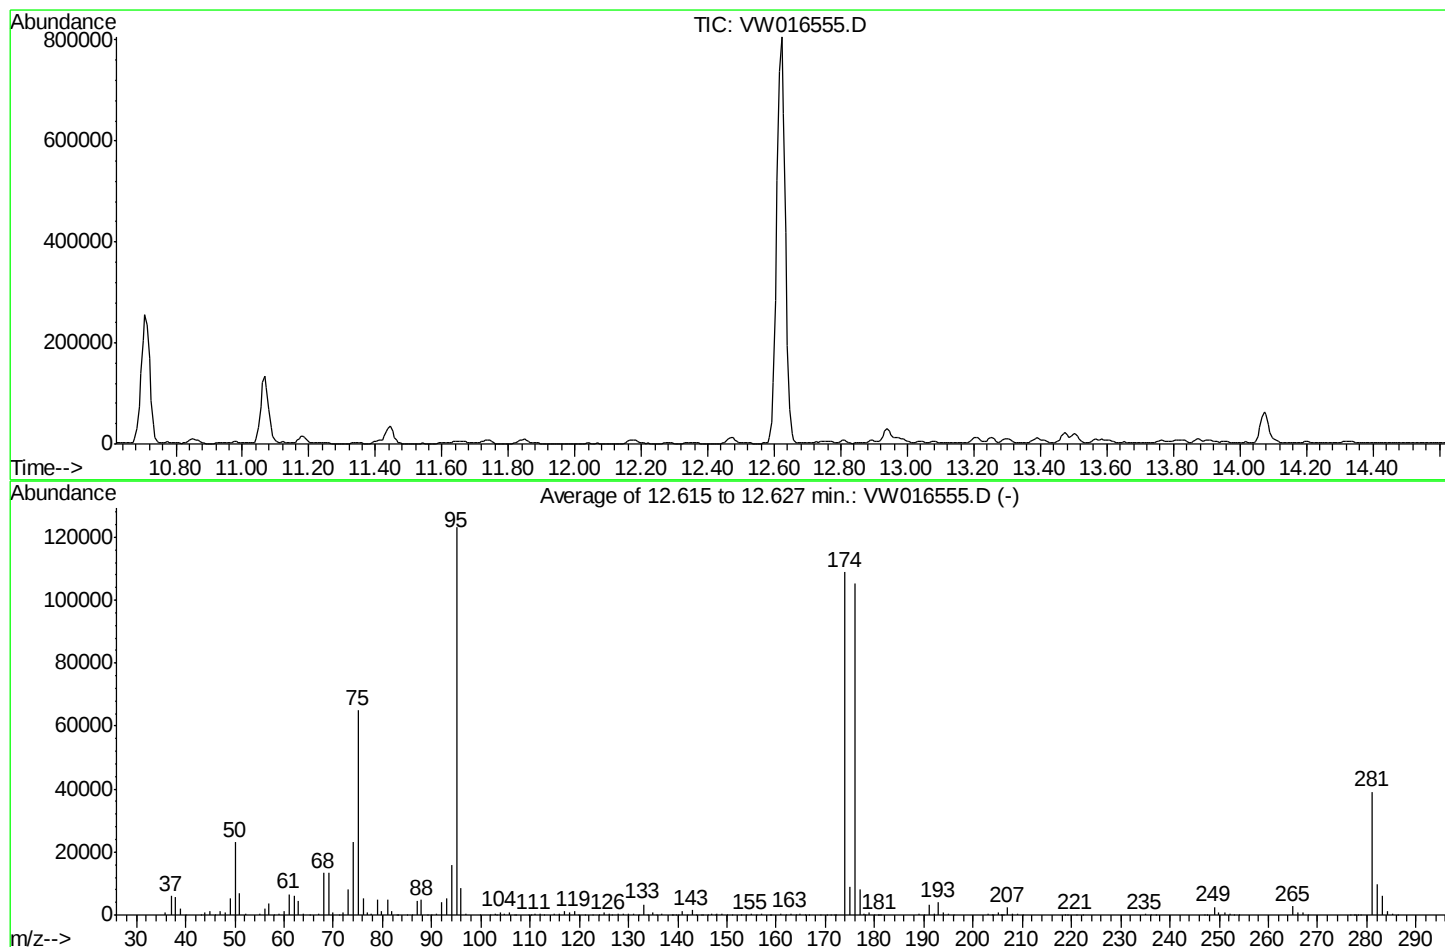

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	23010	PASS
75	95	30	80	52.7	64885	PASS
95	95	100	100	100.0	123149	PASS
96	95	5	9	6.9	8505	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.5	108936	PASS
175	174	5	9	8.2	8933	PASS
176	174	95	101	96.9	105509	PASS
177	176	5	9	7.6	7966	PASS

m/z	Abundance
35.90	1004.0
37.00	6008.0
38.00	5679.0
39.00	2179.0
40.00	201.0
40.90	152.0
43.00	392.0
44.00	1204.0
45.00	1706.0
46.10	223.0
47.00	1189.0
48.10	719.0
49.00	5685.0
50.00	22856.0
51.00	7308.0
52.10	316.0
55.00	314.0
56.00	2314.0
57.00	3709.0
58.00	231.0
59.00	826.0
60.00	1343.0
61.00	6664.0
62.00	6280.0
63.00	4779.0
64.00	482.0
65.10	138.0
67.00	356.0
68.00	13360.0
69.00	13214.0
70.00	1084.0
71.20	115.0
72.00	864.0
73.00	10375.0
74.00	21976.0
75.00	63096.0
76.10	5491.0
76.90	904.0
77.80	371.0
78.90	4872.0
79.90	1479.0
81.00	5042.0
81.90	1061.0
83.00	183.0
84.90	144.0
85.90	107.0
87.00	4757.0
87.90	4507.0
89.10	190.0
90.00	60.0
90.90	540.0
92.00	3920.0
93.00	5336.0
94.00	14795.0
95.00	120088.0
96.00	8263.0
96.90	245.0
102.00	168.0
102.90	788.0
103.90	866.0
104.80	363.0
105.90	572.0
106.80	151.0
110.10	315.0
111.00	645.0
112.00	273.0
112.90	240.0
115.00	435.0
116.00	629.0
116.80	1057.0
117.90	991.0
119.00	1430.0
119.90	237.0
121.10	149.0
123.90	123.0
124.90	1481.0
126.00	606.0
126.70	110.0
127.90	594.0
128.90	215.0
129.80	432.0
131.10	257.0
132.00	168.0
133.00	5489.0
135.00	706.0
135.80	64.0
136.90	296.0
140.00	75.0
140.90	1282.0
141.90	174.0
142.90	1360.0
143.80	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

144.90	245.0
146.00	225.0
146.90	744.0
148.00	401.0
149.00	348.0
150.00	174.0
151.10	58.0
152.90	96.0
154.00	97.0
154.90	363.0
157.00	239.0
158.80	303.0
160.90	394.0
161.80	117.0
163.00	984.0
164.00	206.0
164.90	690.0
165.90	133.0
166.70	85.0
168.90	88.0
171.10	116.0
171.80	312.0
174.00	90792.0
175.00	8279.0
175.90	82488.0
176.90	8185.0
177.90	710.0
179.00	1099.0
180.00	197.0
181.00	142.0
189.00	436.0
191.00	5007.0
192.10	1044.0
193.00	5710.0
194.00	943.0
195.00	702.0
196.00	86.0
203.00	664.0
203.80	168.0
205.00	1262.0
206.00	377.0
207.00	3507.0
208.10	807.0
208.90	366.0
219.00	142.0
220.90	304.0
222.20	86.0
235.00	614.0
236.00	179.0
237.00	111.0
247.00	118.0
249.00	3406.0
249.90	909.0
251.10	1640.0
252.10	432.0
253.10	309.0
254.00	55.0
265.00	3727.0
266.10	1032.0
267.00	882.0
268.20	158.0
277.30	112.0
278.20	136.0
278.70	154.0
281.10	64088.0
282.10	14792.0
283.10	8271.0
284.10	1707.0
285.10	678.0
286.20	112.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

m/z	Abundance
36.00	1075.0
37.00	6960.0
38.00	6261.0
39.00	2484.0
39.90	219.0
40.90	82.0
41.80	65.0
43.00	198.0
44.00	1641.0
45.00	1575.0
46.00	184.0
47.10	1497.0
48.00	943.0
49.00	5662.0
50.00	25344.0
51.00	7713.0
52.10	376.0
55.00	565.0
56.00	2435.0
57.00	4447.0
58.00	255.0
59.00	459.0
60.00	1625.0
61.00	7475.0
62.00	6872.0
63.00	5113.0
63.90	531.0
65.10	158.0
67.00	646.0
68.00	14928.0
69.00	14711.0
70.00	1182.0
71.30	174.0
71.90	844.0
73.00	8005.0
74.00	25664.0
75.00	71792.0
76.00	5990.0
77.00	828.0
77.80	581.0
78.90	4944.0
79.90	1587.0
80.90	5323.0
81.90	1235.0
83.00	220.0
87.00	4949.0
88.00	5247.0
90.90	715.0
92.00	4375.0
93.00	5864.0
94.00	17896.0
95.00	136384.0
96.00	9423.0
97.00	256.0
99.80	57.0
102.80	577.0
103.20	402.0
103.90	1017.0
104.90	399.0
105.90	639.0
107.00	172.0
110.10	244.0
110.80	332.0
112.00	204.0
112.90	164.0
114.80	319.0
115.90	605.0
116.90	1155.0
118.00	1000.0
118.90	1403.0
119.90	81.0
120.90	178.0
122.80	76.0
123.90	118.0
125.00	790.0
125.90	156.0
127.90	539.0
128.90	282.0
129.90	667.0
131.00	354.0
132.00	130.0
133.00	2917.0
133.90	619.0
134.90	814.0
136.90	282.0
138.80	122.0
140.00	59.0
140.90	1387.0
142.00	185.0
142.90	1713.0
143.90	91.0
145.10	198.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

146.00	155.0
146.90	473.0
147.90	399.0
149.00	237.0
149.90	144.0
150.90	67.0
152.70	105.0
153.80	106.0
155.00	404.0
156.10	67.0
156.90	249.0
159.00	224.0
160.90	380.0
161.90	86.0
163.00	518.0
164.00	174.0
164.80	280.0
165.90	140.0
172.00	361.0
173.90	128520.0
175.00	10005.0
175.90	117864.0
177.00	7856.0
178.10	379.0
178.90	842.0
180.00	178.0
180.60	53.0
181.20	56.0
189.00	384.0
190.00	167.0
191.00	2925.0
192.00	556.0
193.00	4249.0
194.10	673.0
195.00	511.0
203.00	349.0
204.00	107.0
205.00	588.0
205.70	130.0
206.20	223.0
207.10	2548.0
208.00	485.0
209.00	339.0
210.10	57.0
218.70	64.0
219.10	87.0
221.00	128.0
222.20	85.0
235.00	314.0
236.10	105.0
237.10	71.0
247.40	68.0
249.00	2564.0
249.90	945.0
251.10	841.0
252.10	295.0
253.10	169.0
265.00	3260.0
266.10	845.0
267.00	788.0
268.00	151.0
276.70	53.0
277.70	55.0
278.30	120.0
278.80	248.0
281.10	35848.0
282.10	9577.0
283.00	6074.0
284.10	1739.0
285.10	572.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

m/z	Abundance
36.00	1007.0
37.00	5120.0
38.00	4946.0
39.00	1730.0
39.90	245.0
41.00	85.0
41.90	70.0
42.90	123.0
44.00	1033.0
45.00	1070.0
46.00	87.0
47.00	1116.0
48.00	750.0
49.10	4951.0
50.00	20832.0
51.00	5999.0
52.10	357.0
55.10	420.0
56.00	1983.0
57.00	3643.0
58.00	125.0
59.10	196.0
60.00	1188.0
61.00	5887.0
62.00	5217.0
63.00	4082.0
64.00	323.0
67.10	351.0
68.00	11443.0
69.00	12367.0
70.00	771.0
71.10	88.0
71.90	622.0
73.00	6570.0
74.00	21736.0
75.00	59768.0
76.00	4897.0
77.00	718.0
77.80	339.0
78.90	4499.0
79.90	1170.0
80.90	4483.0
81.90	969.0
83.20	166.0
86.00	105.0
87.00	4282.0
88.00	4581.0
90.90	476.0
92.00	3762.0
93.00	5128.0
94.00	14394.0
95.00	112976.0
96.00	7830.0
97.10	356.0
99.80	52.0
102.80	282.0
104.00	842.0
104.80	328.0
105.90	671.0
107.10	119.0
109.80	142.0
111.00	168.0
111.80	215.0
112.80	148.0
114.90	227.0
115.90	564.0
117.00	973.0
117.90	678.0
119.00	771.0
119.90	82.0
120.90	83.0
122.80	65.0
124.00	77.0
124.90	257.0
125.80	126.0
127.90	493.0
128.90	212.0
129.90	384.0
131.00	308.0
133.00	1890.0
134.90	414.0
135.80	55.0
136.80	351.0
139.00	56.0
139.70	100.0
140.00	93.0
140.90	1434.0
142.90	1563.0
143.90	94.0
145.00	114.0
146.00	204.0
146.90	273.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

147.70	304.0
148.10	242.0
148.90	183.0
150.00	164.0
152.80	85.0
153.80	94.0
154.80	360.0
156.00	71.0
156.90	230.0
158.90	284.0
161.00	322.0
162.90	325.0
163.80	77.0
164.90	201.0
165.80	71.0
169.00	53.0
170.30	141.0
172.00	292.0
173.90	107496.0
175.00	8516.0
176.00	116176.0
177.00	7858.0
177.90	301.0
179.00	424.0
179.90	84.0
189.10	132.0
191.00	1582.0
193.00	2084.0
193.90	476.0
195.10	254.0
203.00	247.0
205.10	357.0
205.80	140.0
207.10	1280.0
207.90	216.0
208.90	130.0
219.00	70.0
235.00	129.0
249.00	1357.0
250.00	363.0
250.90	442.0
252.20	103.0
253.20	64.0
265.10	1316.0
266.00	399.0
267.00	357.0
278.90	97.0
281.00	17360.0
282.00	4644.0
283.10	3708.0
284.10	587.0
285.00	243.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

Scan 1749 (12.567 min): VW016555.D
BFB25

m/z	Abundance
39.90	191.0
41.00	117.0
42.00	88.0
43.20	141.0
44.00	487.0
45.20	103.0
55.10	87.0
57.00	119.0
98.00	52.0
207.10	100.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25