



Dichlorodifluoromethane

Response Ratio

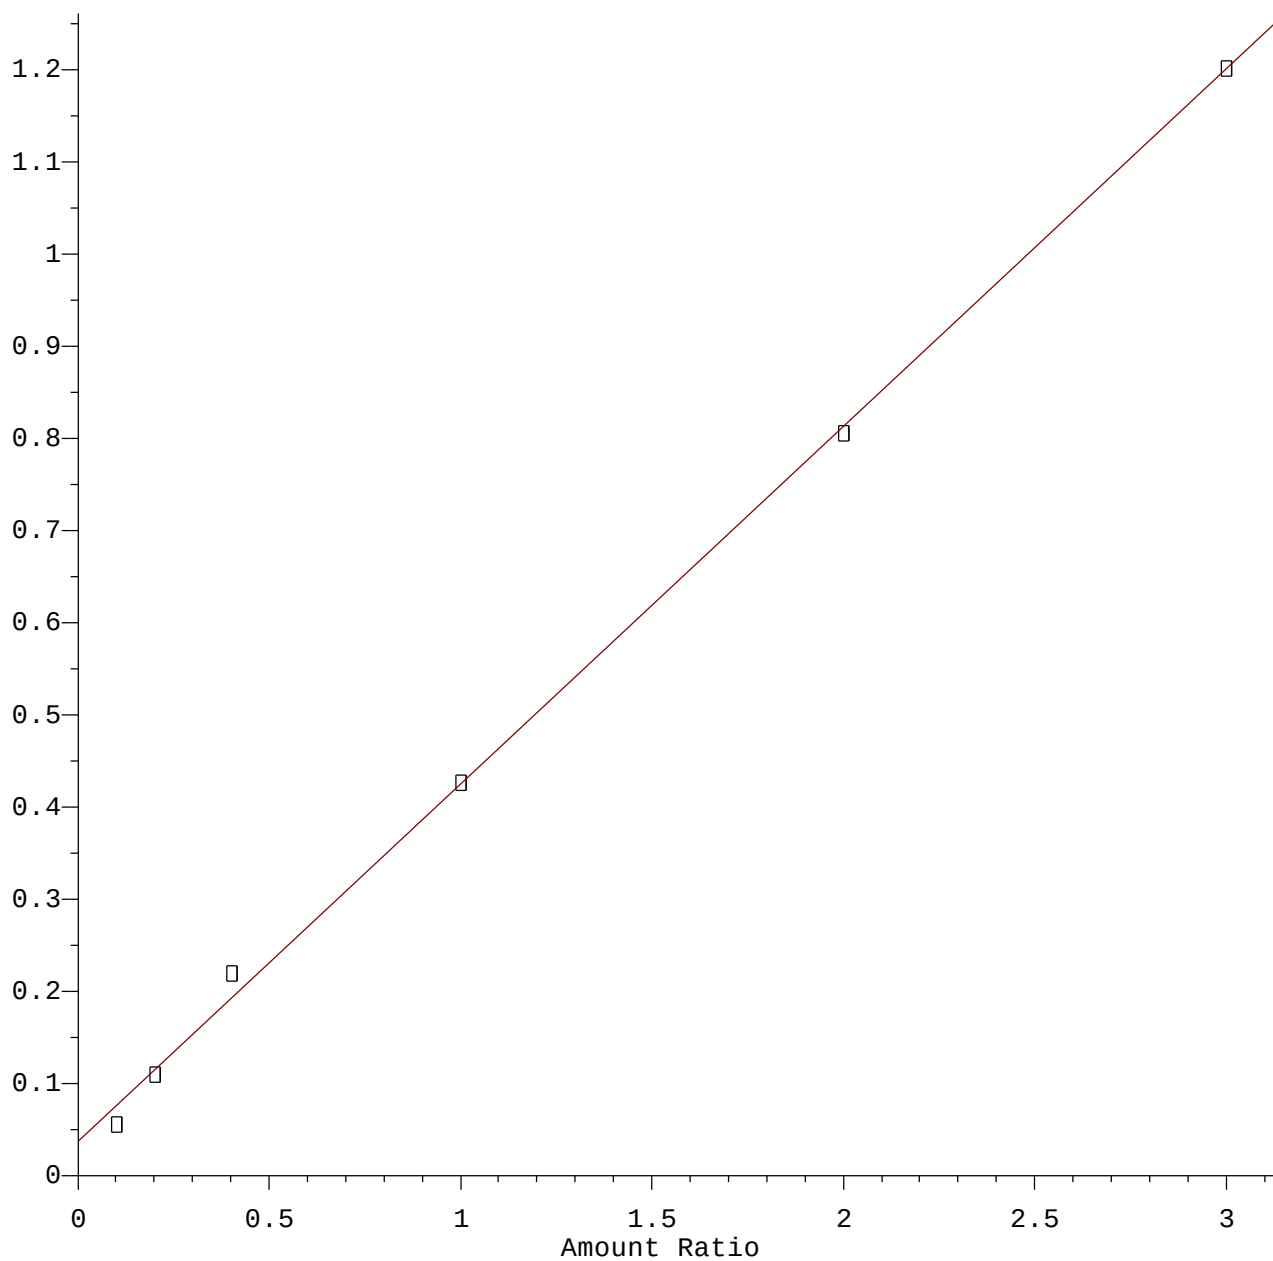


Resp Ratio = $3.88 \times 10^{-1} \times \text{Amt} + 3.67 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
Calibration Table Last Updated: Tue Sep 18 16:07:21 2018

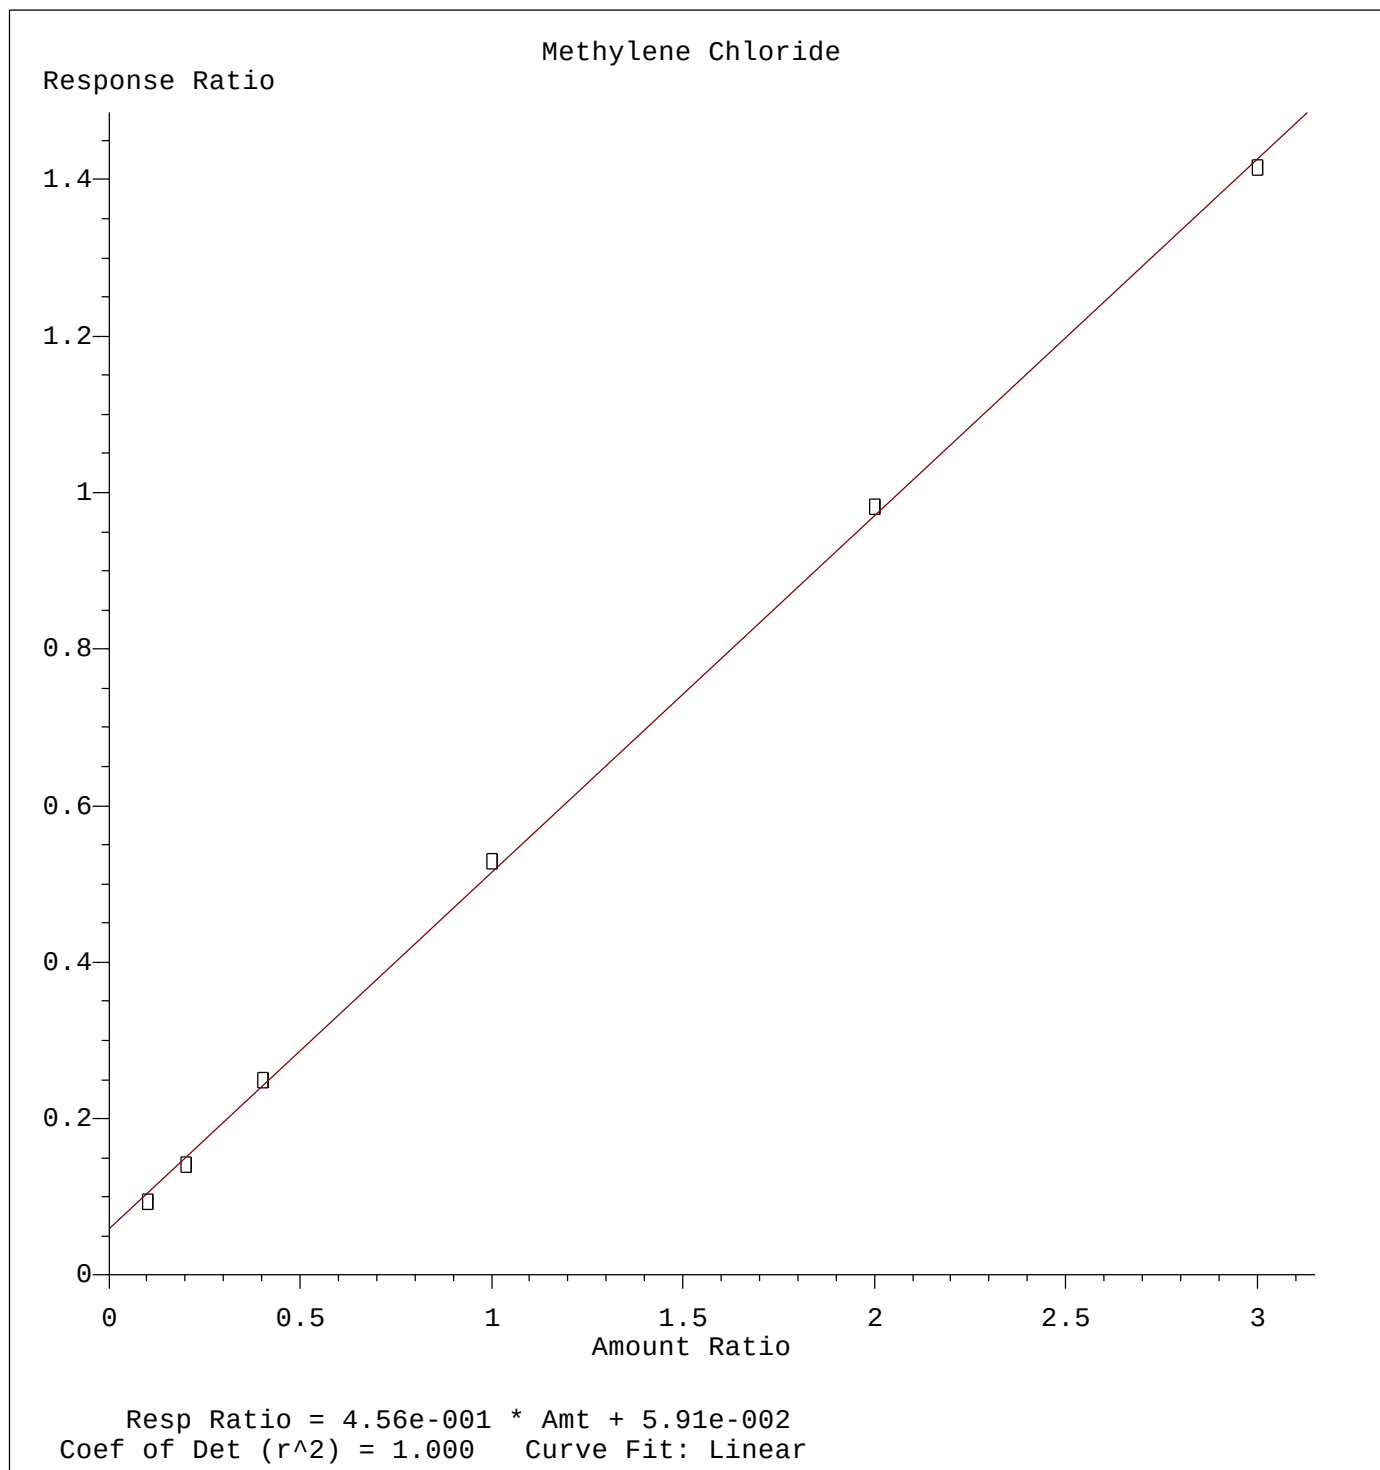


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
Calibration Table Last Updated: Tue Sep 18 16:07:21 2018

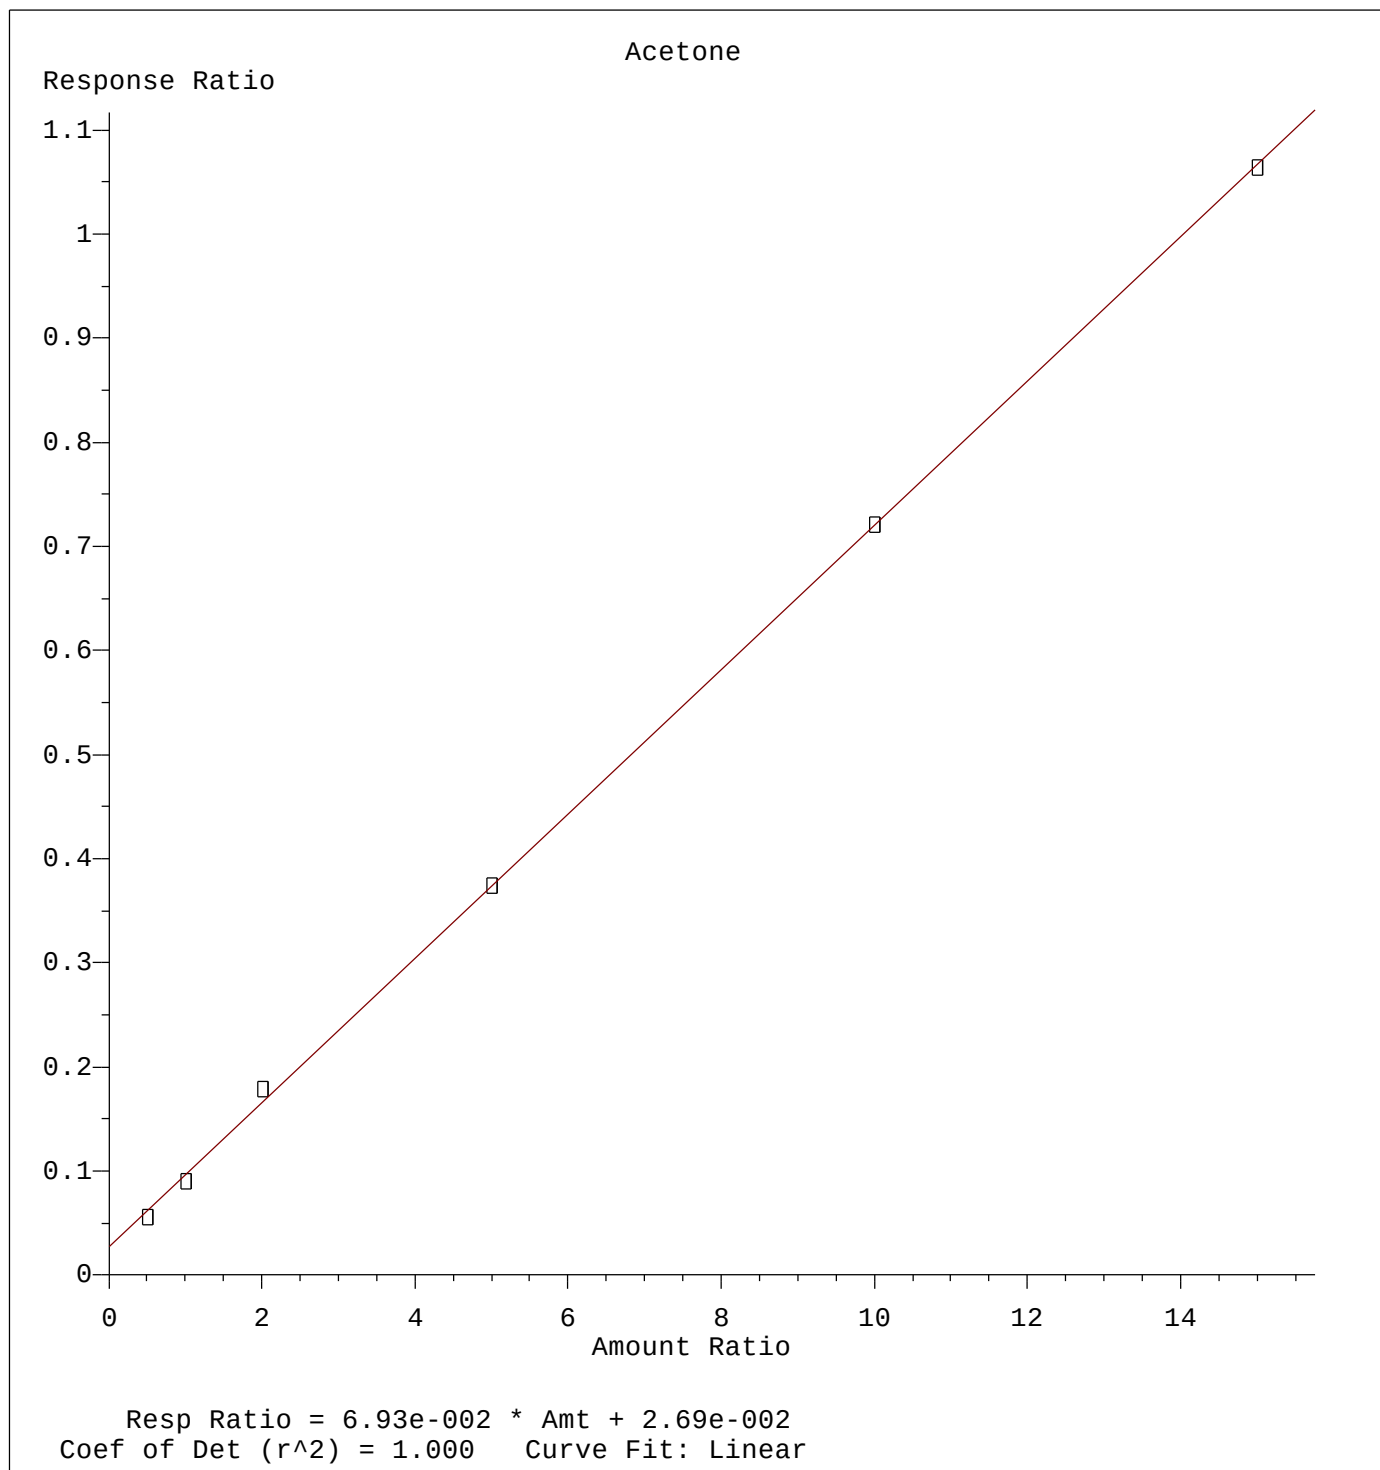


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
Calibration Table Last Updated: Tue Sep 18 16:07:21 2018

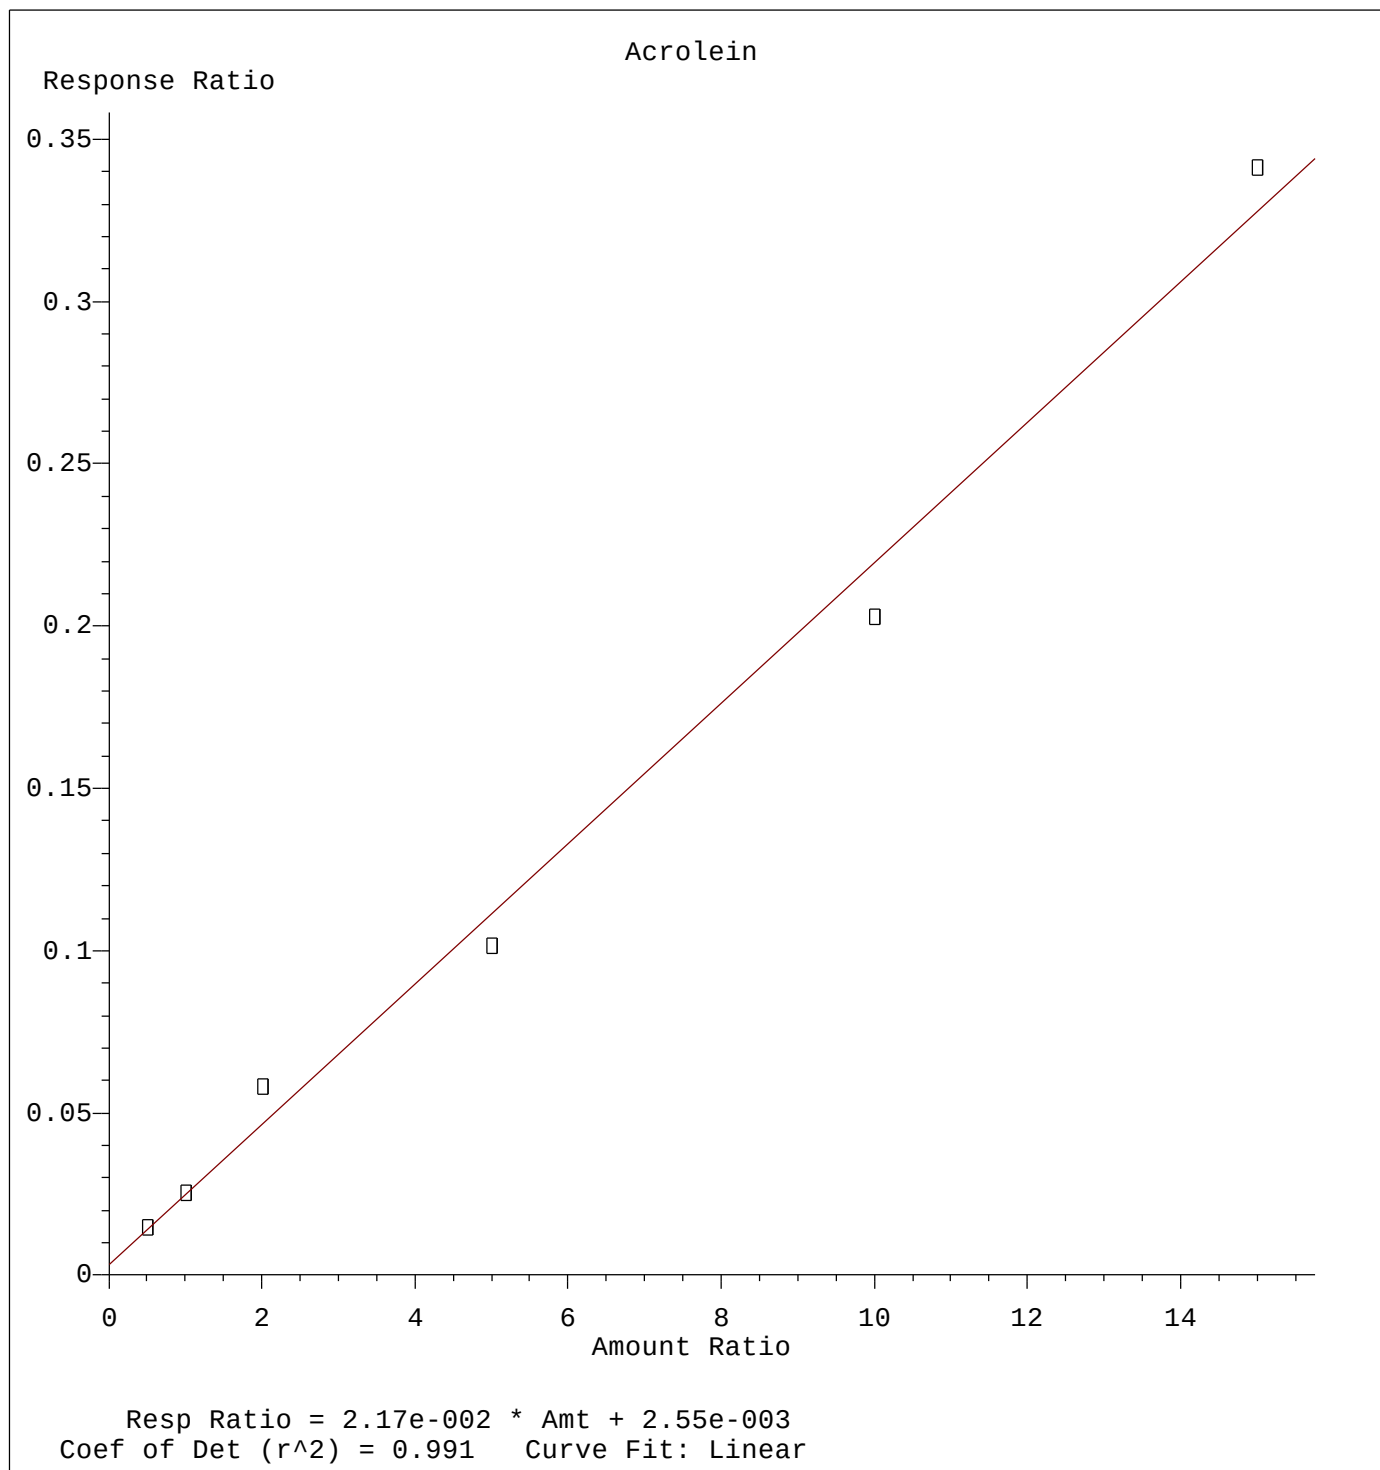


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
Calibration Table Last Updated: Tue Sep 18 16:07:21 2018

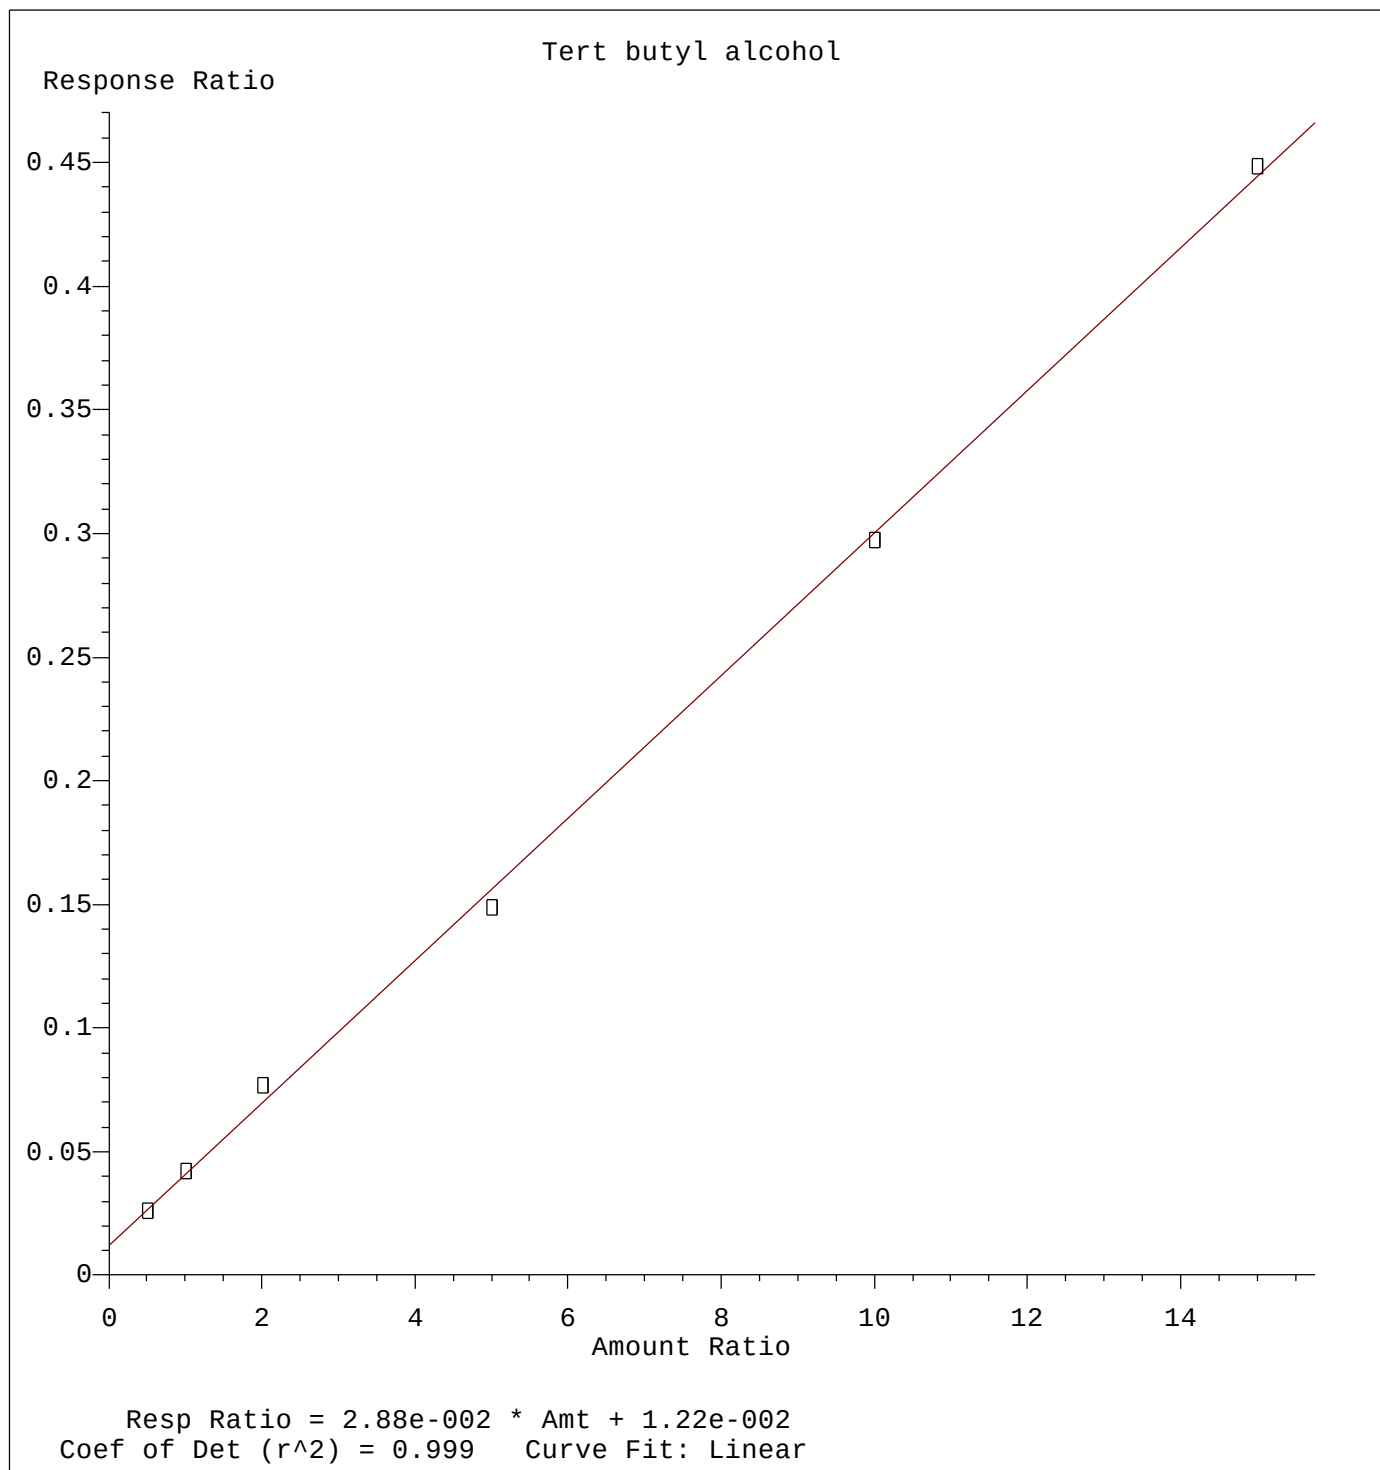

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
Calibration Table Last Updated: Tue Sep 18 16:07:21 2018

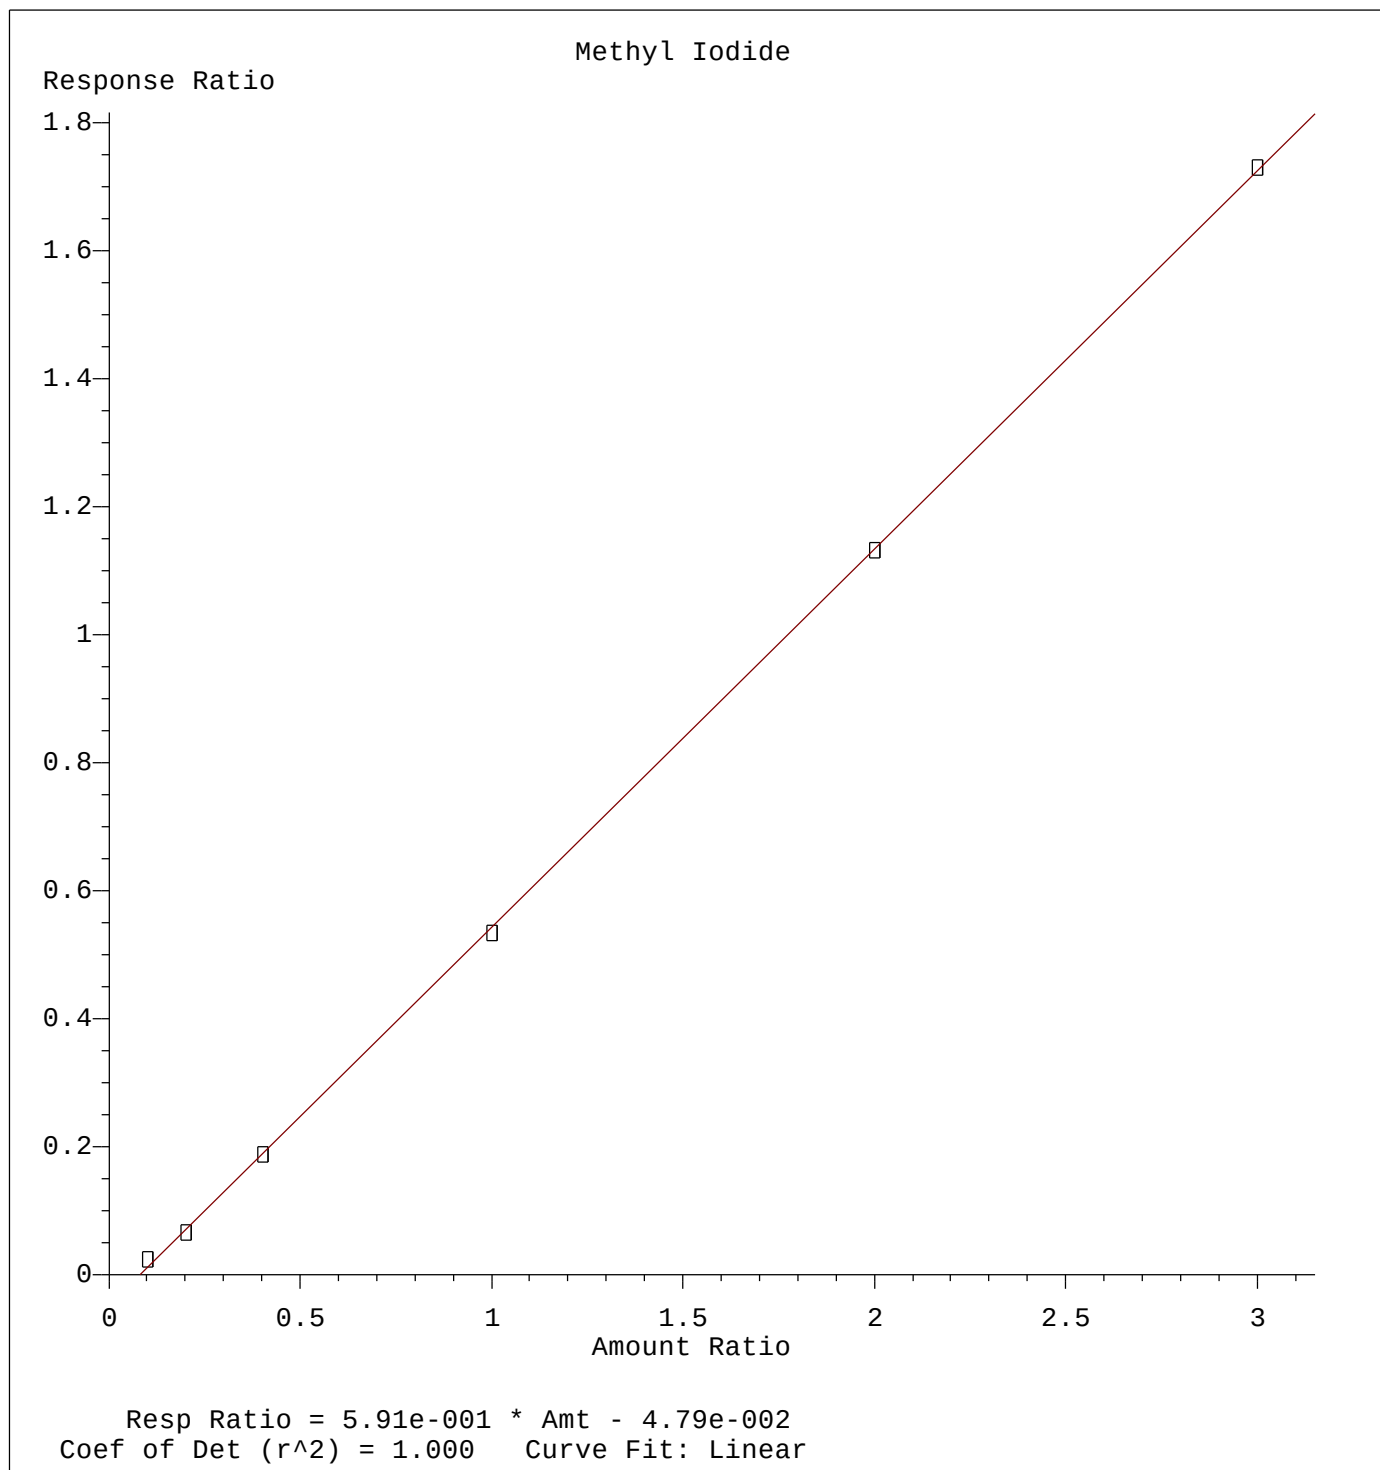

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
Calibration Table Last Updated: Tue Sep 18 16:07:21 2018

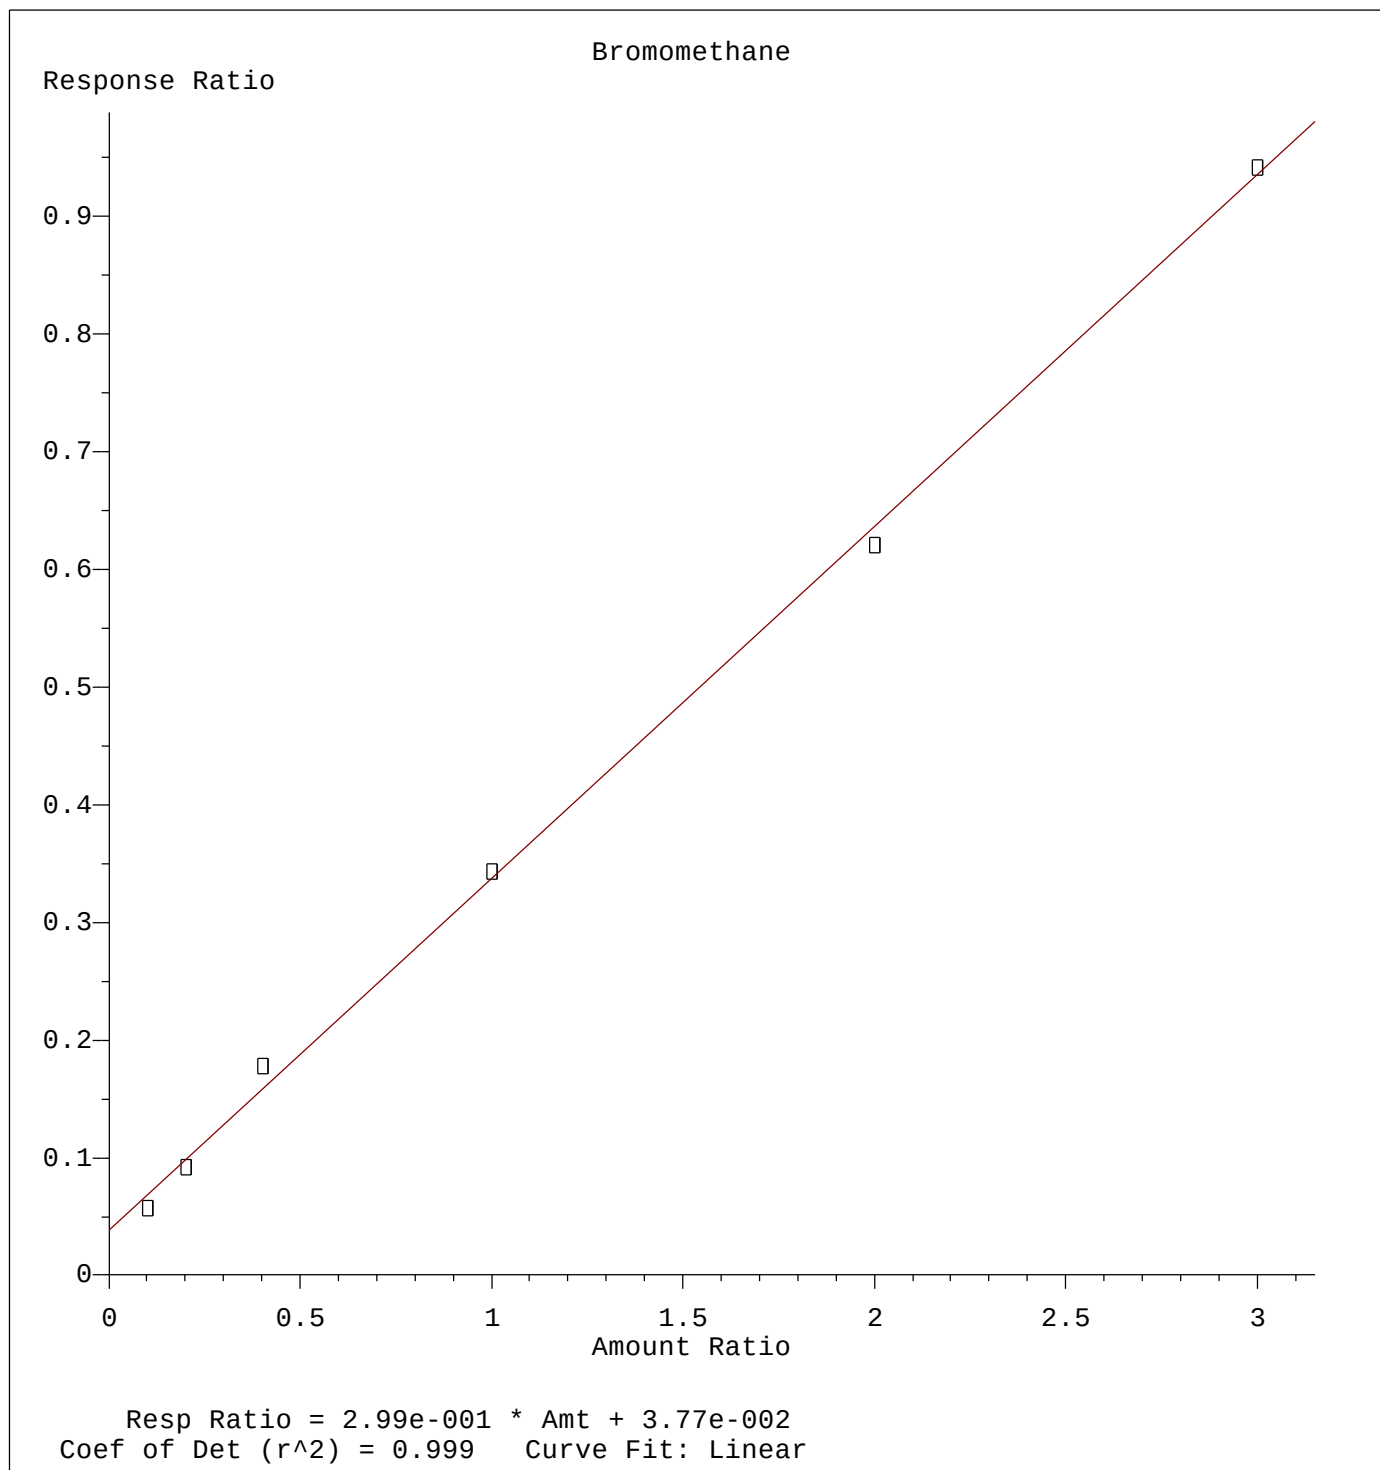

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
Calibration Table Last Updated: Tue Sep 18 16:07:21 2018