


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW091619\
 Data File : VW013055.D
 Acq On : 16 Sep 2019 21:34
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
 Title : SW846 8260
 Last Update : Fri Sep 13 17:26:01 2019

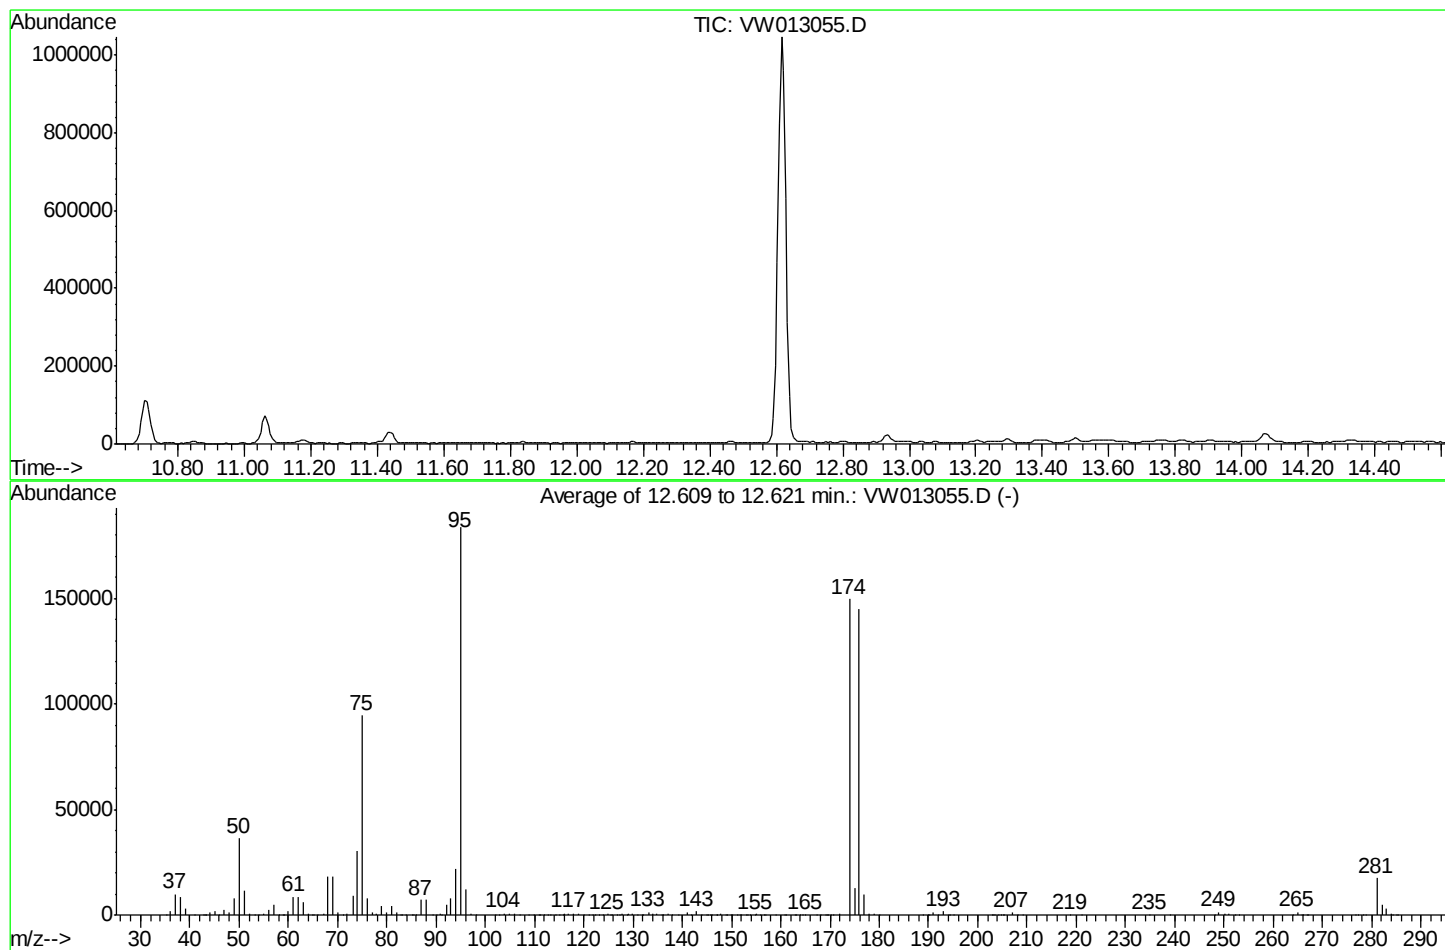

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	36298	PASS
75	95	30	60	51.5	94566	PASS
95	95	100	100	100.0	183752	PASS
96	95	5	9	6.7	12298	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.6	149856	PASS
175	174	5	9	8.7	13019	PASS
176	174	95	101	96.7	144968	PASS
177	176	5	9	6.9	9974	PASS