

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091621\
 Data File : VW020037.D
 Acq On : 16 Sep 2021 11:05
 Operator : SY/VA
 Sample : VW0916SBL07
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 VBLK434

Manual Integrations
 APPROVED

MMDadoda
 9/17/2021 4:38:41 PM

Quant Time: Sep 16 14:40:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 16 00:47:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	250738	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	243469	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	111158	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	116029	28.095	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 112.400%			
7) Chloroethane-d5	2.898	69	91635	25.779	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 103.120%			
11) 1,1-Dichloroethene-d2	4.025	63	129848	19.236	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 76.960%			
21) 2-Butanone-d5	7.080	46	49956	44.218	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 88.440%			
24) Chloroform-d	7.653	84	185763	26.888	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 107.560%			
26) 1,2-Dichloroethane-d4	8.311	65	112666	27.682	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 110.720%			
32) Benzene-d6	8.281	84	356675	26.851	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 107.400%			
36) 1,2-Dichloropropane-d6	9.281	67	106718	27.085	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 108.360%			
41) Toluene-d8	10.329	98	319896	25.691	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 102.760%			
43) trans-1,3-Dichloroprop...	10.579	79	46593	25.708	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 102.840%			
47) 2-Hexanone-d5	10.927	63	35612	44.243	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 88.480%			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	96039	24.777	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 99.120%			
66) 1,2-Dichlorobenzene-d4	13.853	152	110807	29.251	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 117.000%			
Target Compounds					Qvalue	
42) Toluene	10.390	91	5195	0.332	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091621\
 Data File : VW020037.D
 Acq On : 16 Sep 2021 11:05
 Operator : SY/VA
 Sample : VW0916SBL07
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK434

Manual Integrations
 APPROVED

MMDadoda
 9/17/2021 4:38:41 PM

Quant Time: Sep 16 14:40:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 16 00:47:26 2021
 Response via : Initial Calibration

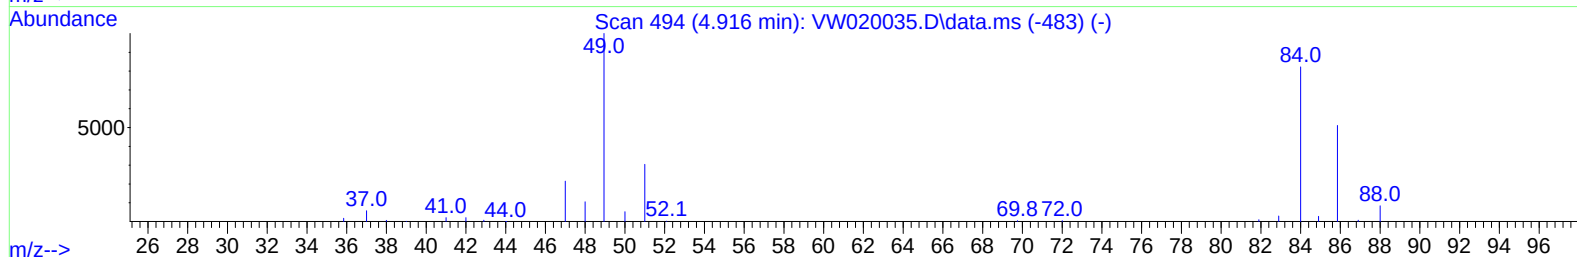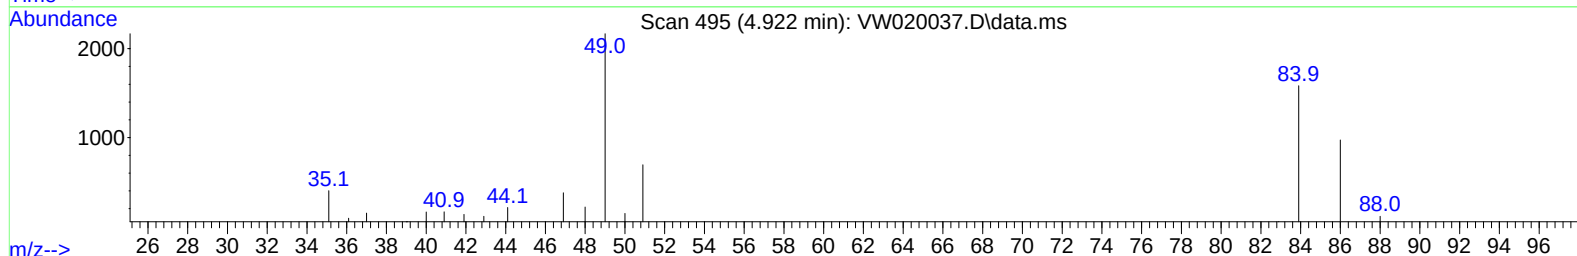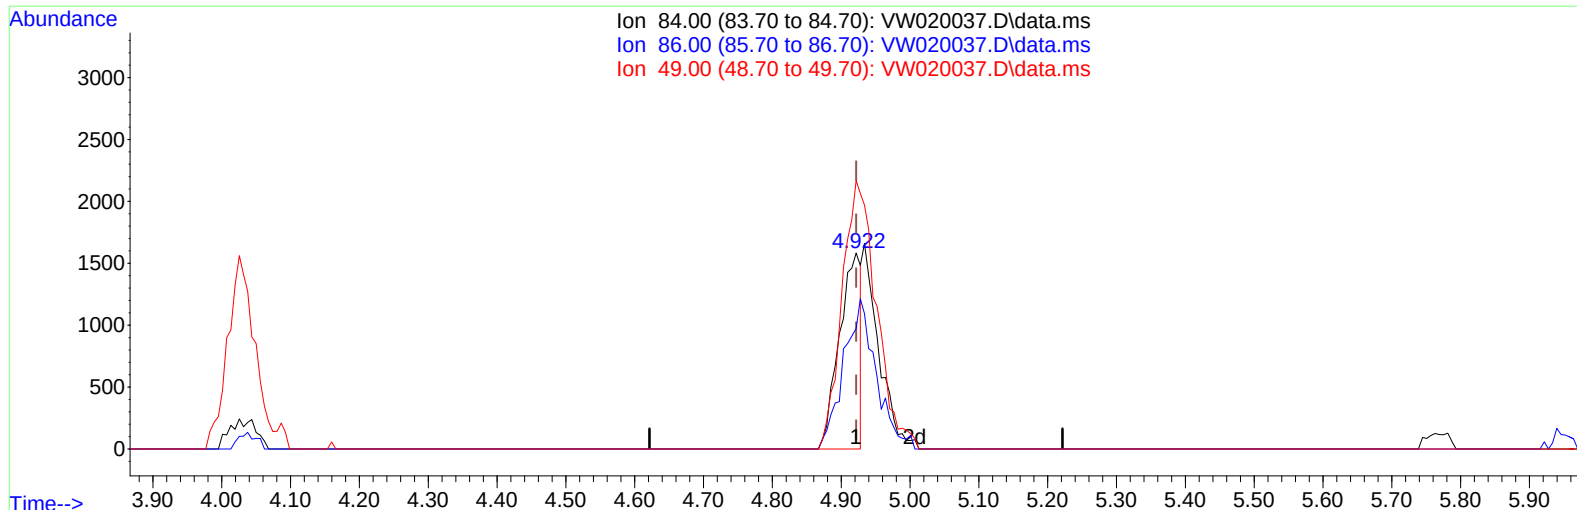

TIC: VW020037.D\data.ms

(16) Methylene chloride (T)

4.922min (-0.000) 0.78 ug/L

response 3431

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	61.47
49.00	123.70	136.96
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091621\
 Data File : VW020037.D
 Acq On : 16 Sep 2021 11:05
 Operator : SY/VA
 Sample : VW0916SBL07
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK434

Manual Integrations
 APPROVED

MMDadoda
 9/17/2021 4:38:41 PM

Quant Time: Sep 16 14:40:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 16 00:47:26 2021
 Response via : Initial Calibration

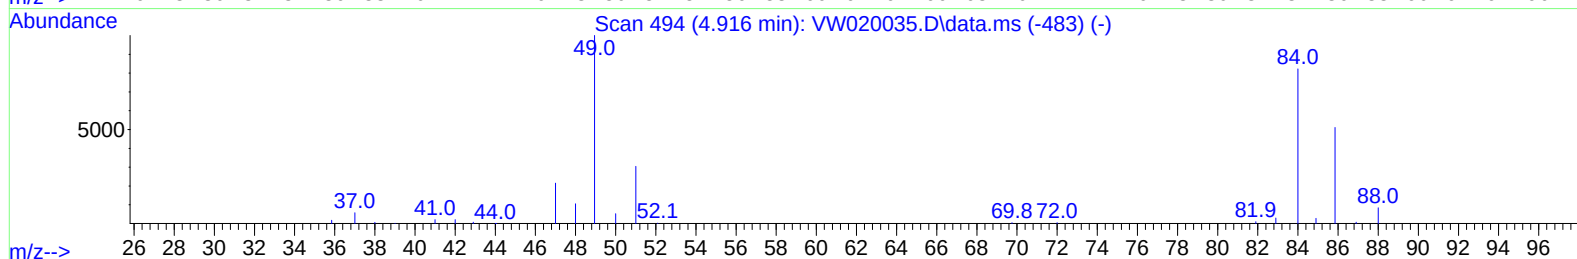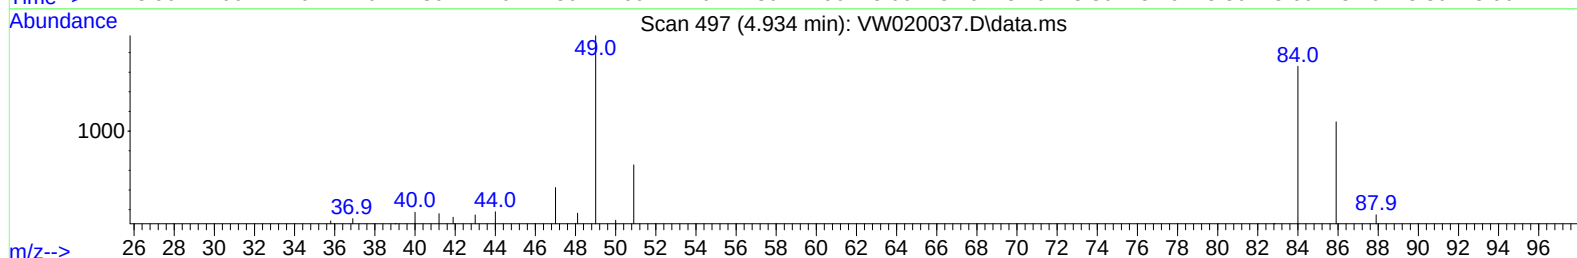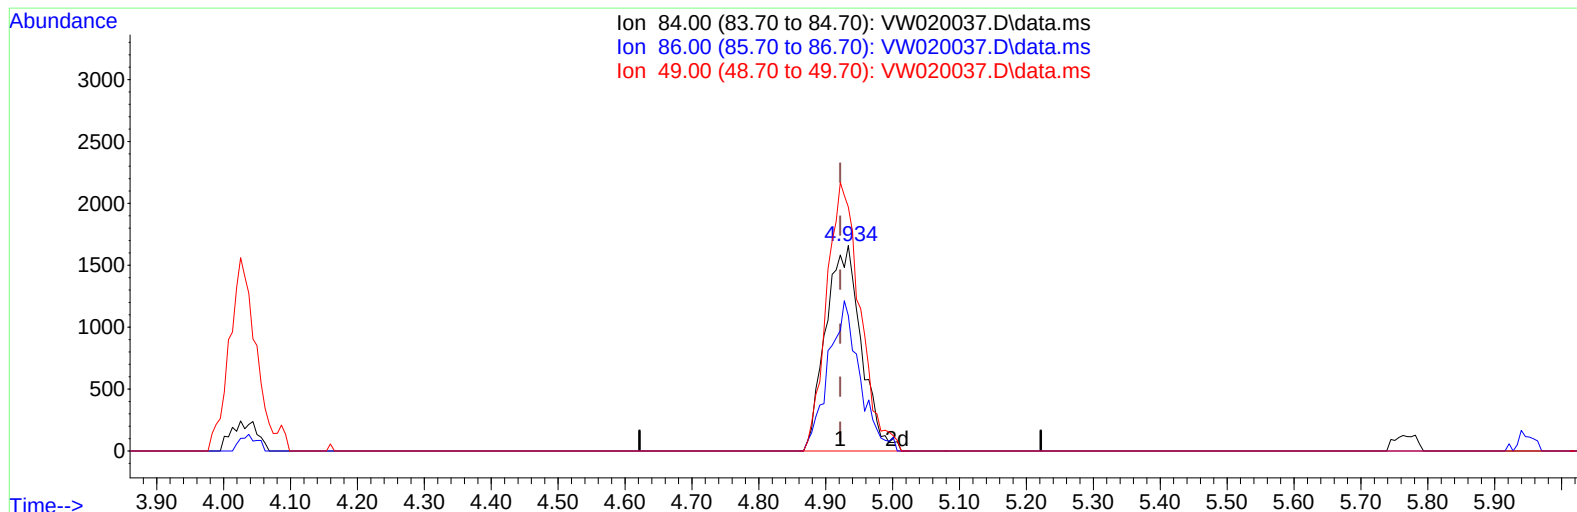

TIC: VW020037.D\data.ms

(16) Methylene chloride (T)

4.934min (+ 0.012) 1.39 ug/L m

response 6140

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	65.94
49.00	123.70	118.81
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091621\
Data File : VW020037.D
Acq On : 16 Sep 2021 11:05
Operator : SY/VA
Sample : VW0916SBL07
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK434

Quant Time: Sep 16 14:40:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 16 00:47:26 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
9/17/2021 4:38:41 PM

