

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091621\
Data File : VW020046.D
Acq On : 16 Sep 2021 18:51
Operator : SY/VA
Sample : M3755-09
Misc : 7.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AL5

Manual Integrations
APPROVED

MMDadoda
9/17/2021 4:38:57 PM

Quant Time: Sep 17 01:08:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
Qlast Update : Thu Sep 16 00:47:26 2021
Response via : Initial Calibration

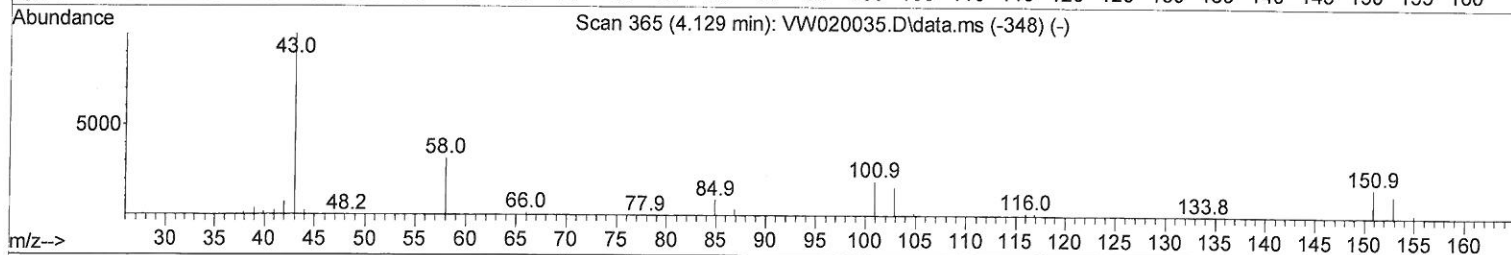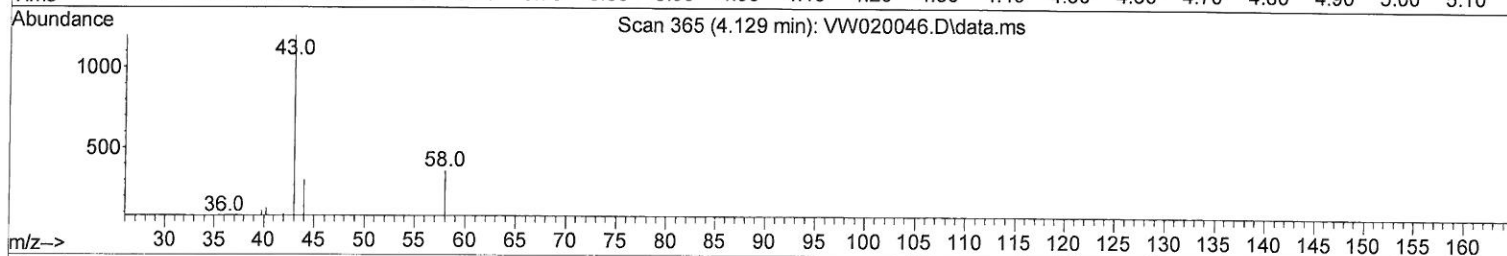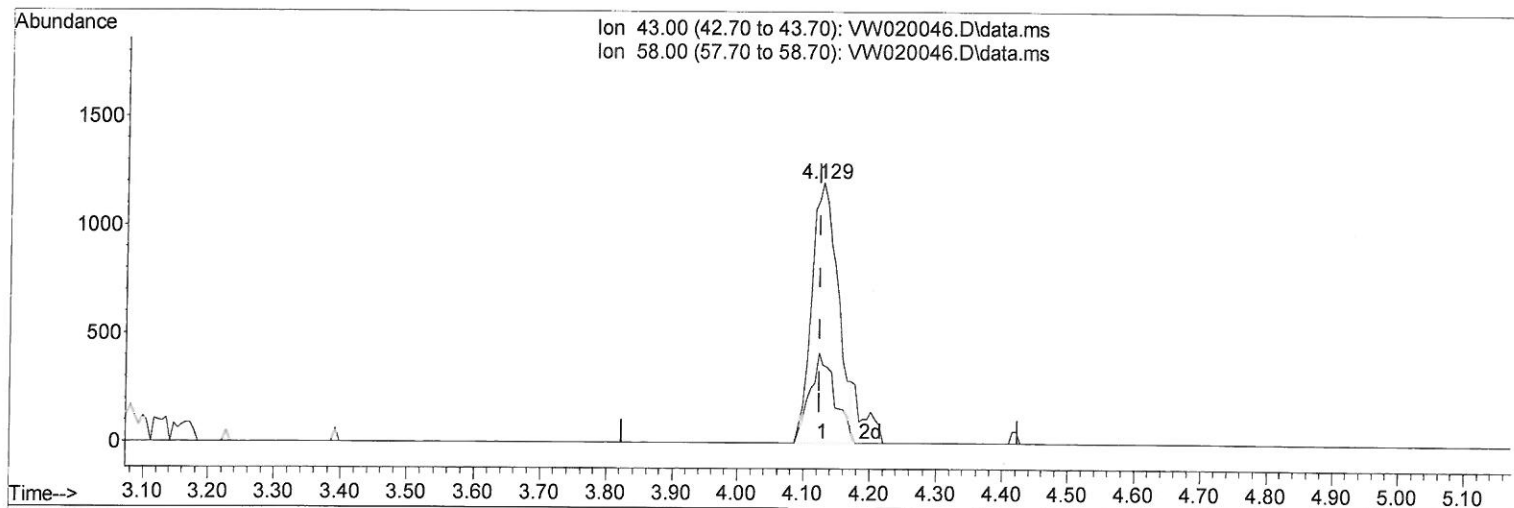

TIC: VW020046.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 7.06 ug/L

response 3337

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	29.34
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091621\
 Data File : VW020046.D
 Acq On : 16 Sep 2021 18:51
 Operator : SY/VA
 Sample : M3755-09
 Misc : 7.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 COAL5

Manual Integrations
 APPROVED

MMDadoda
 9/17/2021 4:38:57 PM

Quant Time: Sep 17 01:08:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 16 00:47:26 2021
 Response via : Initial Calibration

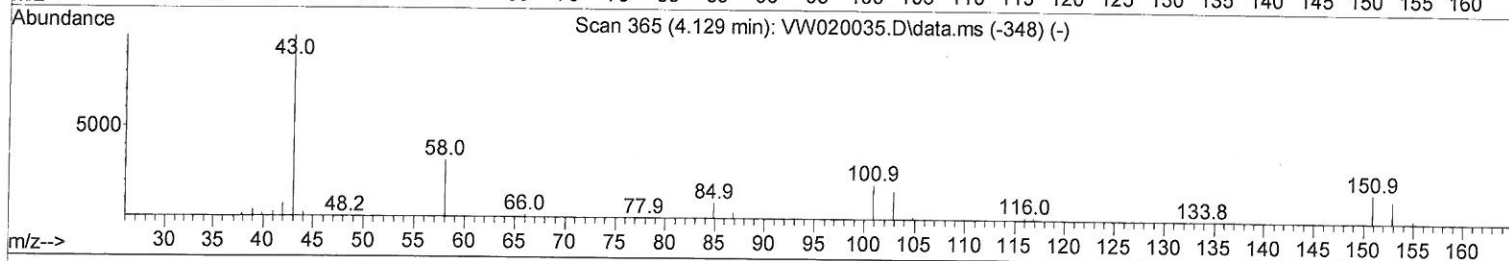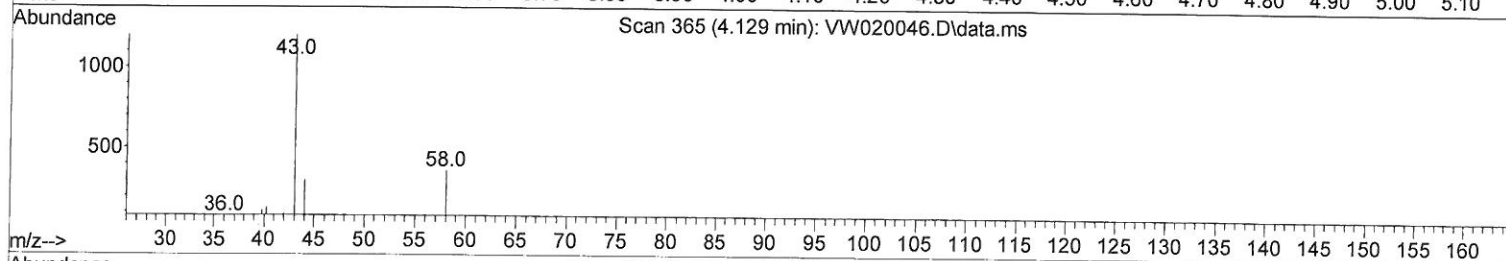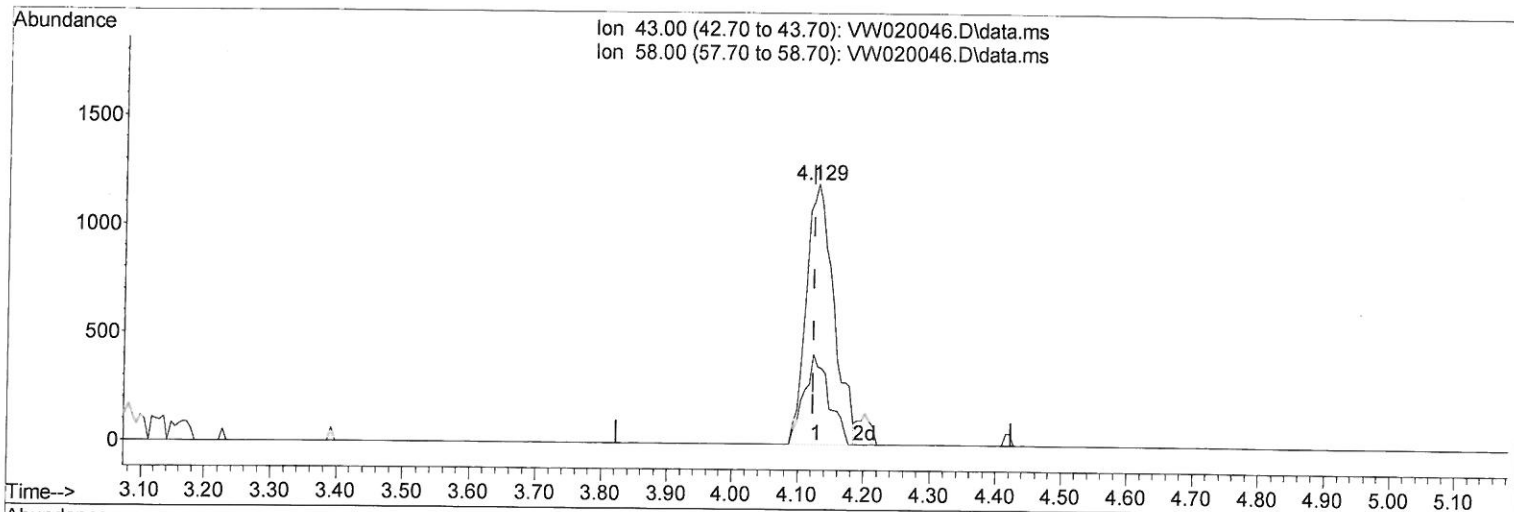

TIC: VW020046.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 7.34 ug/L m) 09/17/21 Sy

response 3472

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	28.20
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091621\
 Data File : VW020046.D
 Acq On : 16 Sep 2021 18:51
 Operator : SY/VA
 Sample : M3755-09
 Misc : 7.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AL5

Manual Integrations
 APPROVED

MMDadoda
 9/17/2021 4:38:57 PM

Quant Time: Sep 17 01:08:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Sep 16 00:47:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	110510	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	101809	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	36734	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	67233	36.938	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 147.760%			
7) Chloroethane-d5	2.898	69	53041	33.856	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 135.440%			
11) 1,1-Dichloroethene-d2	4.019	63	70718	23.770	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery = 95.080%			
21) 2-Butanone-d5	7.080	46	15426	30.980	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 61.960%			
24) Chloroform-d	7.653	84	93049	30.558	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 122.240%			
26) 1,2-Dichloroethane-d4	8.311	65	49228	27.444	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 109.760%			
32) Benzene-d6	8.281	84	171000	30.785	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 123.120%			
36) 1,2-Dichloropropane-d6	9.281	67	51521	31.271	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 125.080%#			
41) Toluene-d8	10.329	98	139277	26.749	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 107.000%			
43) trans-1,3-Dichloroprop...	10.579	79	17764	23.439	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 93.760%			
47) 2-Hexanone-d5	10.927	63	10491	31.169	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 62.340%			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	34065	21.016	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 84.080%			
66) 1,2-Dichlorobenzene-d4	13.853	152	35755	28.561	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 114.240%			
Target Compounds						
13) Acetone	4.129	43	3472m	7.342	ug/L	Qvalue
16) Methylene chloride	4.922	84	4136	2.124	ug/L	90
42) Toluene	10.390	91	2383	0.364	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091621\
Data File : VW020046.D
Acq On : 16 Sep 2021 18:51
Operator : SY/VA
Sample : M3755-09
Misc : 7.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AL5

Manual Integrations
APPROVED

MMDadoda
9/17/2021 4:38:57 PM

Quant Time: Sep 17 01:08:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091421SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Sep 16 00:47:26 2021
Response via : Initial Calibration

