

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW091718\
 Data File : VW005441.D
 Acq On : 17 Sep 2018 18:27
 Operator : SY/AP
 Sample : J4929-09
 Misc : 6.24G/5ML/MSVOA W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SP-PIT-11

Quant Time: Sep 18 01:04:20 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 15 02:32:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.96
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.85
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.64
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.57
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	12.52	95	20	0.00	ug/l	-0.10
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW091718\
Data File : VW005441.D
Acq On : 17 Sep 2018 18:27
Operator : SY/AP
Sample : J4929-09
Misc : 6.24G/5ML/MSVOA W/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SP-PIT-11

Quant Time: Sep 18 01:04:20 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
Quant Title : SW846 8260
QLast Update : Sat Sep 15 02:32:34 2018
Response via : Initial Calibration

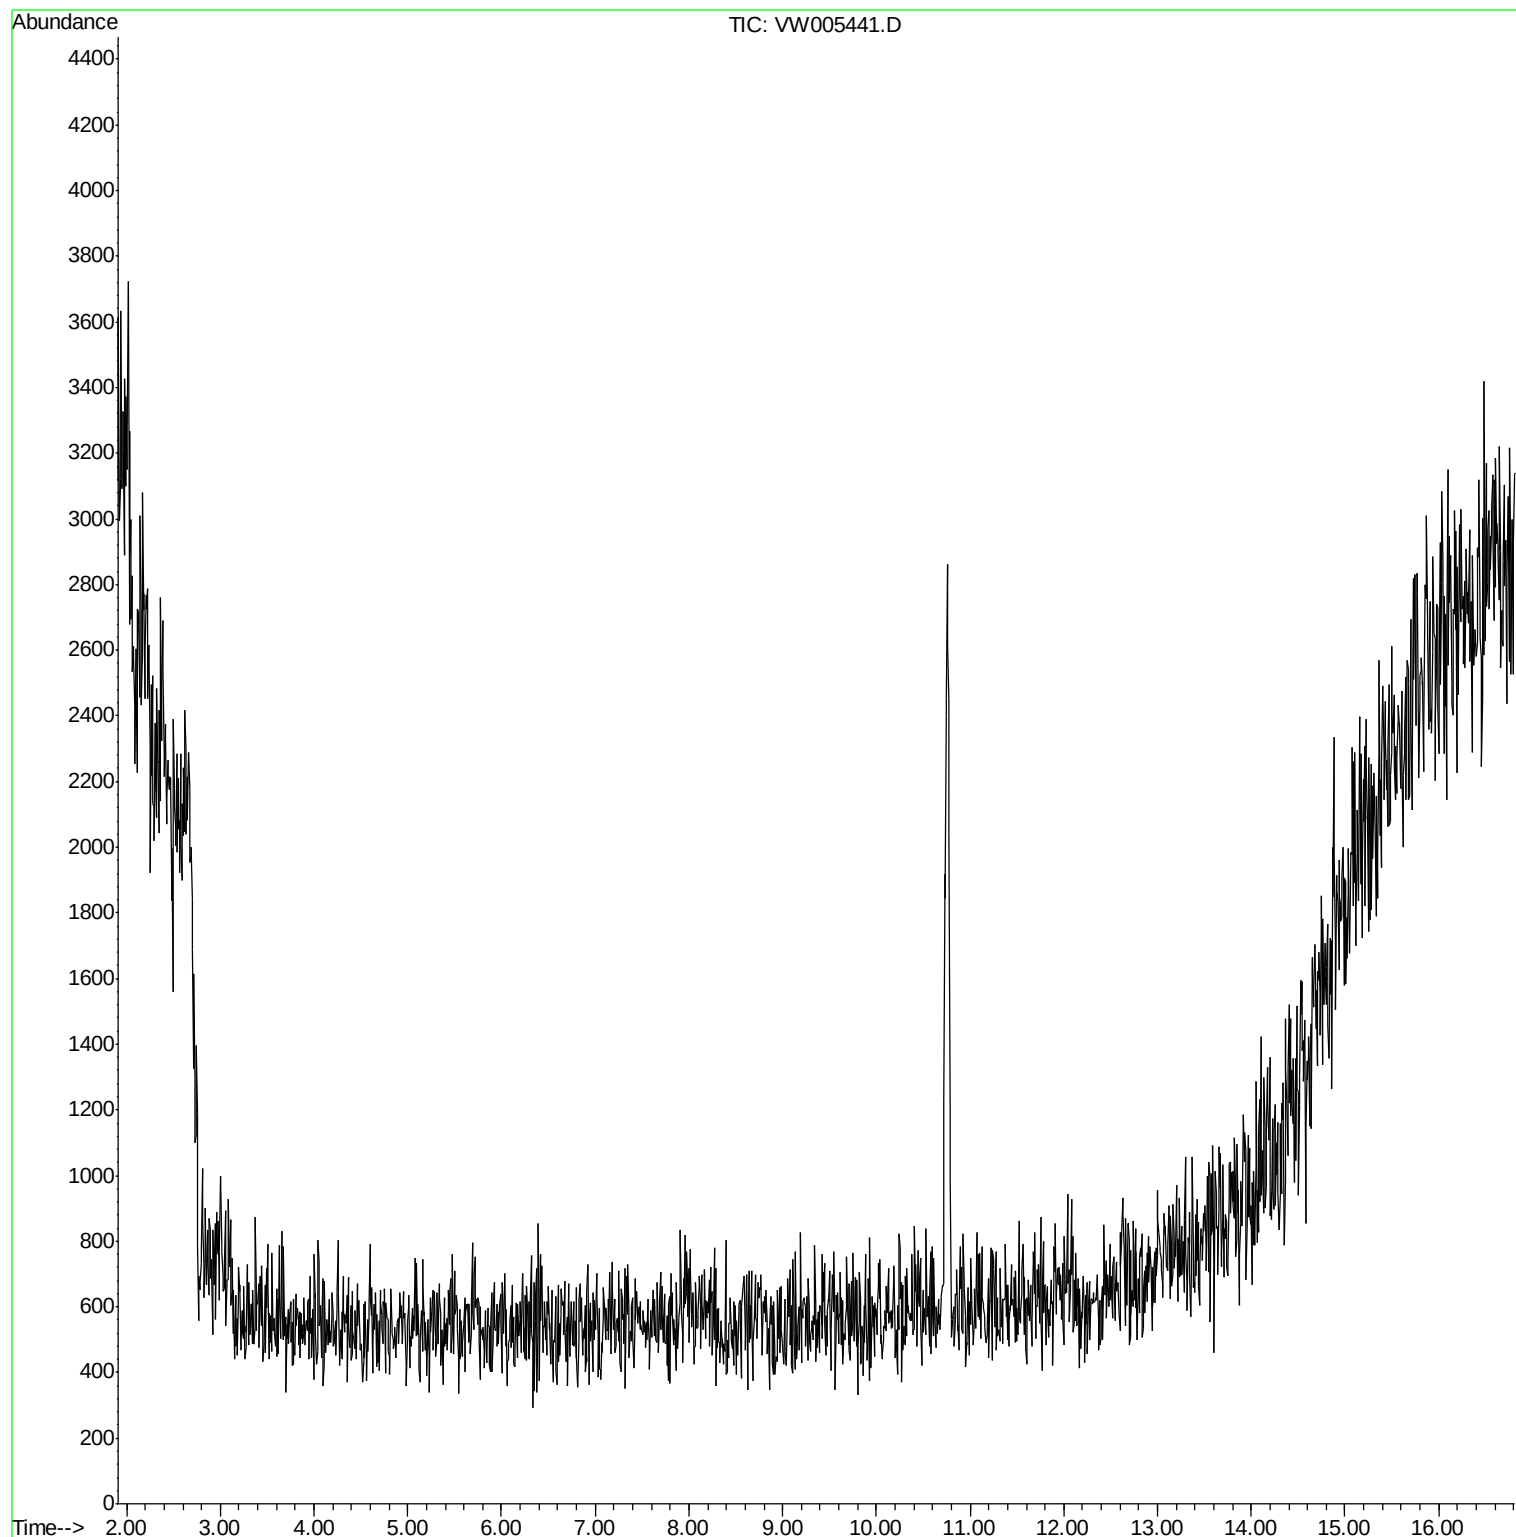

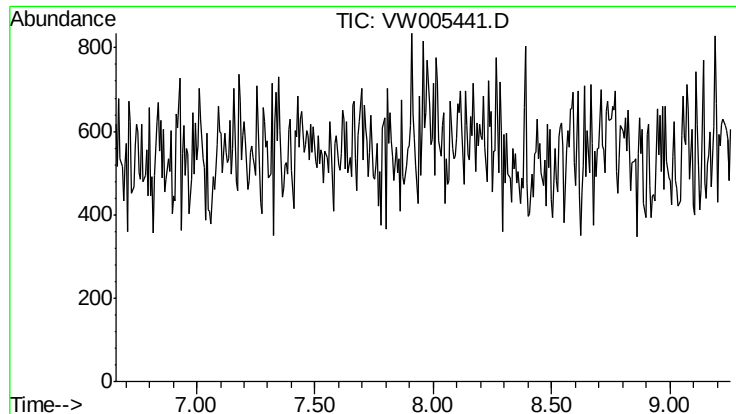

#1

Pentafluorobenzene

Concen: 0.00 ug/l

Expected RT: 7.96 min

Lab File: VW005441.D

Acq: 17 Sep 2018 18:27

Tot Ion: 168

Sig Exp Ratio

168 100



99 56.3

Instrument :

MSVOA_W

ClientSampleId :

SP-PIT-11

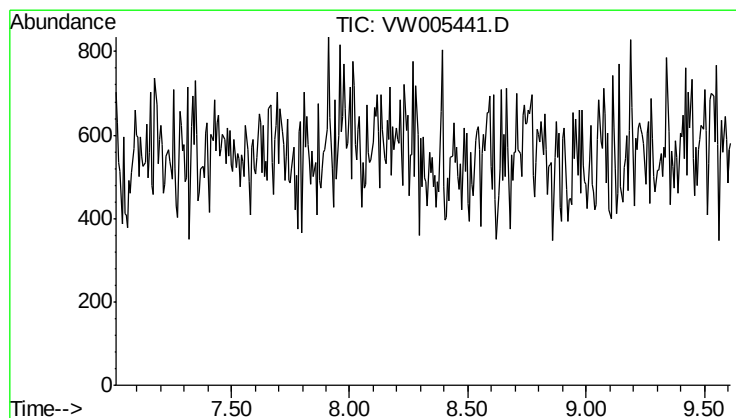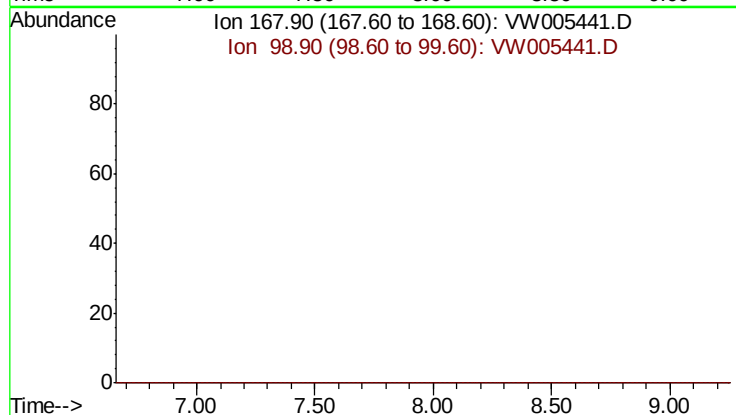

#33

1,2-Dichloroethane-d4

Concen: 0.00 ug/l

Expected RT: 8.31 min

Lab File: VW005441.D


Acq: 17 Sep 2018 18:27


Tgt Ion: 65

Sig Exp Ratio

65 100

67 50.3

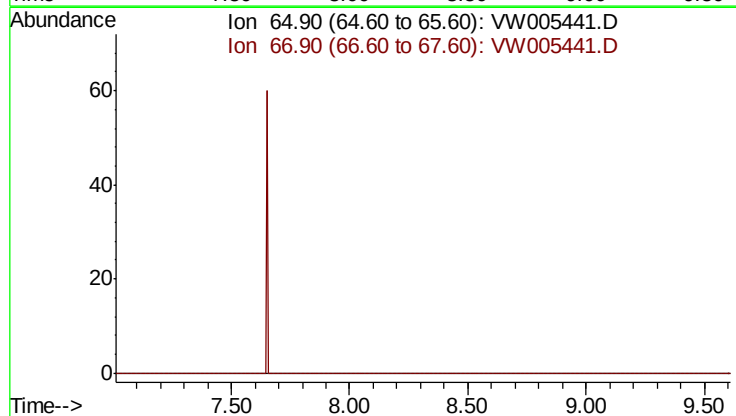


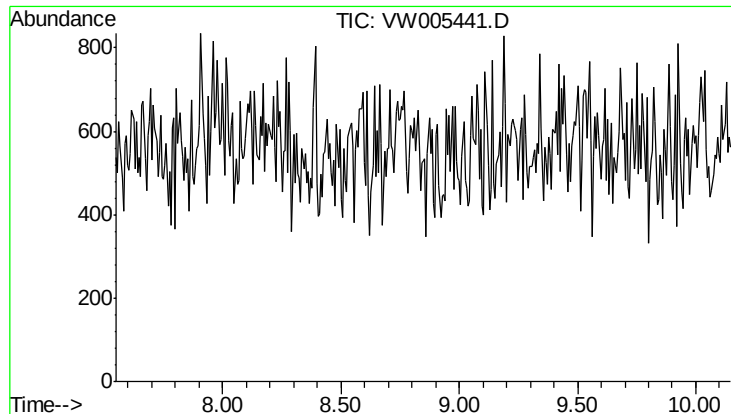


#34
 1,4-Difluorobenzene
 Concen: 0.00 ug/l
 Expected RT: 8.85 min

Lab File: VW005441.D
 Acq: 17 Sep 2018 18:27

Instrument :
 MSVOA_W
 ClientSampleId :
 SP-PIT-11


Tot Ion	114
Sig	Exp Ratio
114	100
63	21.7
88	15.9

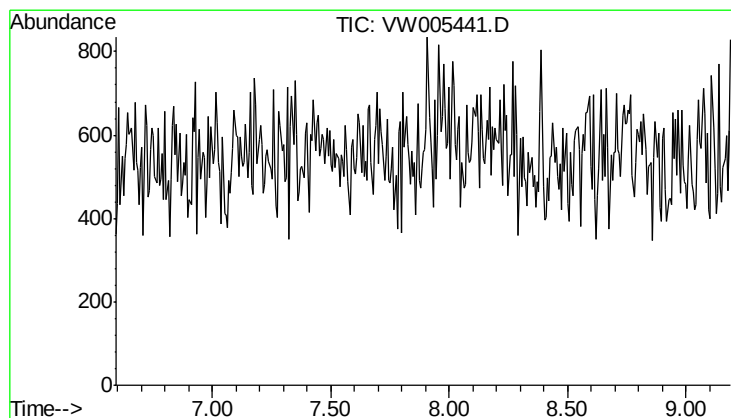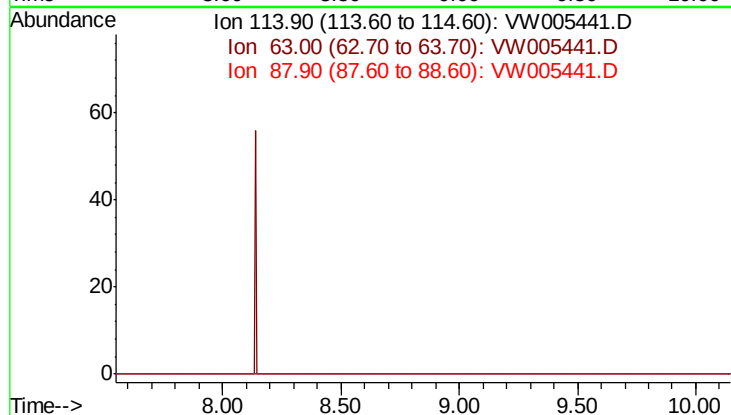


#35
 Dibromofluoromethane
 Concen: 0.00 ug/l
 Expected RT: 7.89 min

Lab File: VW005441.D
 Acq: 17 Sep 2018 18:27

Tgt Ion	113
Sig	Exp Ratio
113	100
111	102.9
192	20.6


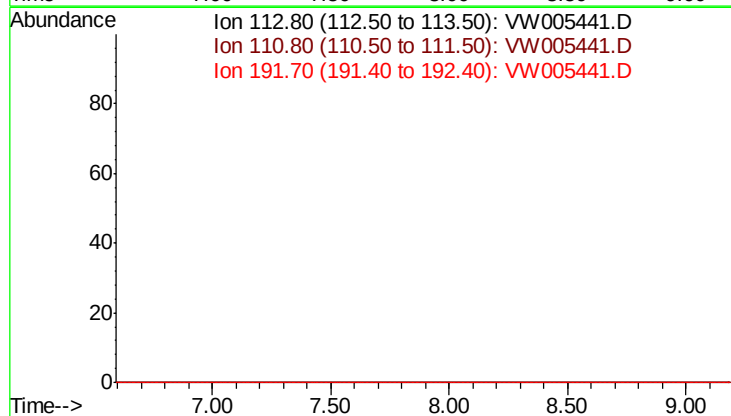


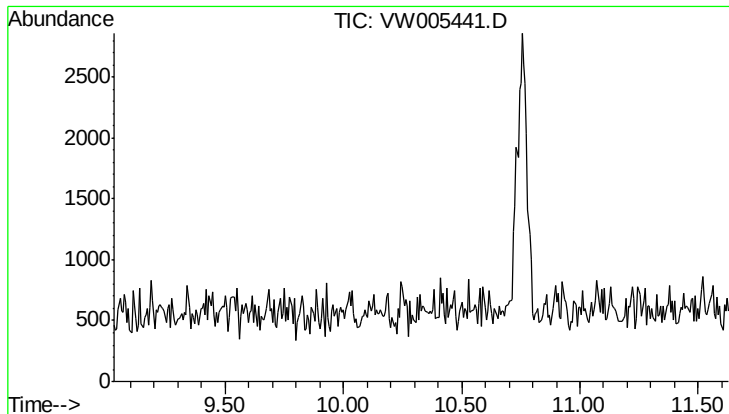

#50
Toluene-d8
Concen: 0.00 ug/l
Expected RT: 10.33 min
Lab File: VW005441.D
Acq: 17 Sep 2018 18:27




Instrument :
MSVOA_W
ClientSampleId :
SP-PIT-11


Tot Ion: 98
Sig Exp Ratio
98 100
100 64.2

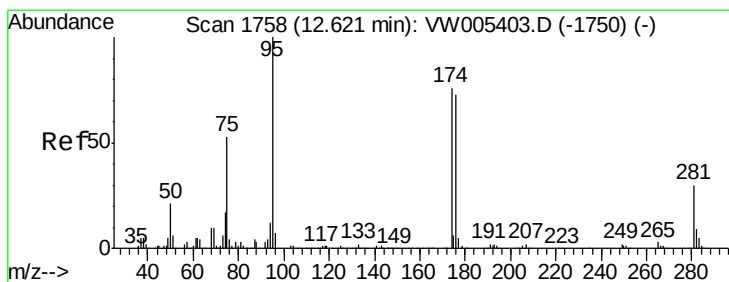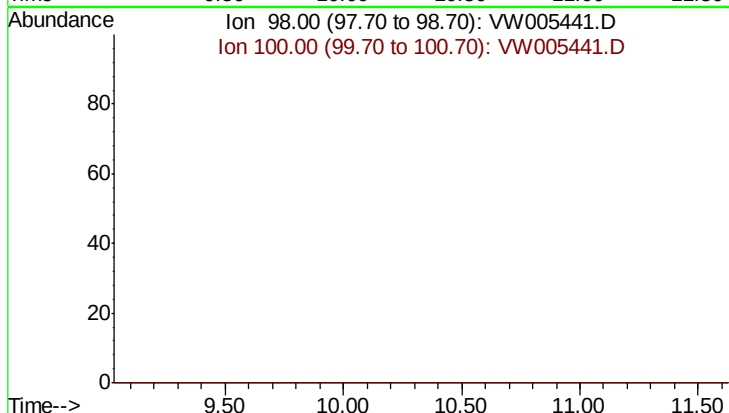

#62
4-Bromofluorobenzene
Concen: 0.00 ug/l
RT: 12.52 min Scan# 1742
Delta R.T. -0.10 min
Lab File: VW005441.D
Acq: 17 Sep 2018 18:27

Tgt Ion: 95 Resp: 20
Ion Ratio Lower Upper
95 100
174 0.0 0.0 161.2
176 0.0 0.0 156.6

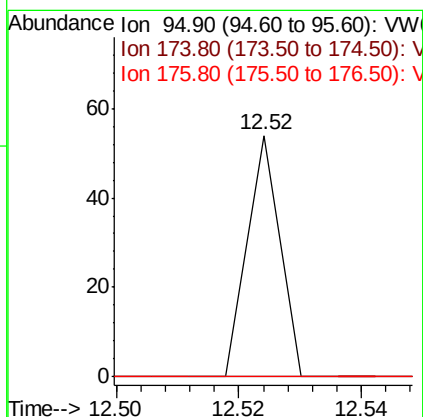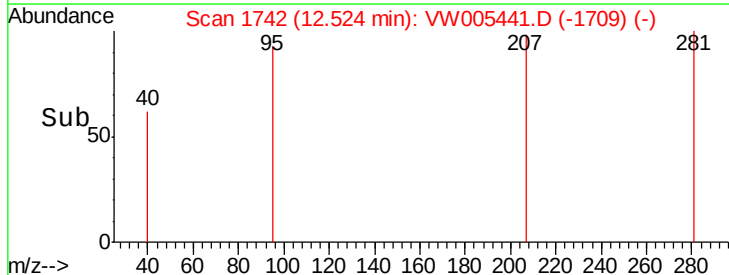
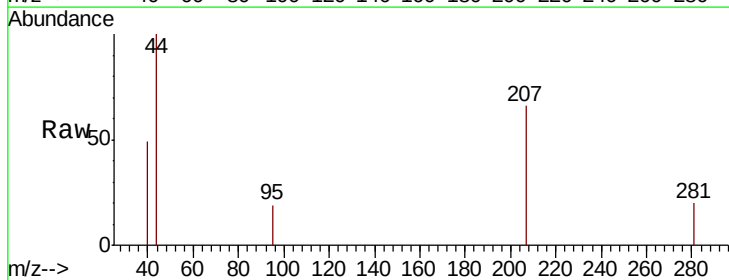


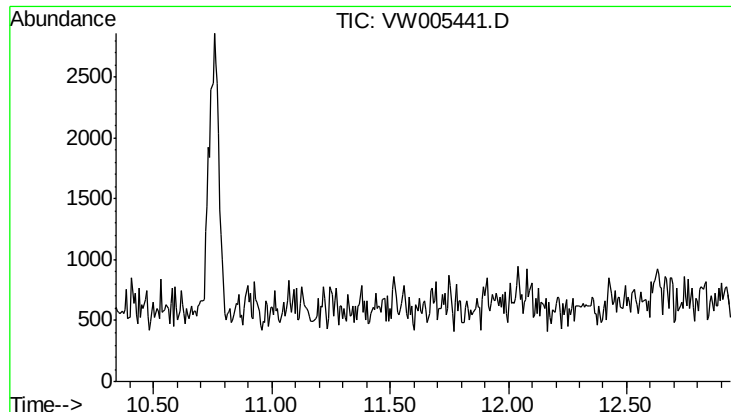

#63
 Chlorobenzene-d5
 Concen: 0.00 ug/l
 Expected RT: 11.64 min
 Lab File: VW005441.D
 Acq: 17 Sep 2018 18:27

Instrument :
 MSVOA_W
 ClientSampleId :
 SP-PIT-11

Tot Ion	117
Sig	Exp Ratio
117	100
82	57.4
119	31.0

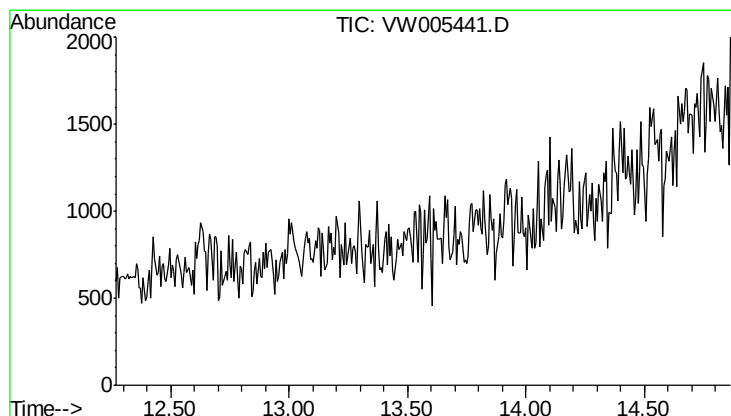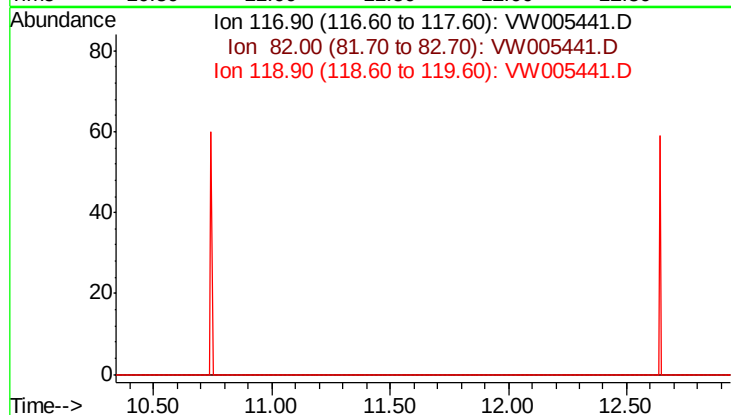

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.00 ug/l
 Expected RT: 13.57 min
 Lab File: VW005441.D
 Acq: 17 Sep 2018 18:27

Tgt Ion	152
Sig	Exp Ratio
152	100
115	59.0
150	172.8

