


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW091718\
Data File : VW005422.D
Acq On : 17 Sep 2018 09:50
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
Title : SW846 8260
Last Update : Sat Sep 15 02:32:34 2018

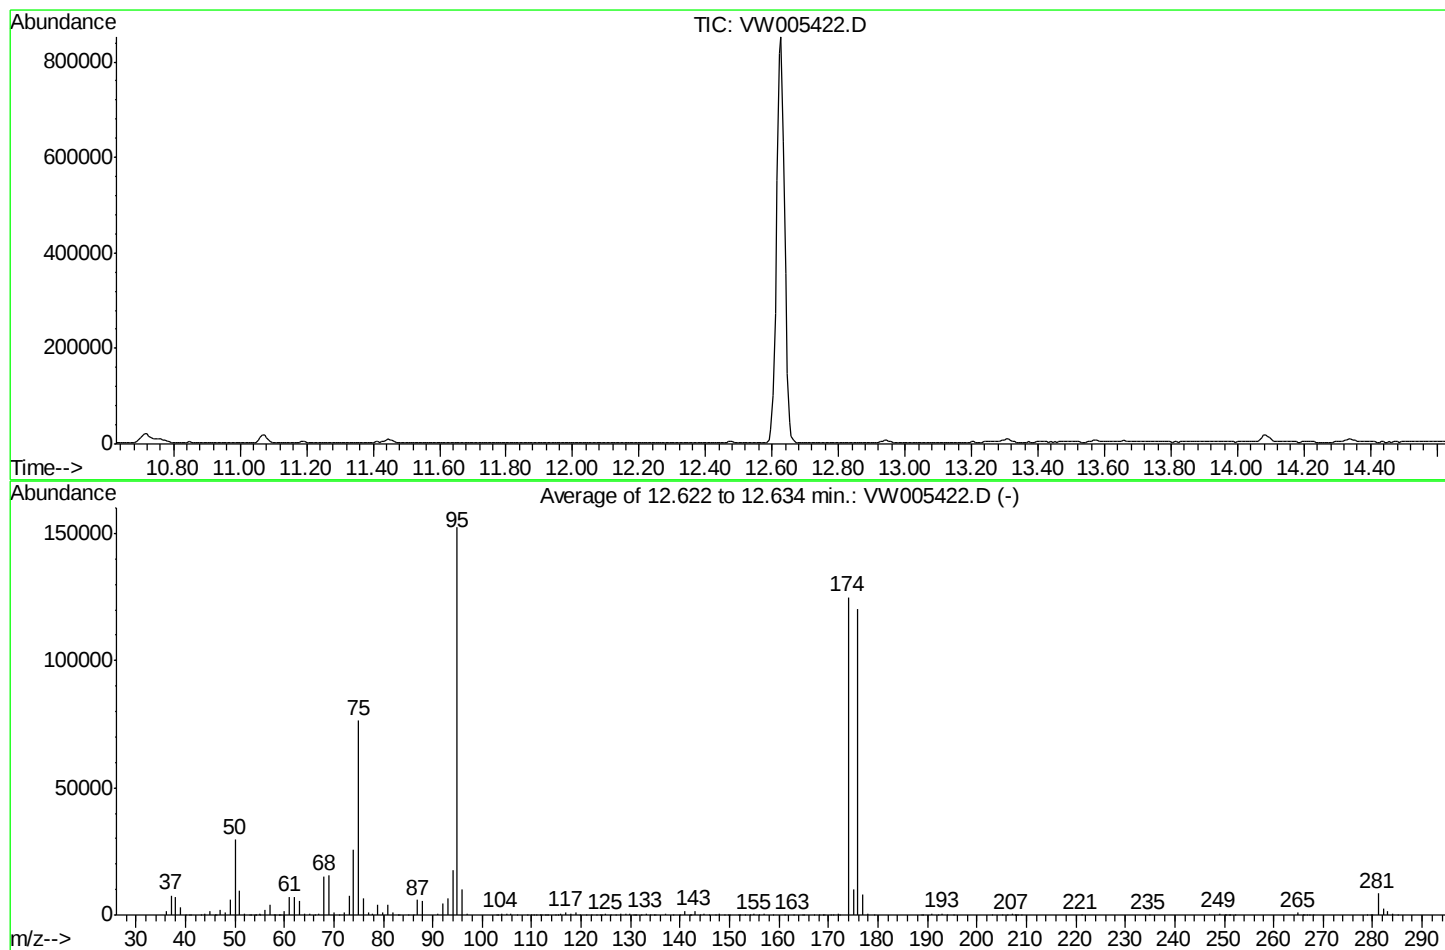

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	29618	PASS
75	95	30	60	50.1	76426	PASS
95	95	100	100	100.0	152405	PASS
96	95	5	9	6.6	10126	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.9	124888	PASS
175	174	5	9	8.2	10273	PASS
176	174	95	101	96.5	120536	PASS
177	176	5	9	6.5	7846	PASS