


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW091719\
Data File : VW013077.D
Acq On : 17 Sep 2019 09:07
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Title : SW846 8260
Last Update : Fri Sep 13 17:26:01 2019

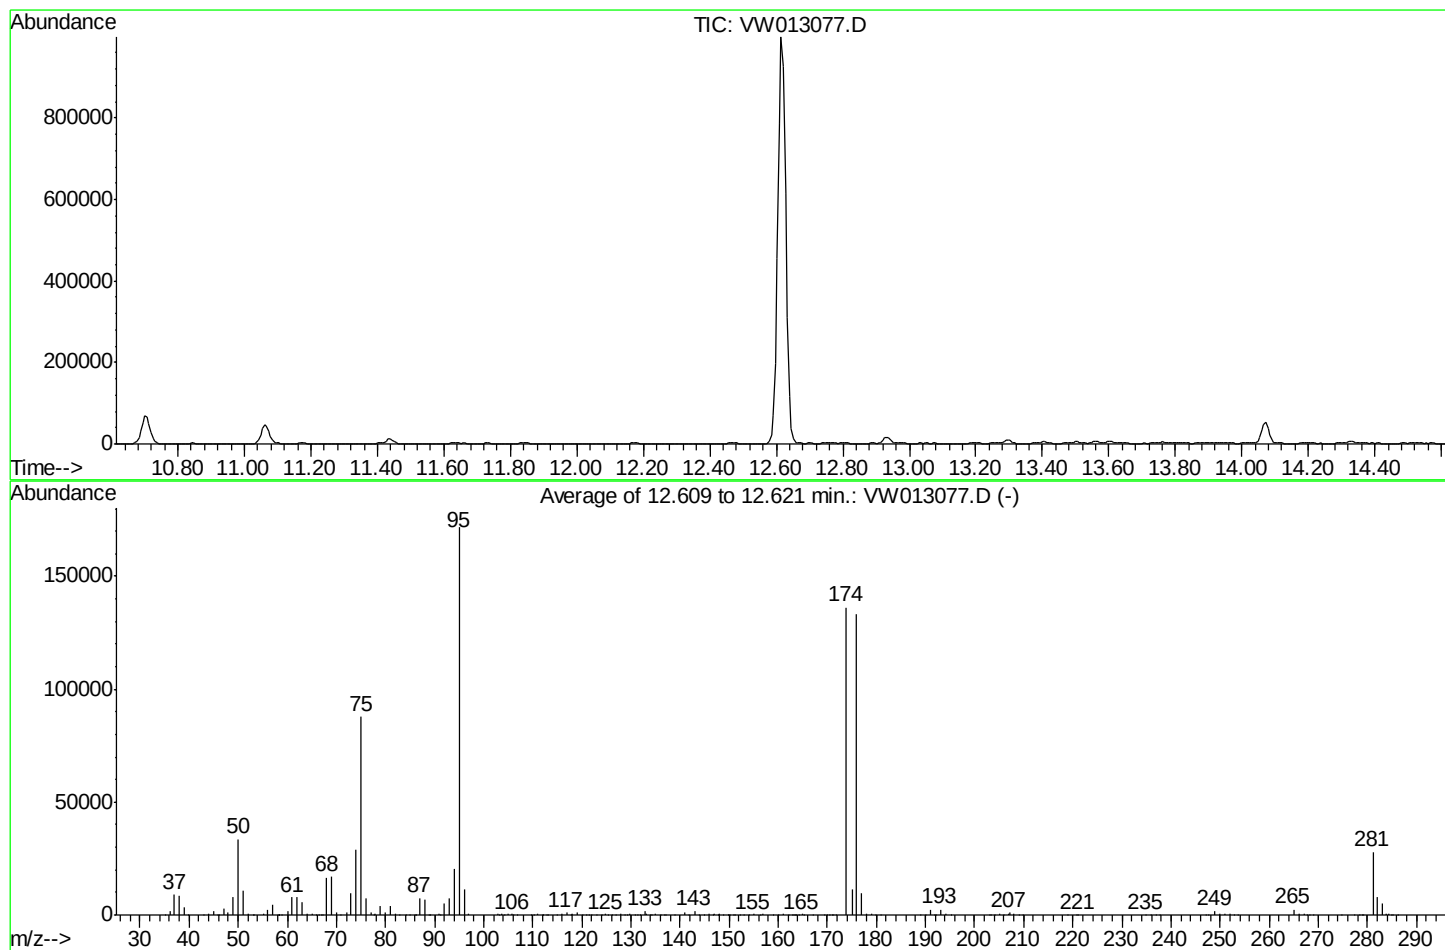

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	33688	PASS
75	95	30	60	51.1	87682	PASS
95	95	100	100	100.0	171712	PASS
96	95	5	9	6.5	11157	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.4	136282	PASS
175	174	5	9	8.4	11423	PASS
176	174	95	101	97.9	133442	PASS
177	176	5	9	7.2	9569	PASS