

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW091818\
 Data File : VW005475.D
 Acq On : 18 Sep 2018 13:33
 Operator : SY/AP
 Sample : VW0918SBL01
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0918SBL01

Quant Time: Sep 18 16:55:30 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 15 02:32:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.96	168	315504	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	486667	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	465185	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	229420	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	154079	47.05	ug/l	0.00
Spiked Amount						
			Recovery	=	94.10%	
35) Dibromofluoromethane	7.89	113	130716	47.90	ug/l	0.00
Spiked Amount						
			Recovery	=	95.80%	
50) Toluene-d8	10.33	98	610014	48.82	ug/l	0.00
Spiked Amount						
			Recovery	=	97.64%	
62) 4-Bromofluorobenzene	12.62	95	216628	47.28	ug/l	0.00
Spiked Amount						
			Recovery	=	94.56%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
20) Methylene Chloride	4.92	84	22363	1.29	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW091818\
Data File : VW005475.D
Acq On : 18 Sep 2018 13:33
Operator : SY/AP
Sample : VW0918SBL01
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW0918SBL01

Quant Time: Sep 18 16:55:30 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W091618S.M
Quant Title : SW846 8260
QLast Update : Sat Sep 15 02:32:34 2018
Response via : Initial Calibration

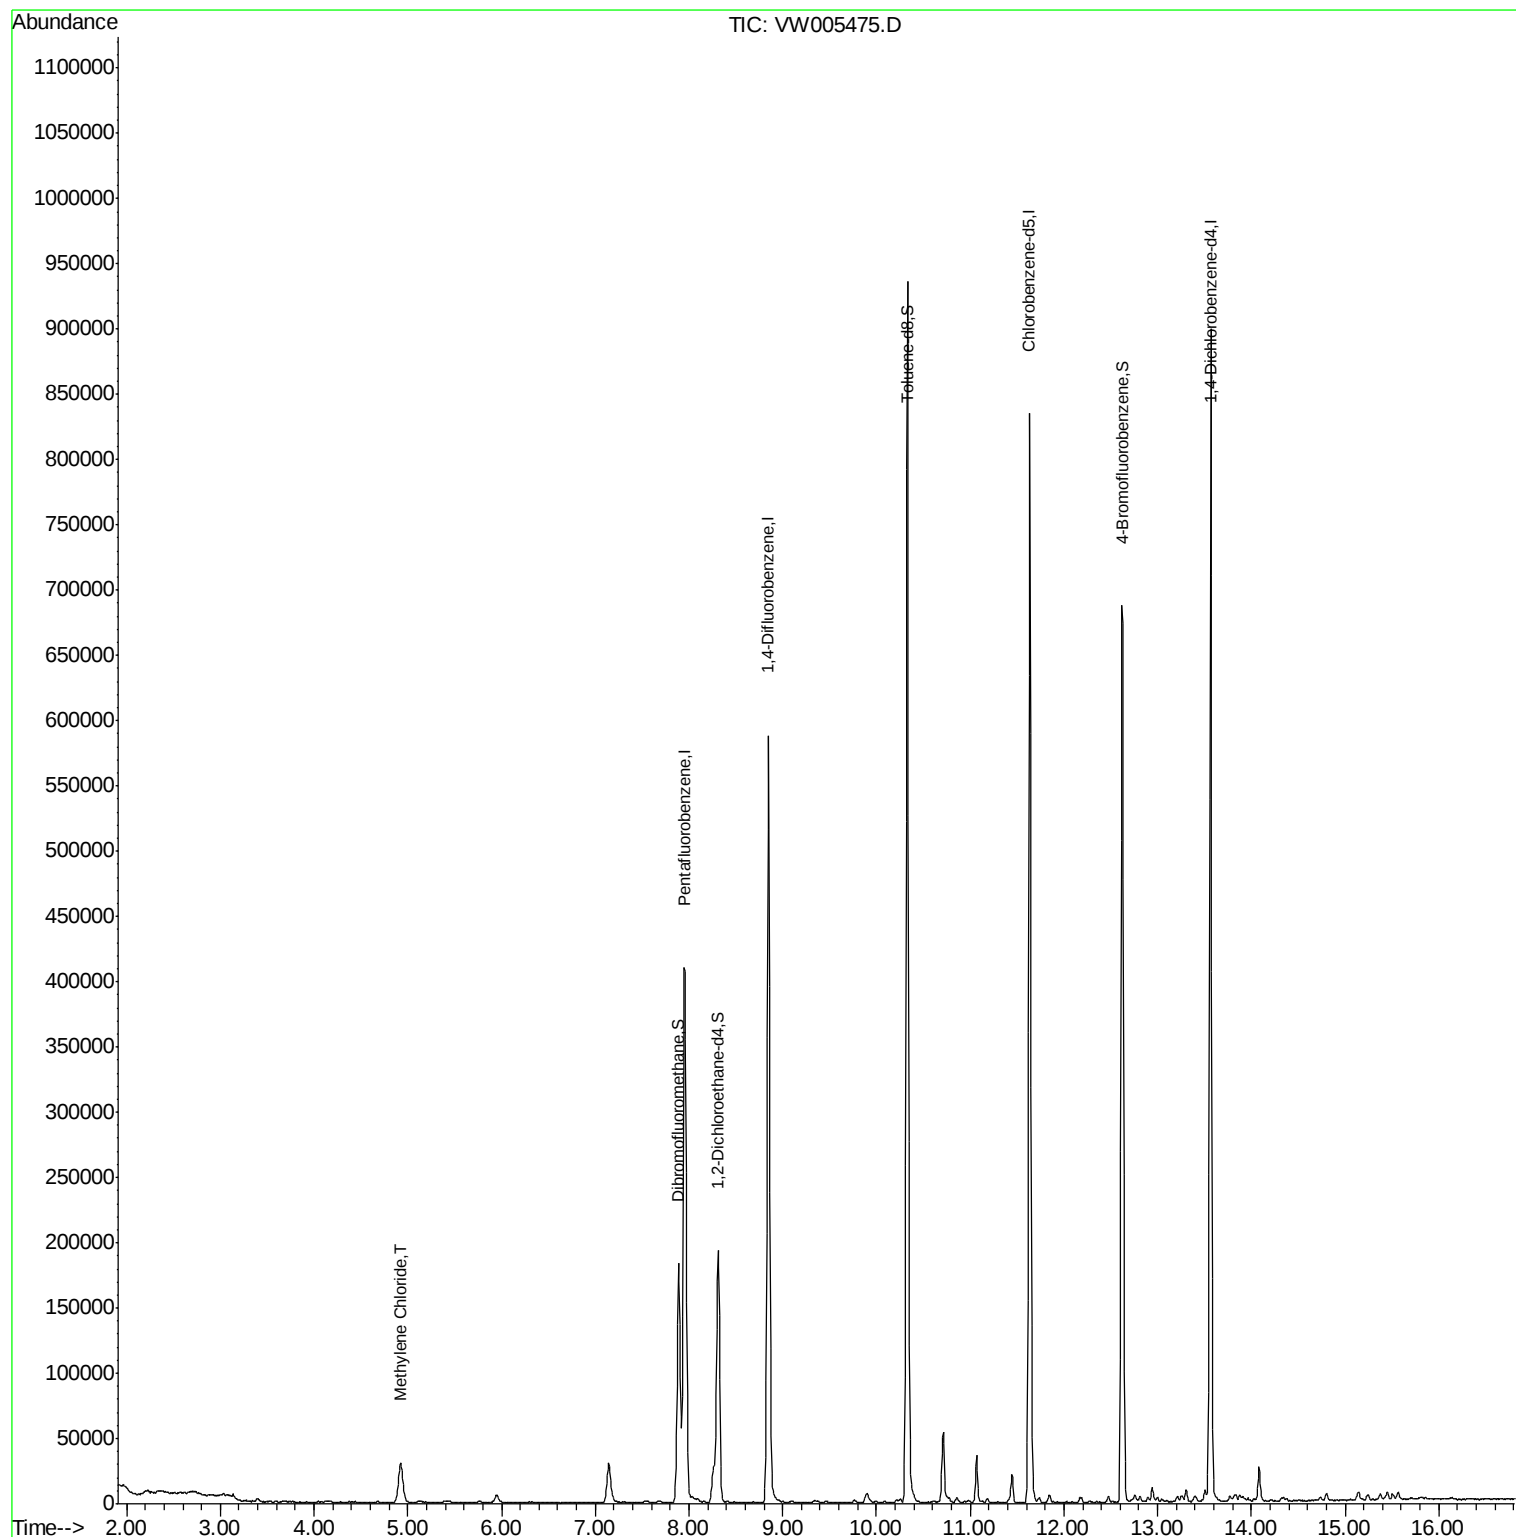

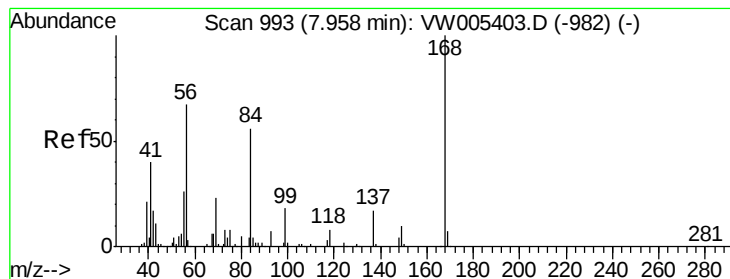

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.96 min Scan# 993

Delta R.T. -0.00 min

Lab File: VW005475.D

Acq: 18 Sep 2018 13:33

Instrument :

MSVOA_W

ClientSampleId :


VW0918SBL01

Tot Ion:168 Resp: 315504

Ion Ratio Lower Upper

168 100

99 56.5 45.0 67.6

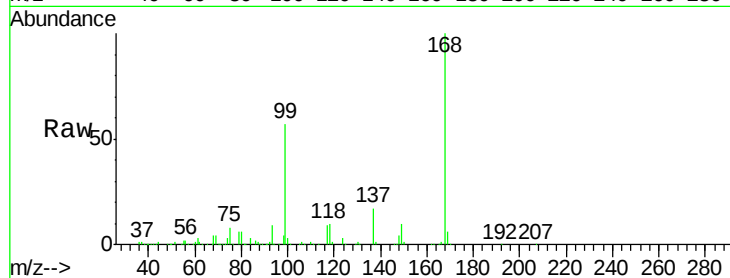

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.96



150000

100000

50000

0

Time--> 7.80 7.90 8.00 8.10

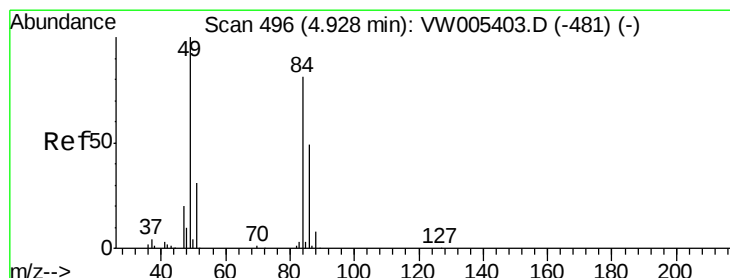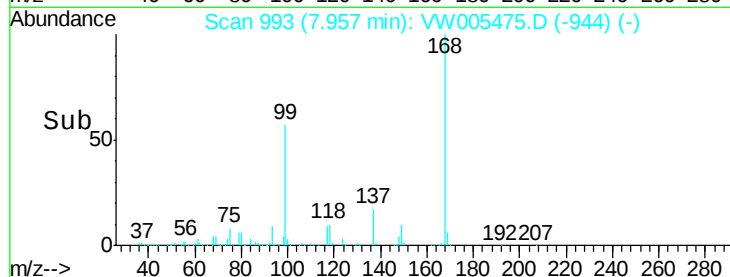

#20

Methylene Chloride

Concen: 1.29 ug/l

RT: 4.92 min Scan# 495

Delta R.T. -0.01 min

Lab File: VW005475.D

Acq: 18 Sep 2018 13:33

Tgt Ion: 84 Resp: 22363


Ion Ratio Lower Upper

84 100

49 131.9 99.3 148.9

51 38.9 31.1 46.7

86 60.6 49.1 73.7

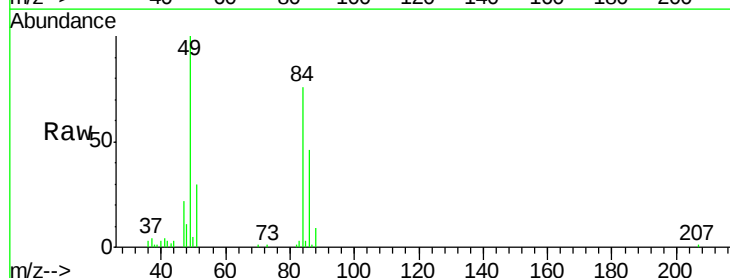

Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW


15000


10000

5000

0

Time--> 4.80 4.90 5.00

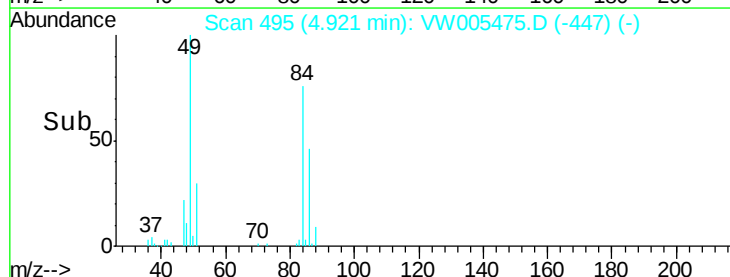

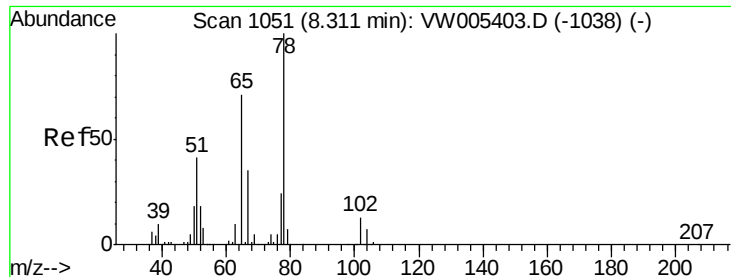

#33

1,2-Dichloroethane-d4

Concen: 47.05 ug/l

RT: 8.31 min Scan# 1051

Delta R.T. -0.00 min

Lab File: VW005475.D

Acq: 18 Sep 2018 13:33

Instrument :

MSVOA_W

ClientSampleId :





VW0918SBL01

Tot Ion: 65 Resp: 154079

Ion Ratio Lower Upper

65 100

67 52.8 0.0 100.6

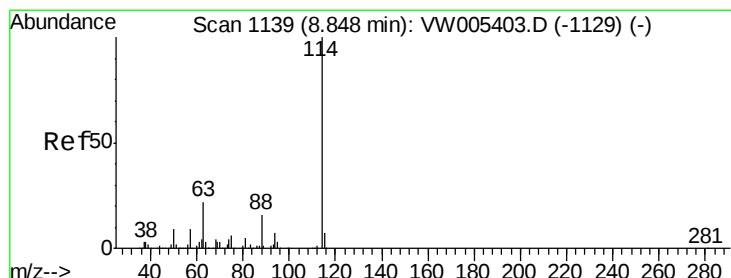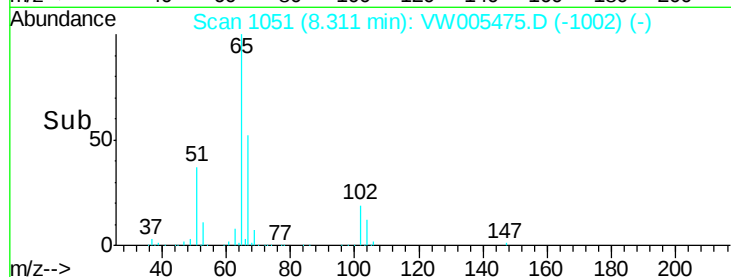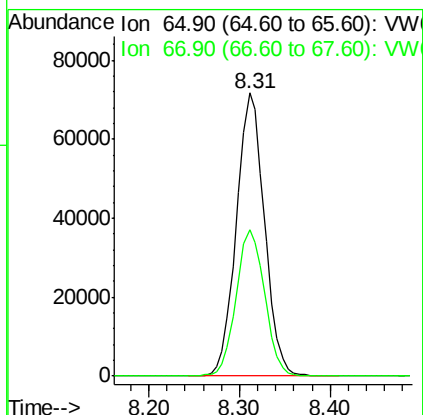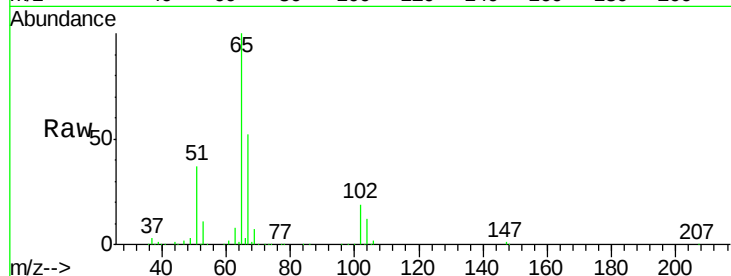

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.85 min Scan# 1139

Delta R.T. -0.00 min

Lab File: VW005475.D

Acq: 18 Sep 2018 13:33




Tgt Ion: 114 Resp: 486667


Ion Ratio Lower Upper

114 100

63 22.7 0.0 43.4

88 16.5 0.0 31.8

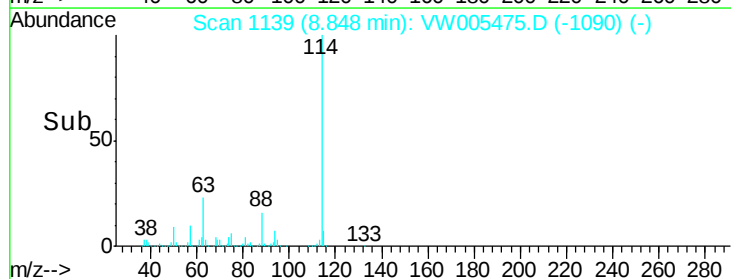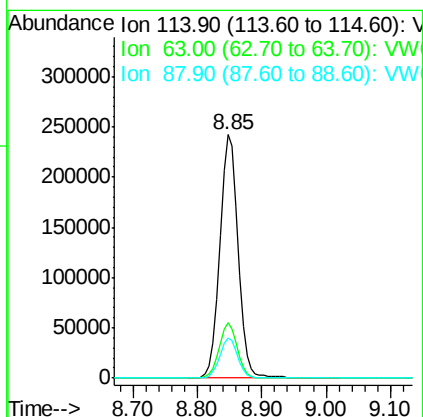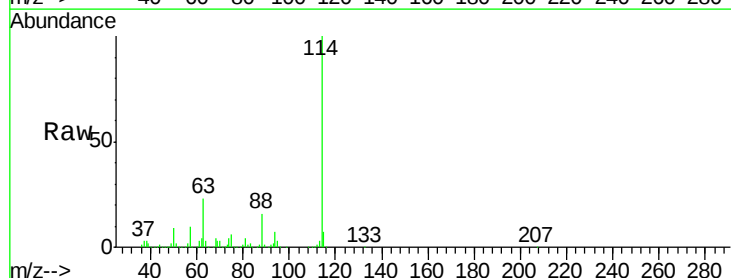


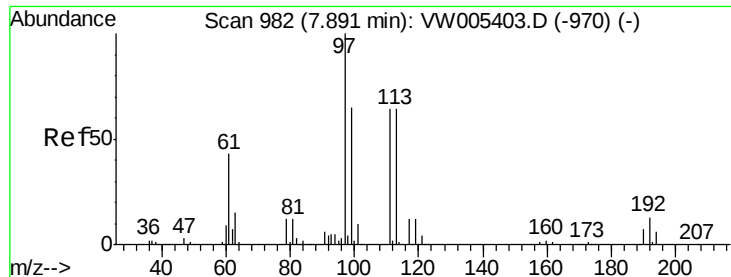




#35
 Dibromofluoromethane
 Concen: 47.90 ug/l
 RT: 7.89 min Scan# 982
 Delta R.T. -0.00 min
 Lab File: VW005475.D
 Acq: 18 Sep 2018 13:33

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0918SBL01

Tot Ion	Ratio	Lower	Upper
113	100		
111	103.6	82.3	123.5
192	20.0	16.5	24.7

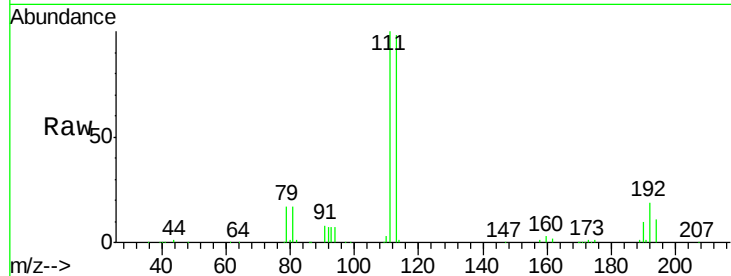


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

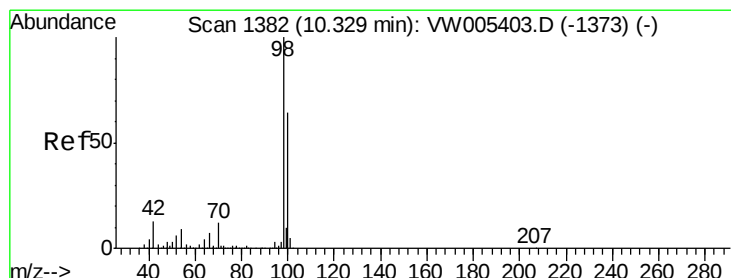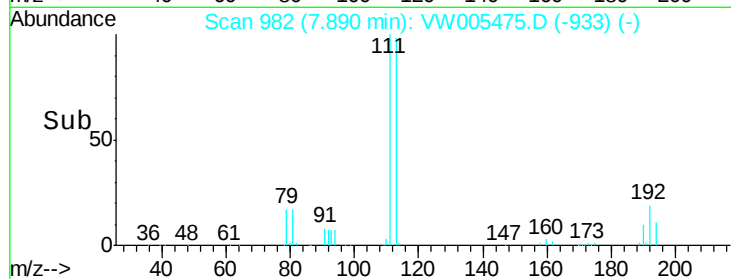
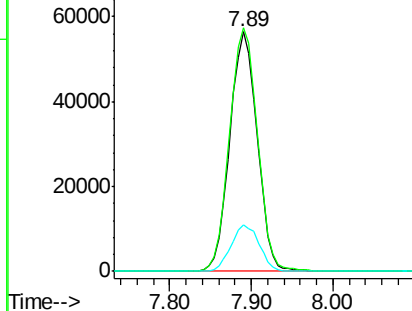



#50
 Toluene-d8
 Concen: 48.82 ug/l
 RT: 10.33 min Scan# 1382
 Delta R.T. -0.00 min
 Lab File: VW005475.D
 Acq: 18 Sep 2018 13:33

Tgt Ion	Ratio	Lower	Upper
98	100		
100	63.8	51.4	77.0

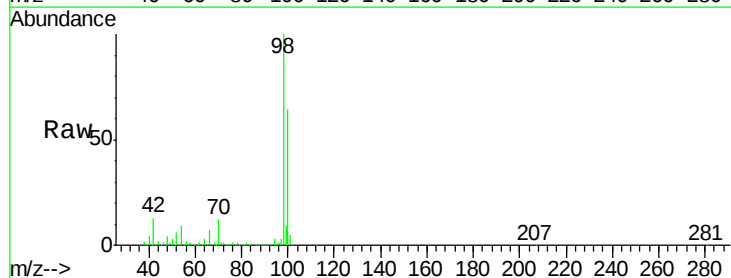

Abundance Ion 98.00 (97.70 to 98.70): VW
 Ion 100.00 (99.70 to 100.70): VW



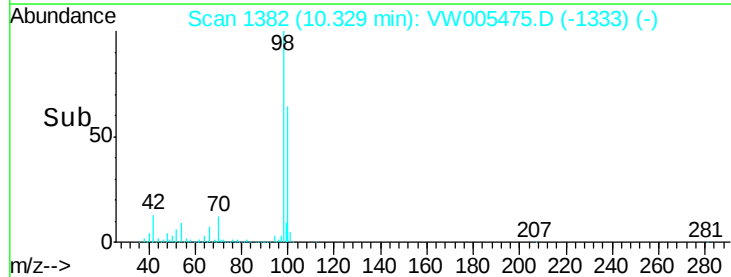
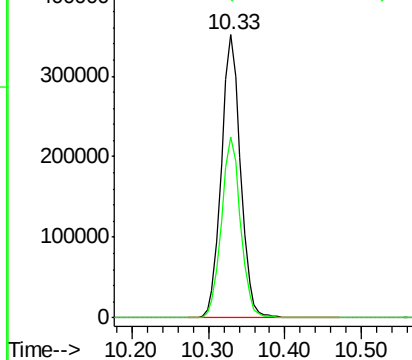


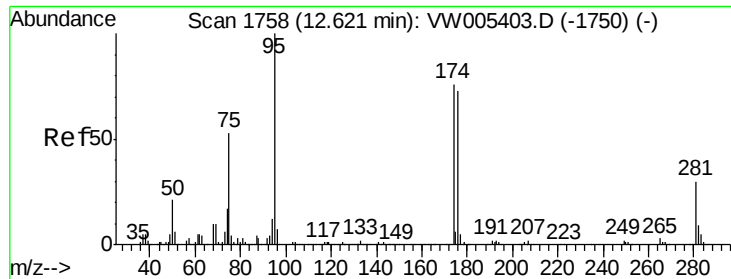

#62
4-Bromofluorobenzene
Concen: 47.28 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. -0.00 min
Lab File: VW005475.D
Acq: 18 Sep 2018 13:33




Instrument :
MSVOA_W
ClientSampleId :
VW0918SBL01




Tot Ion: 95 Resp: 216628
Ion Ratio Lower Upper
95 100
174 79.4 0.0 161.2
176 76.2 0.0 156.6

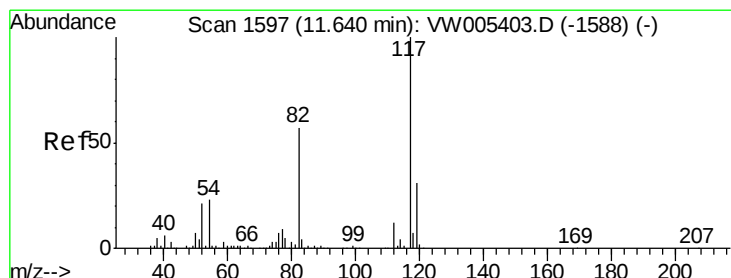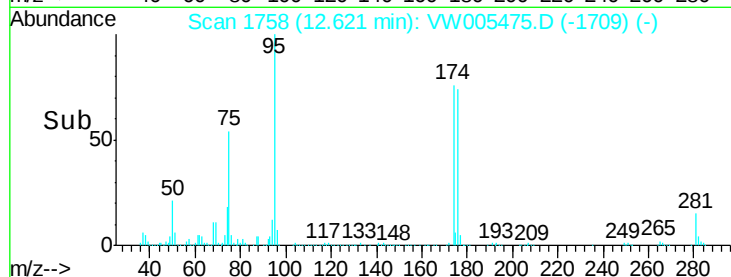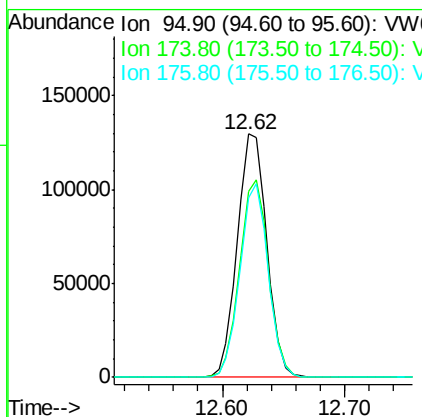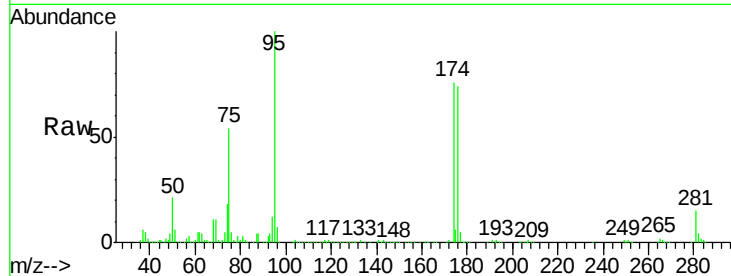

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.01 min
Lab File: VW005475.D
Acq: 18 Sep 2018 13:33

Tgt Ion: 117 Resp: 465185
Ion Ratio Lower Upper
117 100
82 58.9 45.9 68.9
119 31.9 24.8 37.2

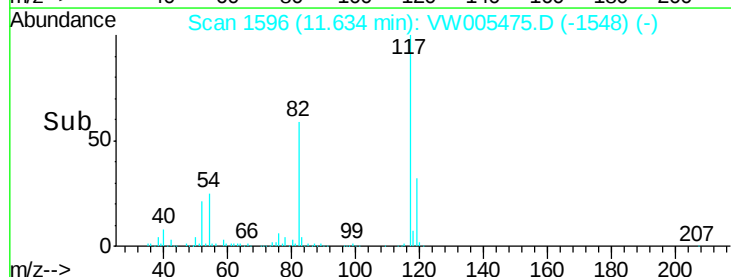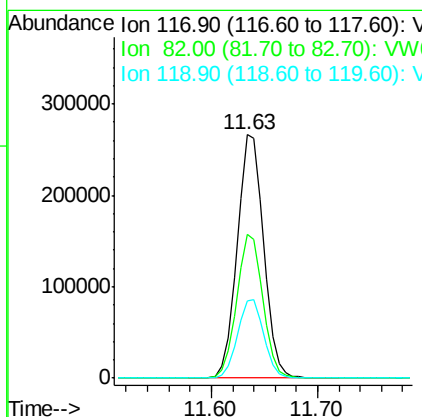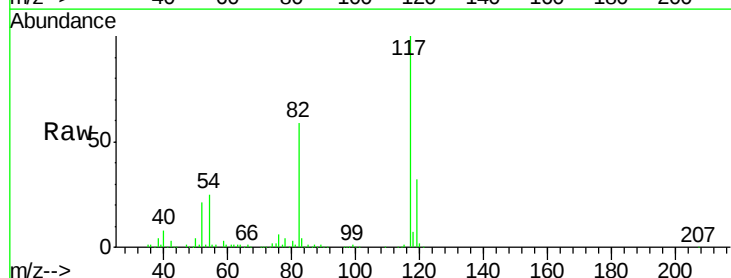

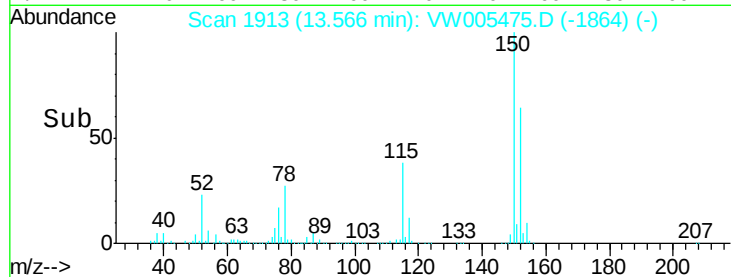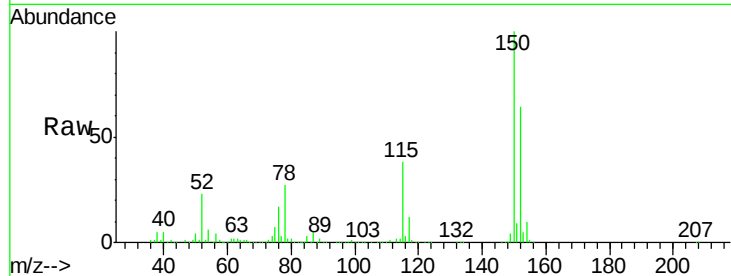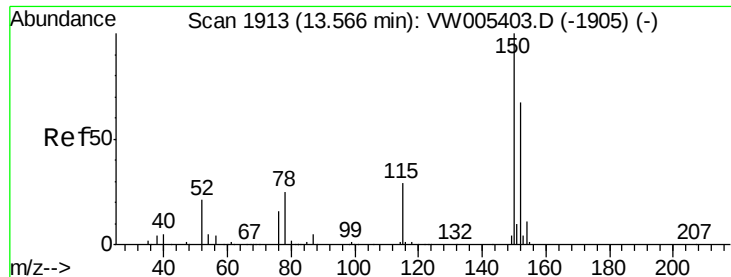

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.57 min Scan# 1913

Delta R.T. -0.00 min

Lab File: VW005475.D

Acq: 18 Sep 2018 13:33

Instrument :

MSVOA_W

ClientSampleId :

VW0918SBL01

Tot Ion:152 Resp: 229420

Ion Ratio Lower Upper

152 100

115 59.9 29.5 88.5

150 157.8 0.0 345.6

