

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW091819\
 Data File : VW013120.D
 Acq On : 18 Sep 2019 18:11
 Operator : SY/VA
 Sample : K4923-09
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SB-46-9.5-10.0

Quant Time: Sep 19 09:03:00 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 13 17:26:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	332793	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	499804	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	417621	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.55	152	180385	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	136003	44.25	ug/l	0.00
Spiked Amount	50.000		Recovery	=	88.50%	
35) Dibromofluoromethane	7.88	113	138090	50.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.84%	
50) Toluene-d8	10.32	98	580382	54.69	ug/l	0.00
Spiked Amount	50.000		Recovery	=	109.38%	
62) 4-Bromofluorobenzene	12.62	95	178625	46.81	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.62%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW091819\
Data File : VW013120.D
Acq On : 18 Sep 2019 18:11
Operator : SY/VA
Sample : K4923-09
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SB-46-9.5-10.0

Quant Time: Sep 19 09:03:00 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Quant Title : SW846 8260
QLast Update : Fri Sep 13 17:26:01 2019
Response via : Initial Calibration

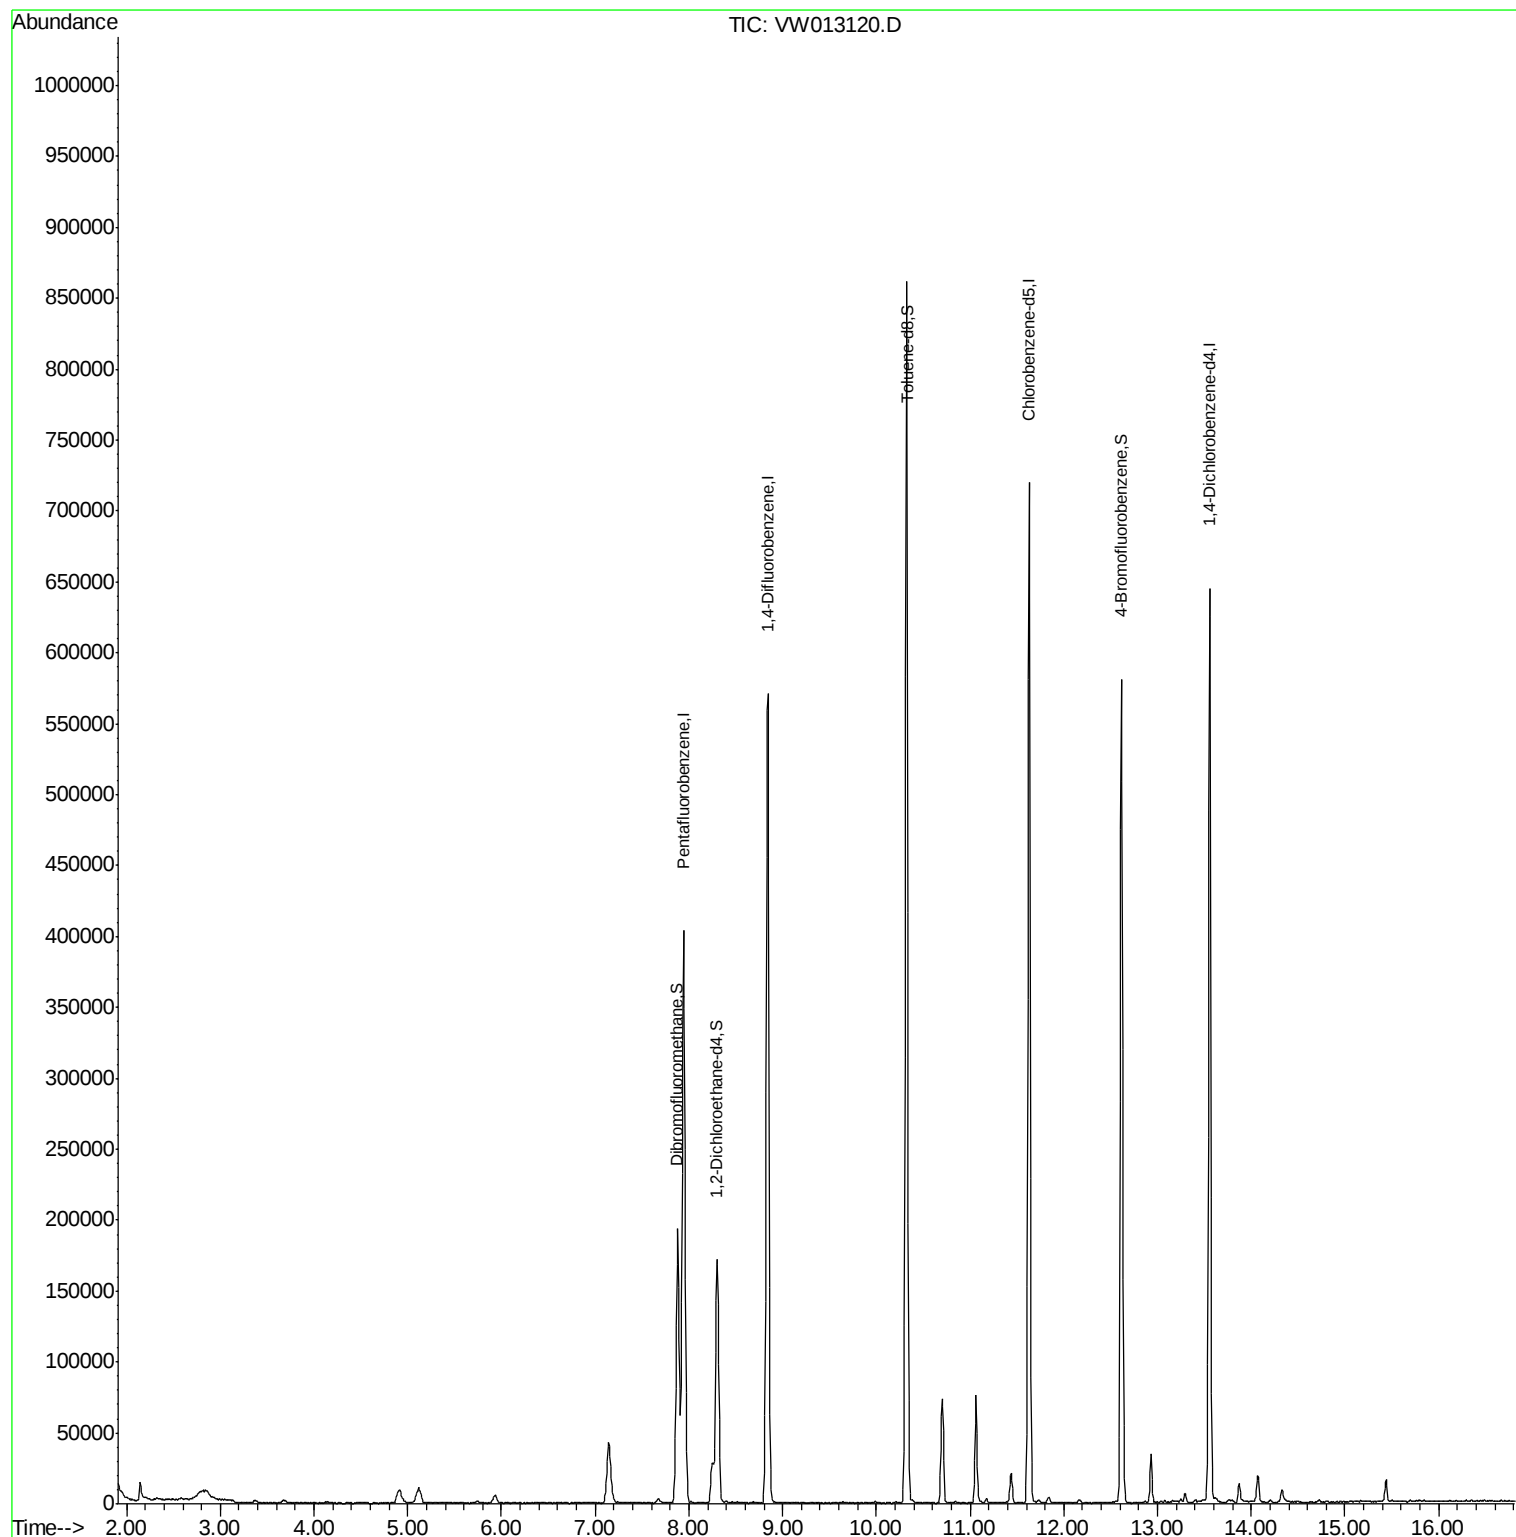

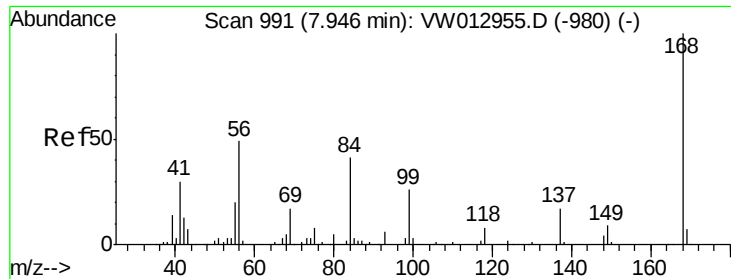

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW013120.D

Acq: 18 Sep 2019 18:11

Instrument :

MSVOA_W

ClientSampleId :


SB-46-9.5-10.0

Tot Ion:168 Resp: 332793

Ion Ratio Lower Upper

168 100

99 48.4 46.2 69.2

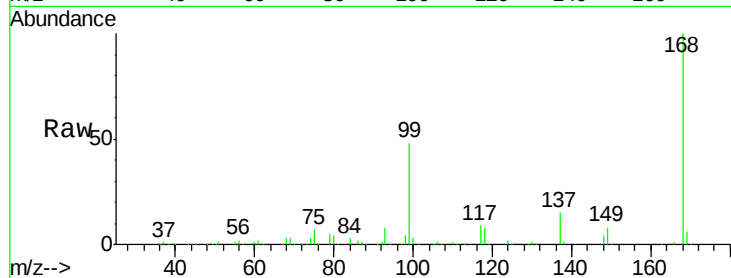

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95



150000

100000

50000

0

Time--> 7.80 7.90 8.00 8.10

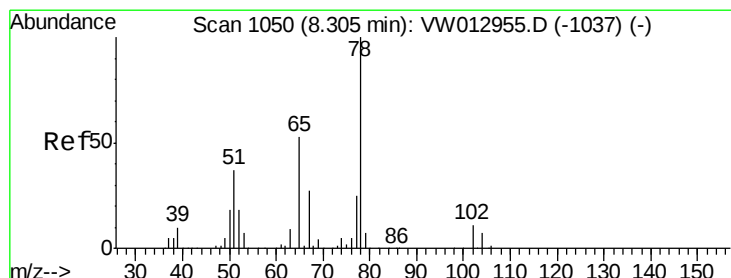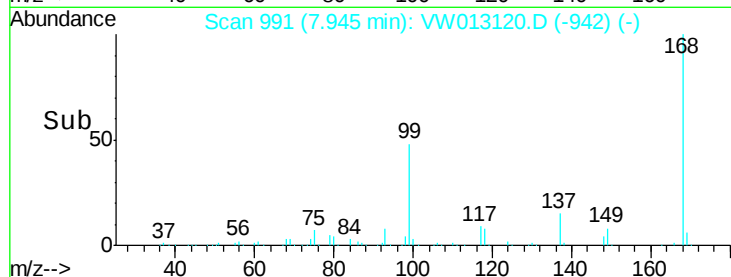

#33

1,2-Dichloroethane-d4

Concen: 44.249 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW013120.D


Acq: 18 Sep 2019 18:11

Tgt Ion: 65 Resp: 136003

Ion Ratio Lower Upper

65 100

67 53.6 0.0 101.2

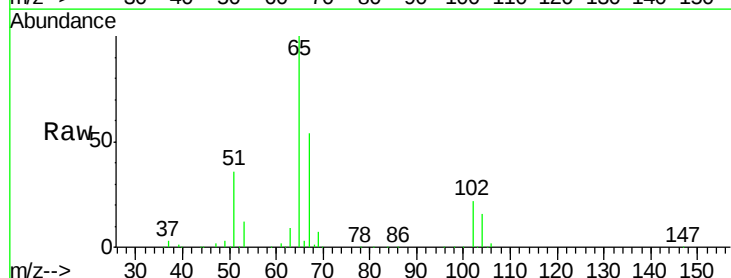

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31


60000


40000

20000

0

Time--> 8.20 8.25 8.30 8.35 8.40

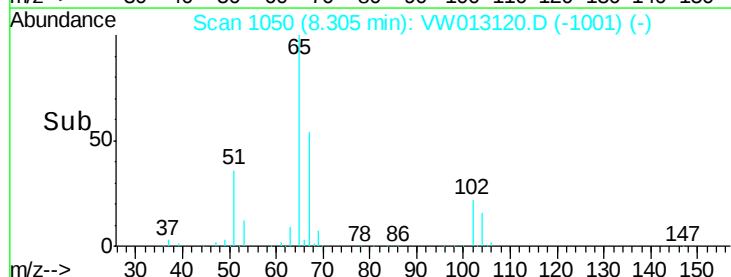

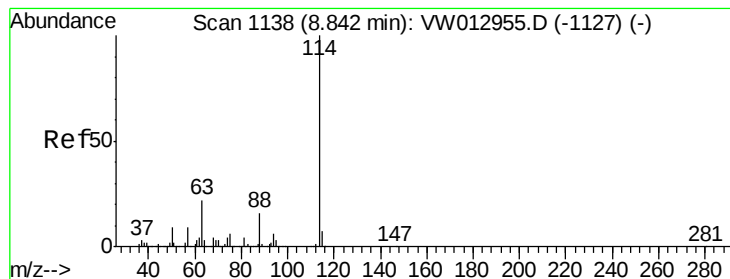

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. -0.00 min

Lab File: VW013120.D

Acq: 18 Sep 2019 18:11

Instrument :

MSVOA_W

ClientSampleId :

SB-46-9.5-10.0


Tot Ion:114 Resp: 499804

Ion Ratio Lower Upper

114 100

63 19.8 0.0 43.4




88 14.9 0.0 31.6

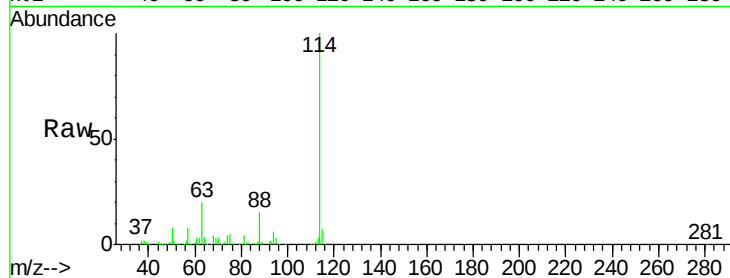

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

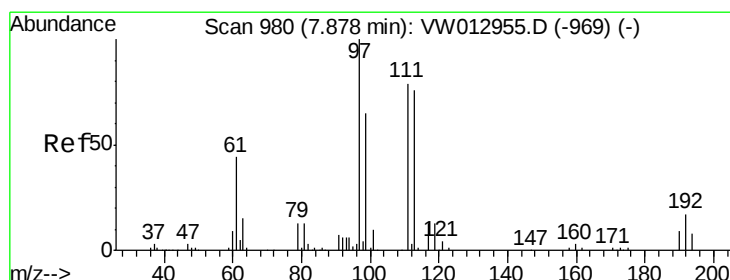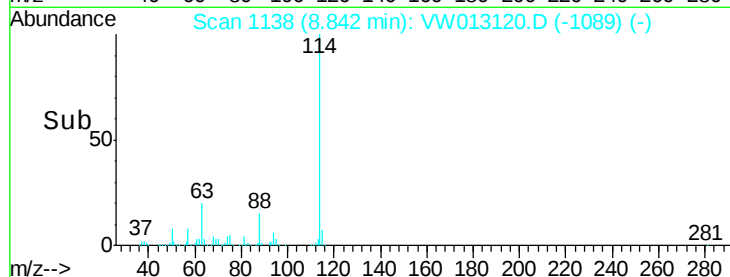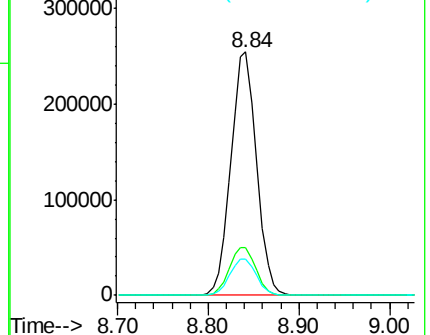

#35

Dibromofluoromethane

Concen: 50.918 ug/l

RT: 7.88 min Scan# 980

Delta R.T. -0.00 min

Lab File: VW013120.D

Acq: 18 Sep 2019 18:11


Tgt Ion:113 Resp: 138090

Ion Ratio Lower Upper

113 100

111 103.6 82.8 124.2



192 23.1 17.8 26.8

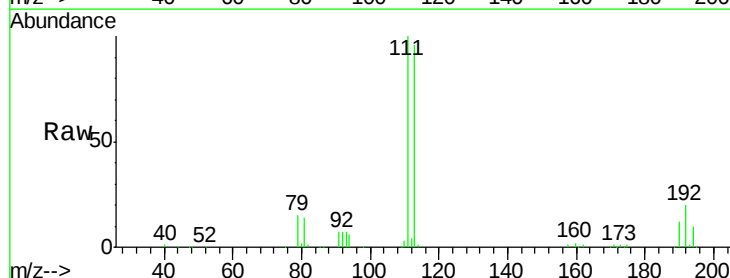


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

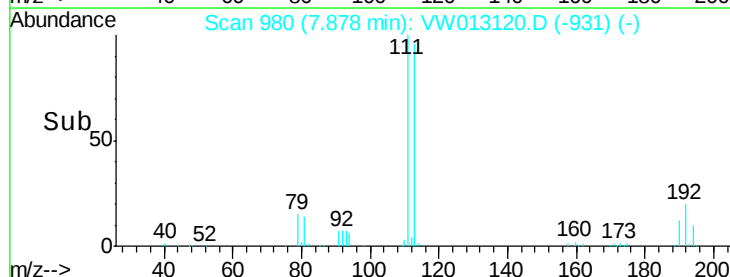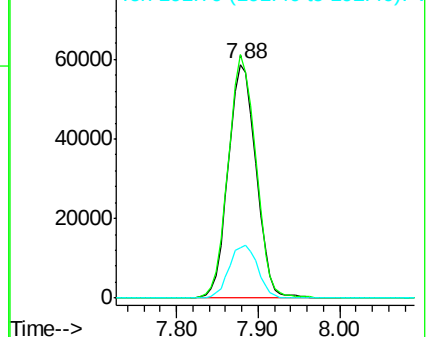

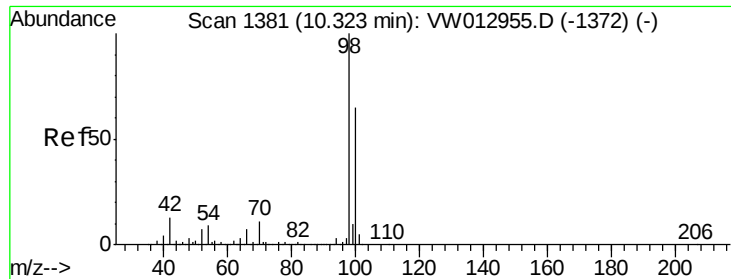

#50

Toluene-d8

Concen: 54.689 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.00 min

Lab File: VW013120.D

Acq: 18 Sep 2019 18:11

Instrument :

MSVOA_W

ClientSampleId :


SB-46-9.5-10.0

Tot Ion: 98 Resp: 580382

Ion Ratio Lower Upper




98 100

100 65.8 52.1 78.1

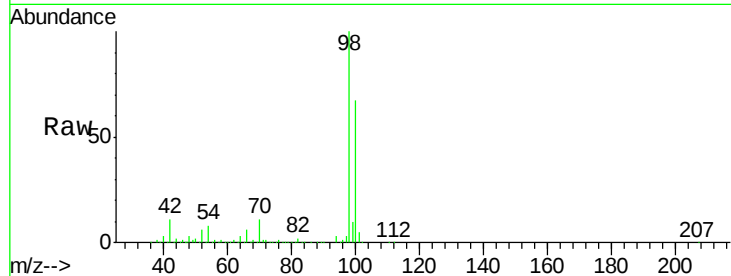

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

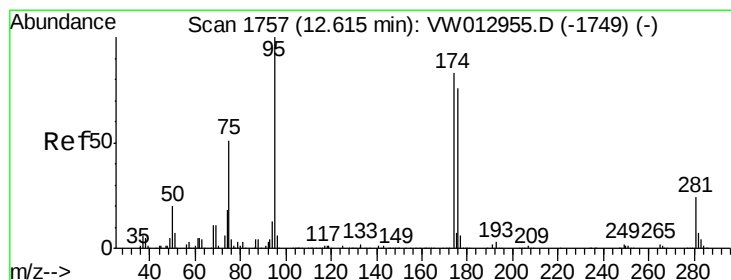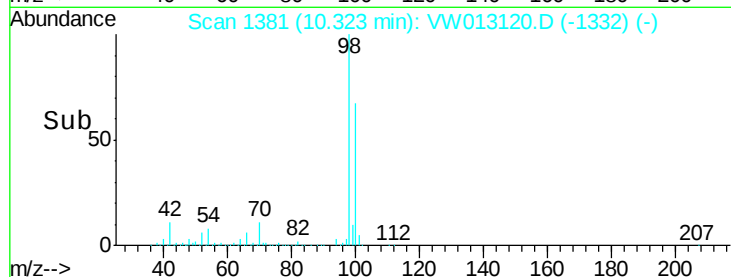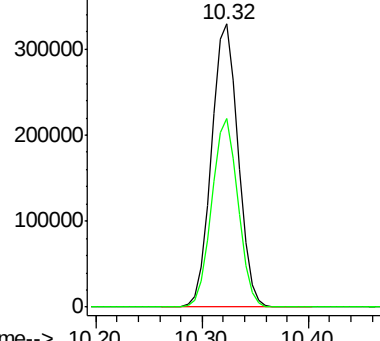

#62

4-Bromofluorobenzene

Concen: 46.810 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. -0.00 min

Lab File: VW013120.D

Acq: 18 Sep 2019 18:11


Tgt Ion: 95 Resp: 178625

Ion Ratio Lower Upper

95 100

174 87.9 0.0 170.4



176 84.1 0.0 164.6

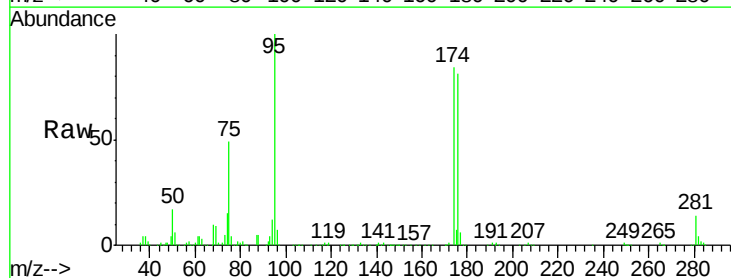

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



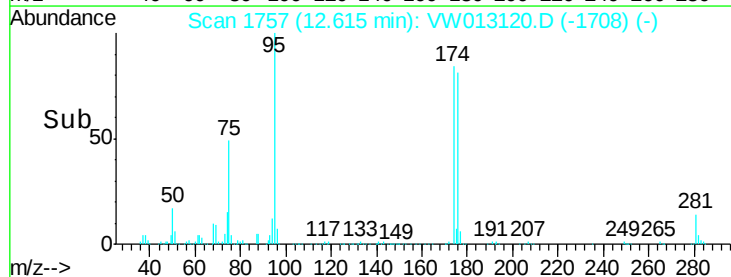
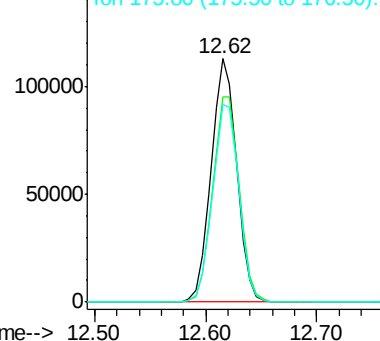




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1595
Delta R.T. -0.00 min
Lab File: VW013120.D
Acq: 18 Sep 2019 18:11

Instrument :
MSVOA_W
ClientSampleId :
SB-46-9.5-10.0

Tot Ion:117 Resp: 417621
Ion Ratio Lower Upper
117 100
82 54.9 46.3 69.5
119 31.6 26.2 39.4

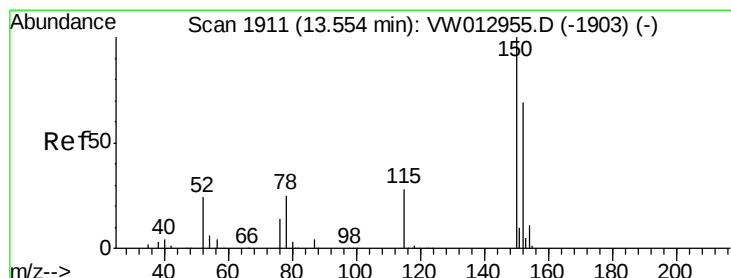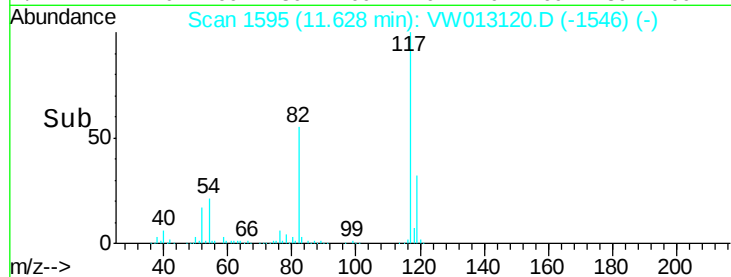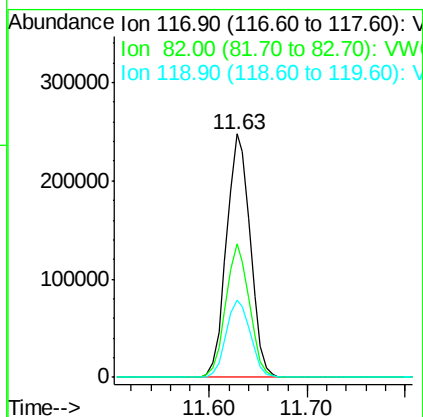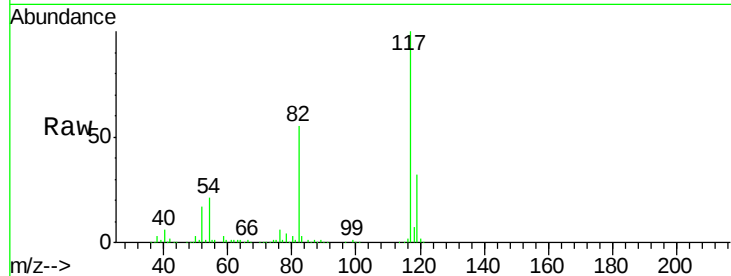

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.55 min Scan# 1911
Delta R.T. -0.00 min
Lab File: VW013120.D
Acq: 18 Sep 2019 18:11

Tgt Ion:152 Resp: 180385
Ion Ratio Lower Upper
152 100
115 56.1 28.8 86.4
150 155.6 0.0 340.2

