

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW091819\
 Data File : VW013146.D
 Acq On : 19 Sep 2019 07:07
 Operator : SY/VA
 Sample : K4825-07
 Misc : 5.87G/5ML/MSVOA W/SOIL
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 CSA-4-1-2

Quant Time: Sep 19 09:53:15 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 13 17:26:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	358889	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	546817	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	377106	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	102161	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	162012	48.88	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.76%	
35) Dibromofluoromethane	7.88	113	154205	51.97	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.94%	
50) Toluene-d8	10.32	98	579280	49.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.78%	
62) 4-Bromofluorobenzene	12.62	95	133852	32.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	64.12%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW091819\
Data File : VW013146.D
Acq On : 19 Sep 2019 07:07
Operator : SY/VA
Sample : K4825-07
Misc : 5.87G/5ML/MSVOA W/SOIL
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
CSA-4-1-2

Quant Time: Sep 19 09:53:15 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
Quant Title : SW846 8260
QLast Update : Fri Sep 13 17:26:01 2019
Response via : Initial Calibration

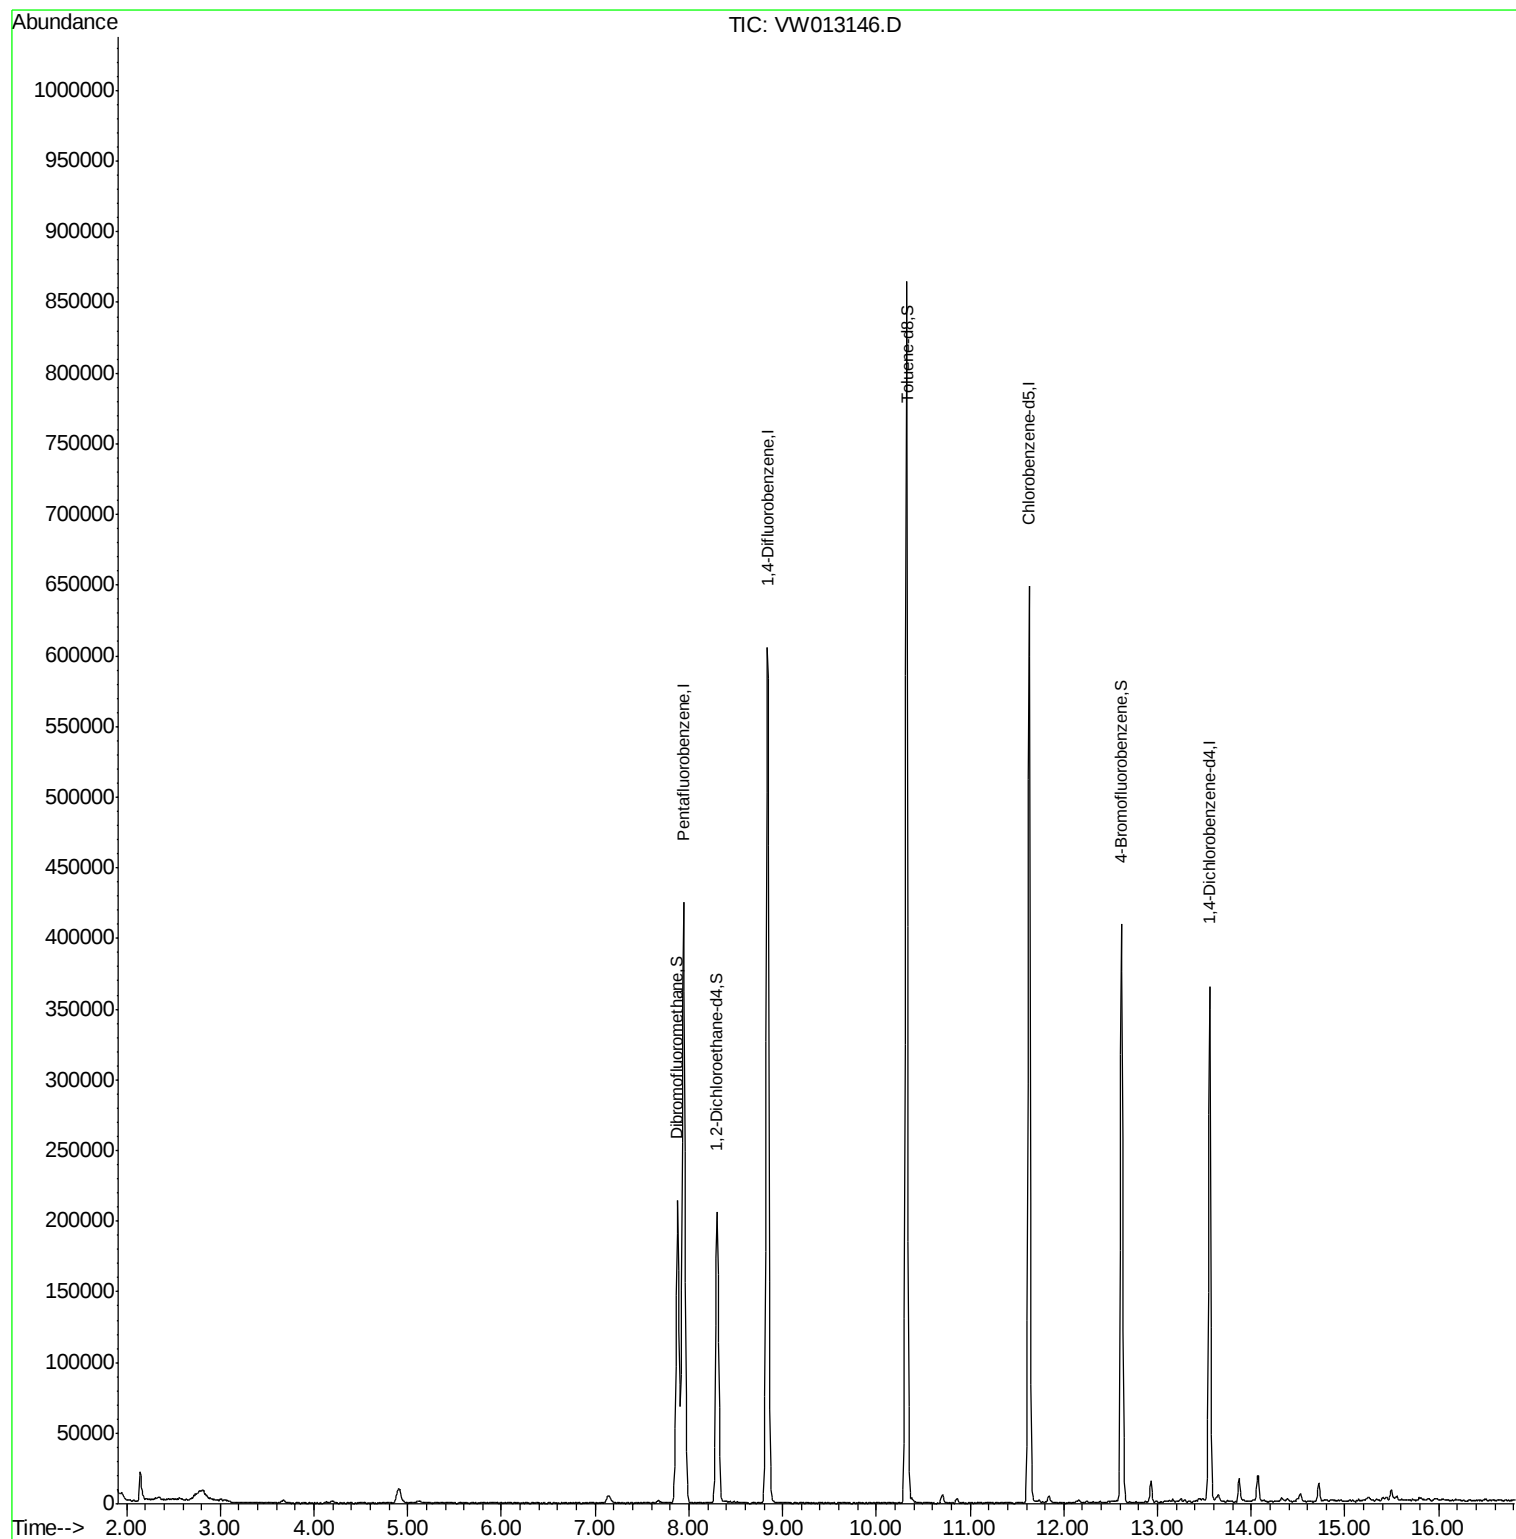

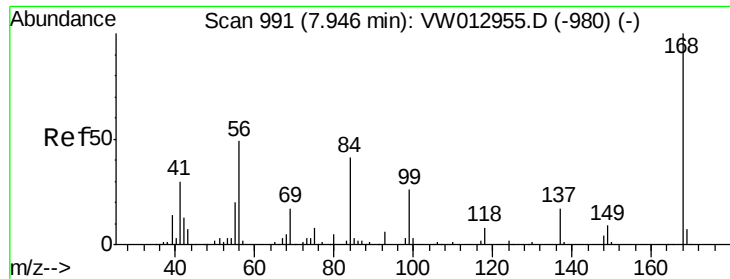

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW013146.D

Acq: 19 Sep 2019 07:07

Instrument :

MSVOA_W

ClientSampled :


CSA-4-1-2

Tot Ion:168 Resp: 358889

Ion Ratio Lower Upper




168 100

99 47.5 46.2 69.2

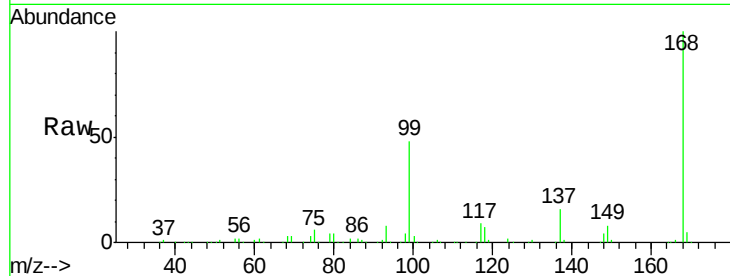

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

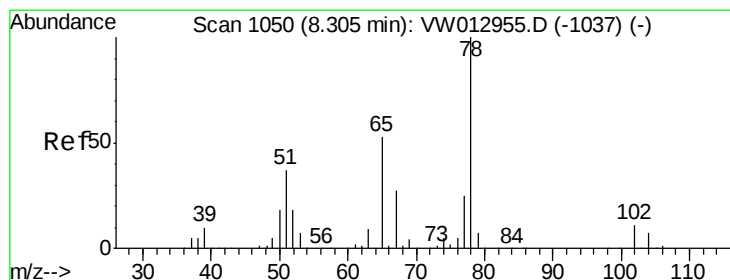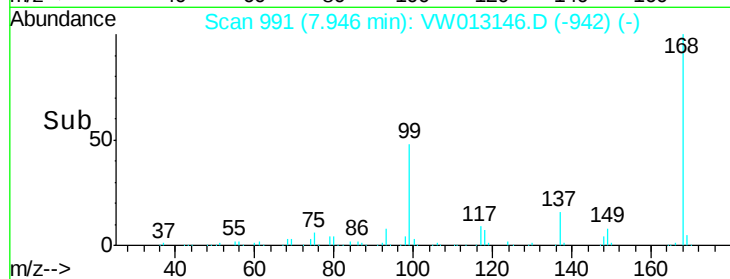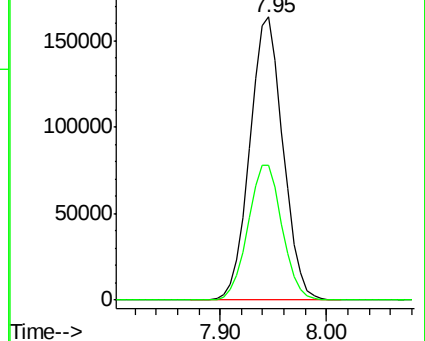

#33

1,2-Dichloroethane-d4

Concen: 48.878 ug/l

RT: 8.30 min Scan# 1049

Delta R.T. -0.01 min

Lab File: VW013146.D


Acq: 19 Sep 2019 07:07

Tgt Ion: 65 Resp: 162012

Ion Ratio Lower Upper



65 100


67 53.8 0.0 101.2

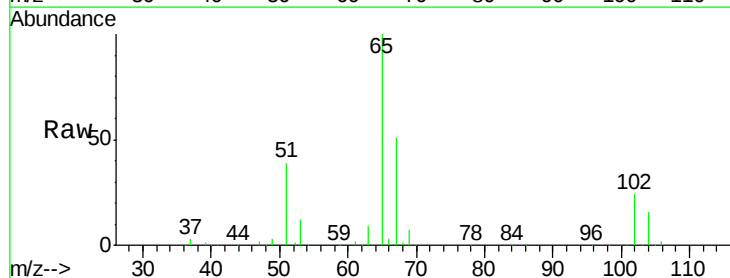

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

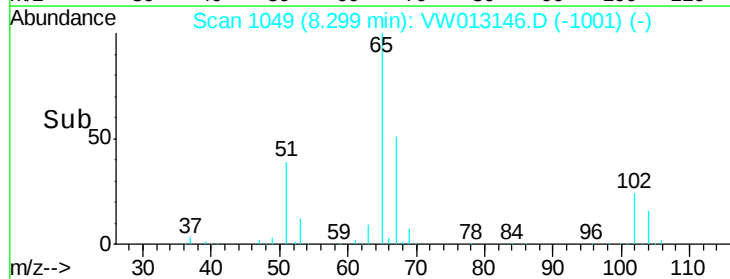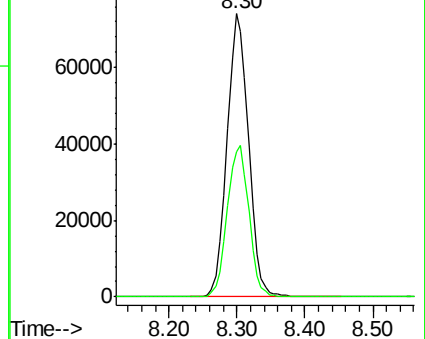

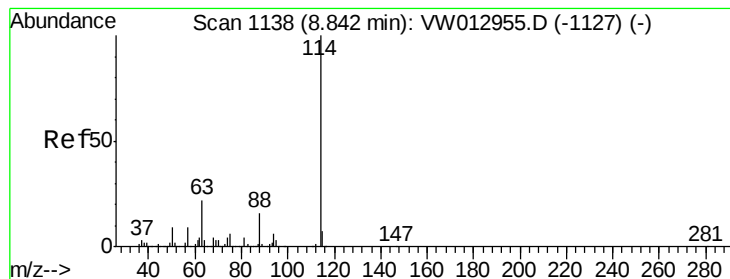

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1137

Delta R.T. -0.01 min

Lab File: VW013146.D

Acq: 19 Sep 2019 07:07

Instrument :

MSVOA_W

ClientSampleId :

CSA-4-1-2


Tot Ion:114 Resp: 546817

Ion Ratio Lower Upper

114 100

63 21.1 0.0 43.4




88 16.2 0.0 31.6

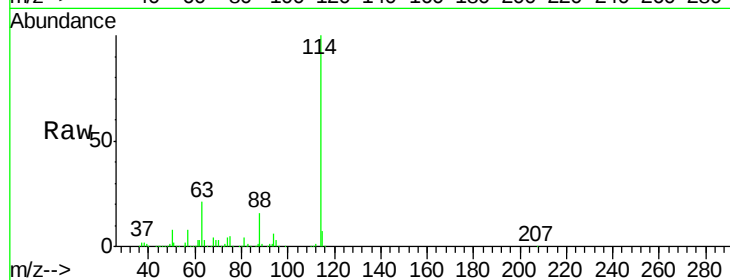

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

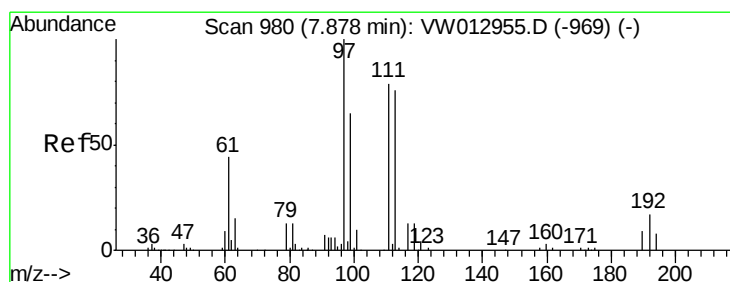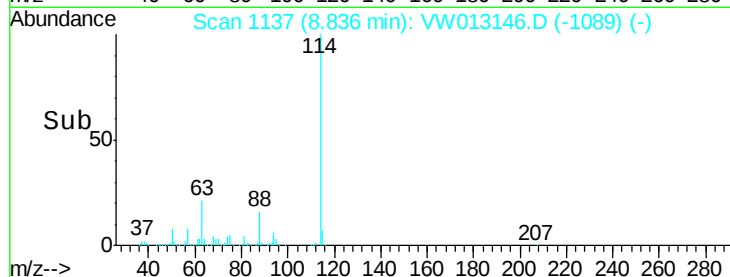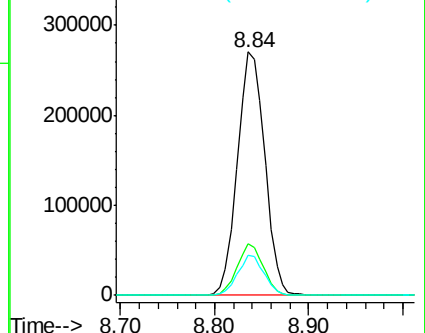

#35

Dibromofluoromethane

Concen: 51.972 ug/l

RT: 7.88 min Scan# 980

Delta R.T. 0.00 min

Lab File: VW013146.D

Acq: 19 Sep 2019 07:07


Tgt Ion:113 Resp: 154205

Ion Ratio Lower Upper

113 100

111 103.7 82.8 124.2



192 24.1 17.8 26.8

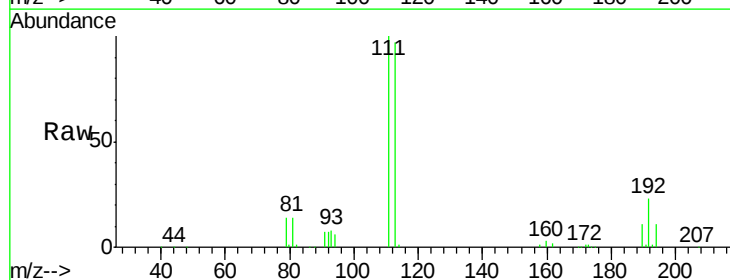


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

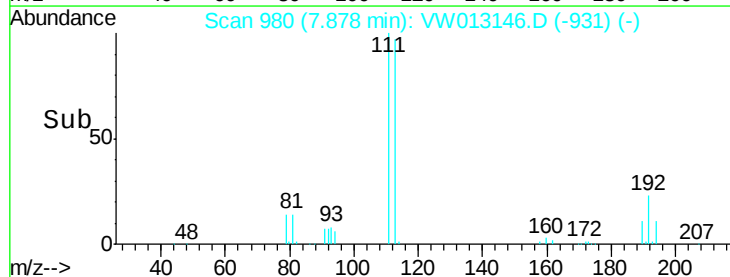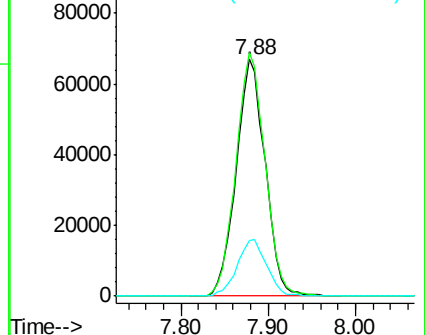

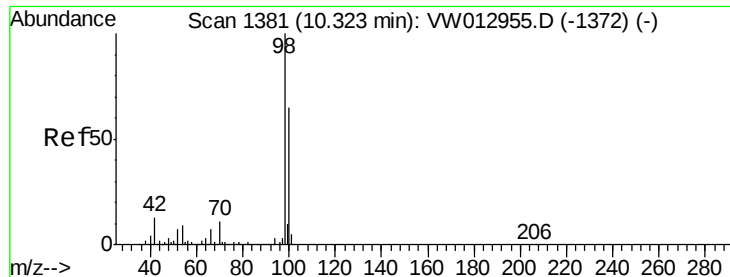

#50

Toluene-d8

Concen: 49.892 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW013146.D

Acq: 19 Sep 2019 07:07

Instrument :

MSVOA_W

ClientSampleId :





CSA-4-1-2

Tot Ion: 98 Resp: 579280

Ion Ratio Lower Upper

98 100

100 66.7 52.1 78.1

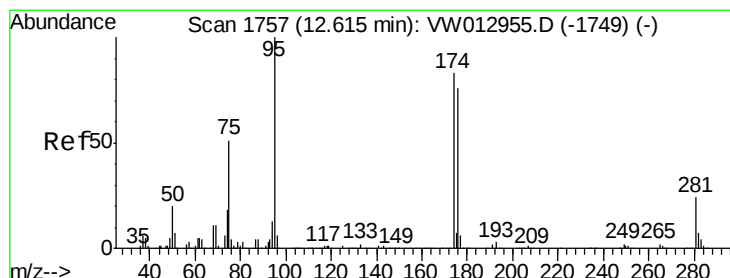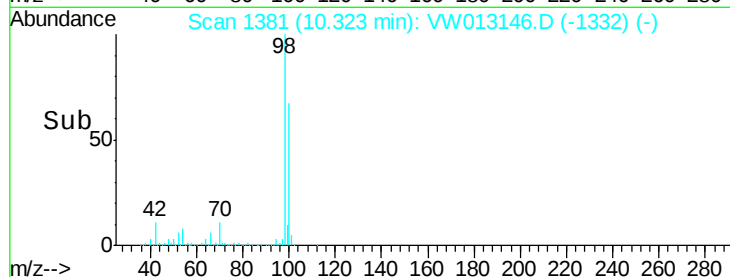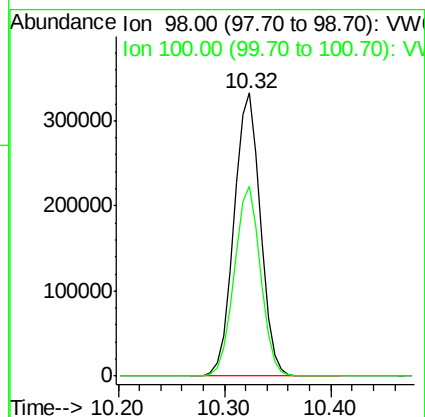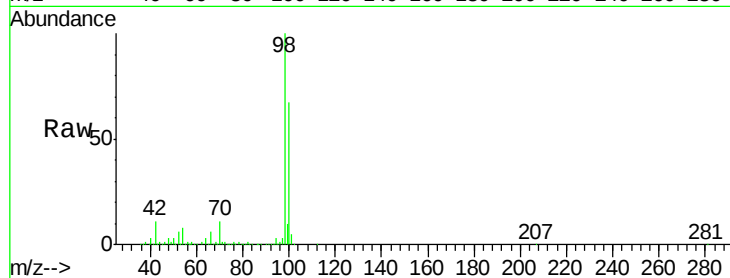

#62

4-Bromofluorobenzene

Concen: 32.061 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. 0.00 min

Lab File: VW013146.D

Acq: 19 Sep 2019 07:07




Tgt Ion: 95 Resp: 133852


Ion Ratio Lower Upper

95 100

174 90.7 0.0 170.4

176 86.9 0.0 164.6


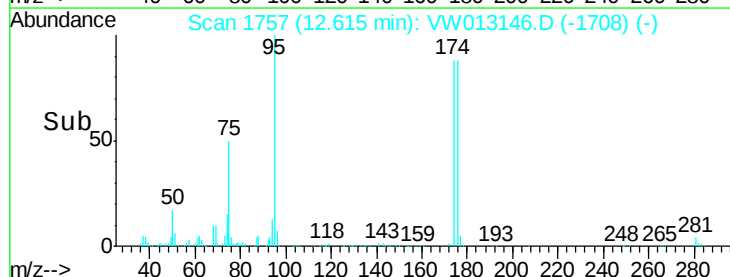
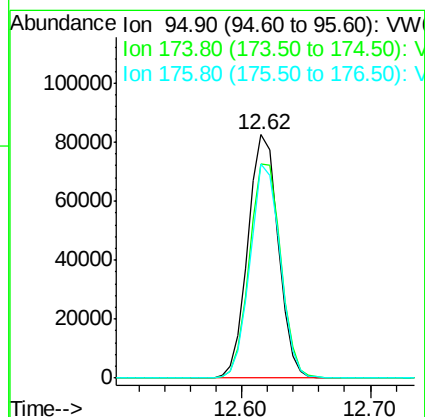
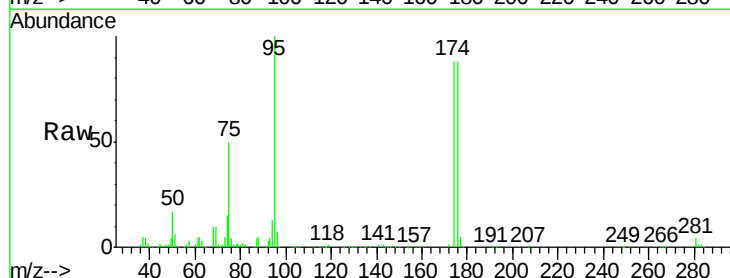


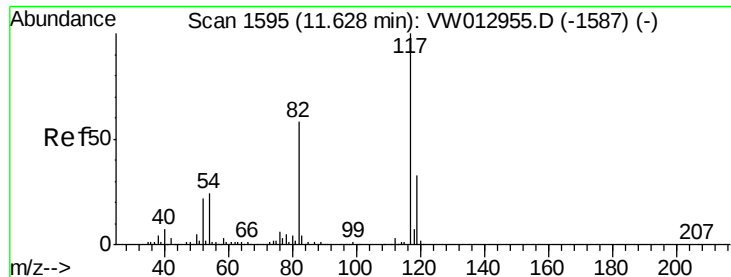

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1595
Delta R.T. 0.00 min
Lab File: VW013146.D
Acq: 19 Sep 2019 07:07

Instrument :
MSVOA_W
ClientSampleId :
CSA-4-1-2

Tot Ion	Ratio	Lower	Upper
117	100		
82	53.6	46.3	69.5
119	31.9	26.2	39.4

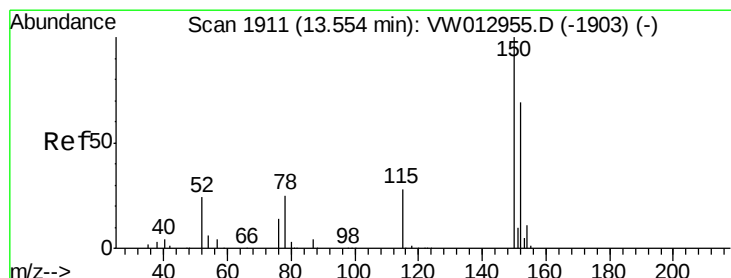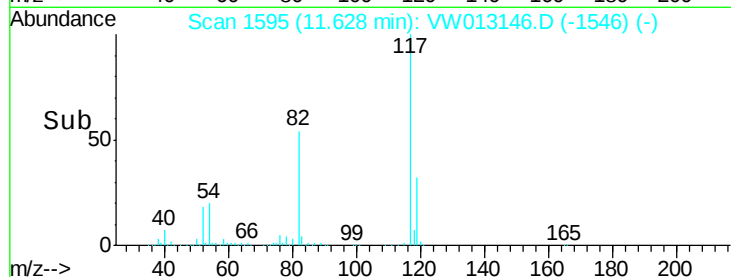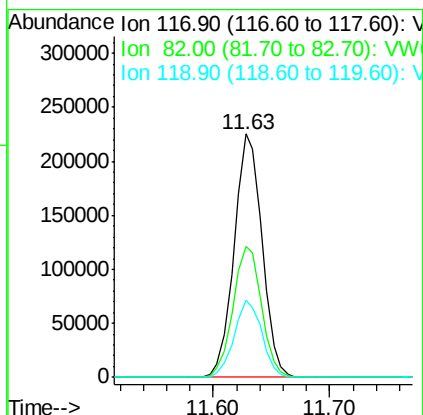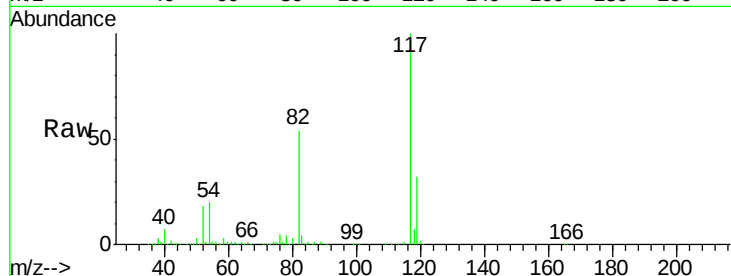

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. 0.01 min
Lab File: VW013146.D
Acq: 19 Sep 2019 07:07

Tgt Ion	Ratio	Lower	Upper
152	100		
115	56.1	28.8	86.4
150	157.1	0.0	340.2

