


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW091819\
 Data File : VW013129.D
 Acq On : 18 Sep 2019 22:29
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W091419S.M
 Title : SW846 8260
 Last Update : Fri Sep 13 17:26:01 2019

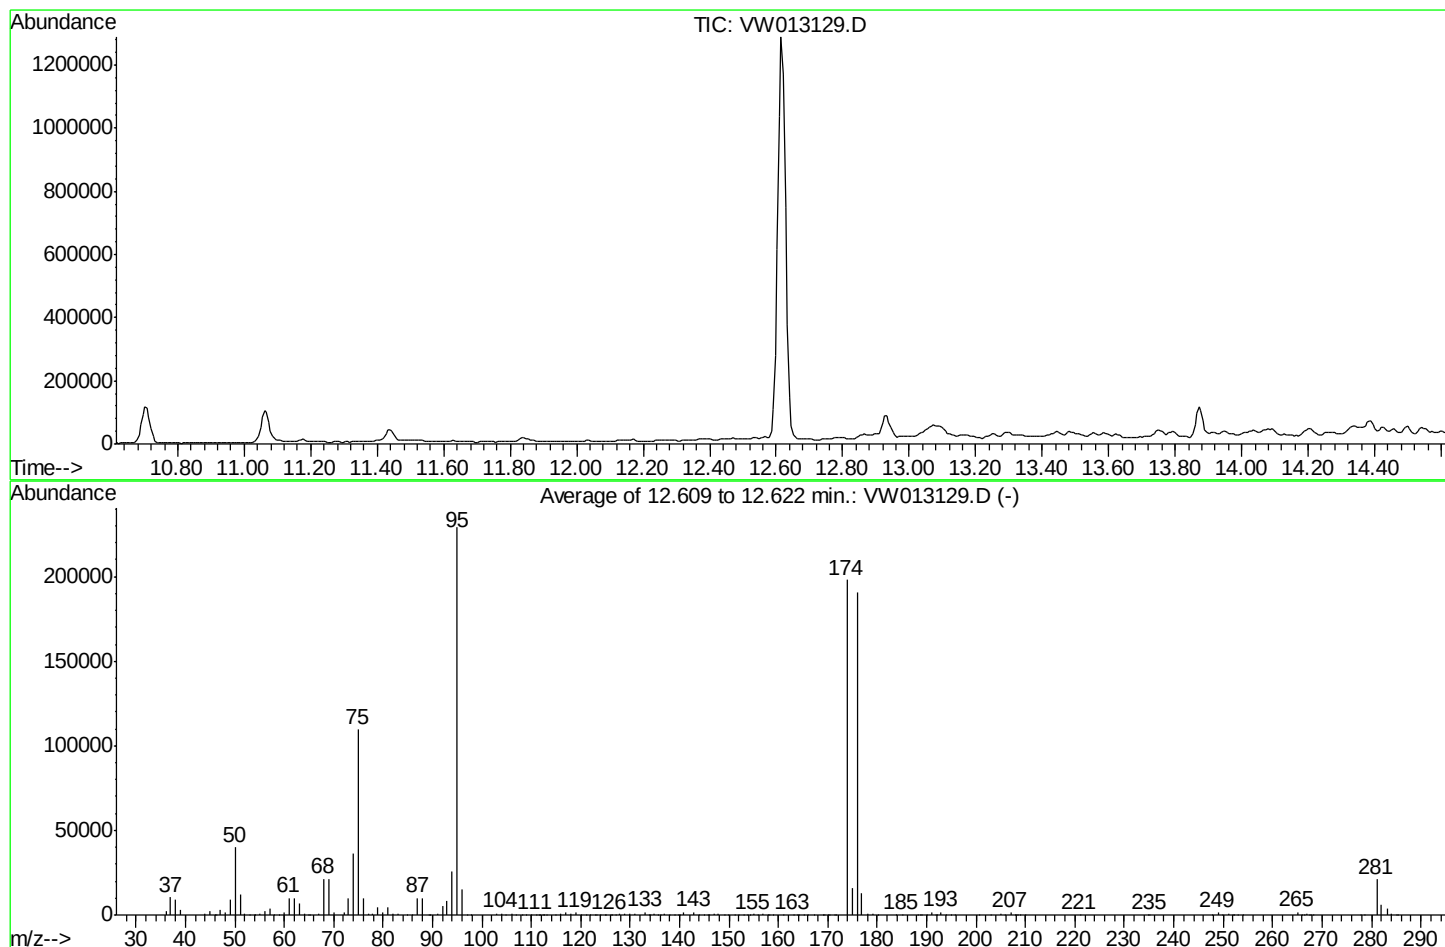

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	40088	PASS
75	95	30	60	47.8	109581	PASS
95	95	100	100	100.0	229106	PASS
96	95	5	9	6.5	15001	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.5	198165	PASS
175	174	5	9	8.2	16213	PASS
176	174	95	101	96.1	190400	PASS
177	176	5	9	6.6	12583	PASS