

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW091820\
 Data File : VW016584.D
 Acq On : 18 Sep 2020 14:30
 Operator : SY/VA
 Sample : VW0918SBL03
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK103

Quant Time: Sep 19 00:37:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SFAMWLM091820SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 18 13:07:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	595663	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	526314	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.56	152	253039	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	163007	24.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.00%
7) Chloroethane-d5	2.90	69	129746	23.75	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.00%
11) 1,1-Dichloroethene-d2	4.03	63	245936	17.52	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.08%
21) 2-Butanone-d5	7.09	46	75959	50.48	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.96%
24) Chloroform-d	7.65	84	344052	24.51	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.04%
26) 1,2-Dichloroethane-d4	8.31	65	184051	25.68	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.72%
32) Benzene-d6	8.28	84	681460	25.35	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.40%
36) 1,2-Dichloropropane-d6	9.28	67	186969	25.29	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.16%
41) Toluene-d8	10.33	98	642934	24.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.08%
43) trans-1,3-Dichloropropene-	10.58	79	88728	24.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.96%
47) 2-Hexanone-d5	10.93	63	60814	52.27	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.54%
56) 1,1,2,2-Tetrachloroethane-	12.69	84	148096	25.73	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.92%
66) 1,2-Dichlorobenzene-d4	13.86	152	238645	26.04	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.16%


Target Compounds					Ovalue
16) Methylene chloride	4.93	84	18306	2.097 ug/L	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW091820\
Data File : VW016584.D
Acq On : 18 Sep 2020 14:30
Operator : SY/VA
Sample : VW0918SBL03
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK103

Quant Time: Sep 19 00:37:24 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SFAMWLM091820SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 18 13:07:26 2020
Response via : Initial Calibration

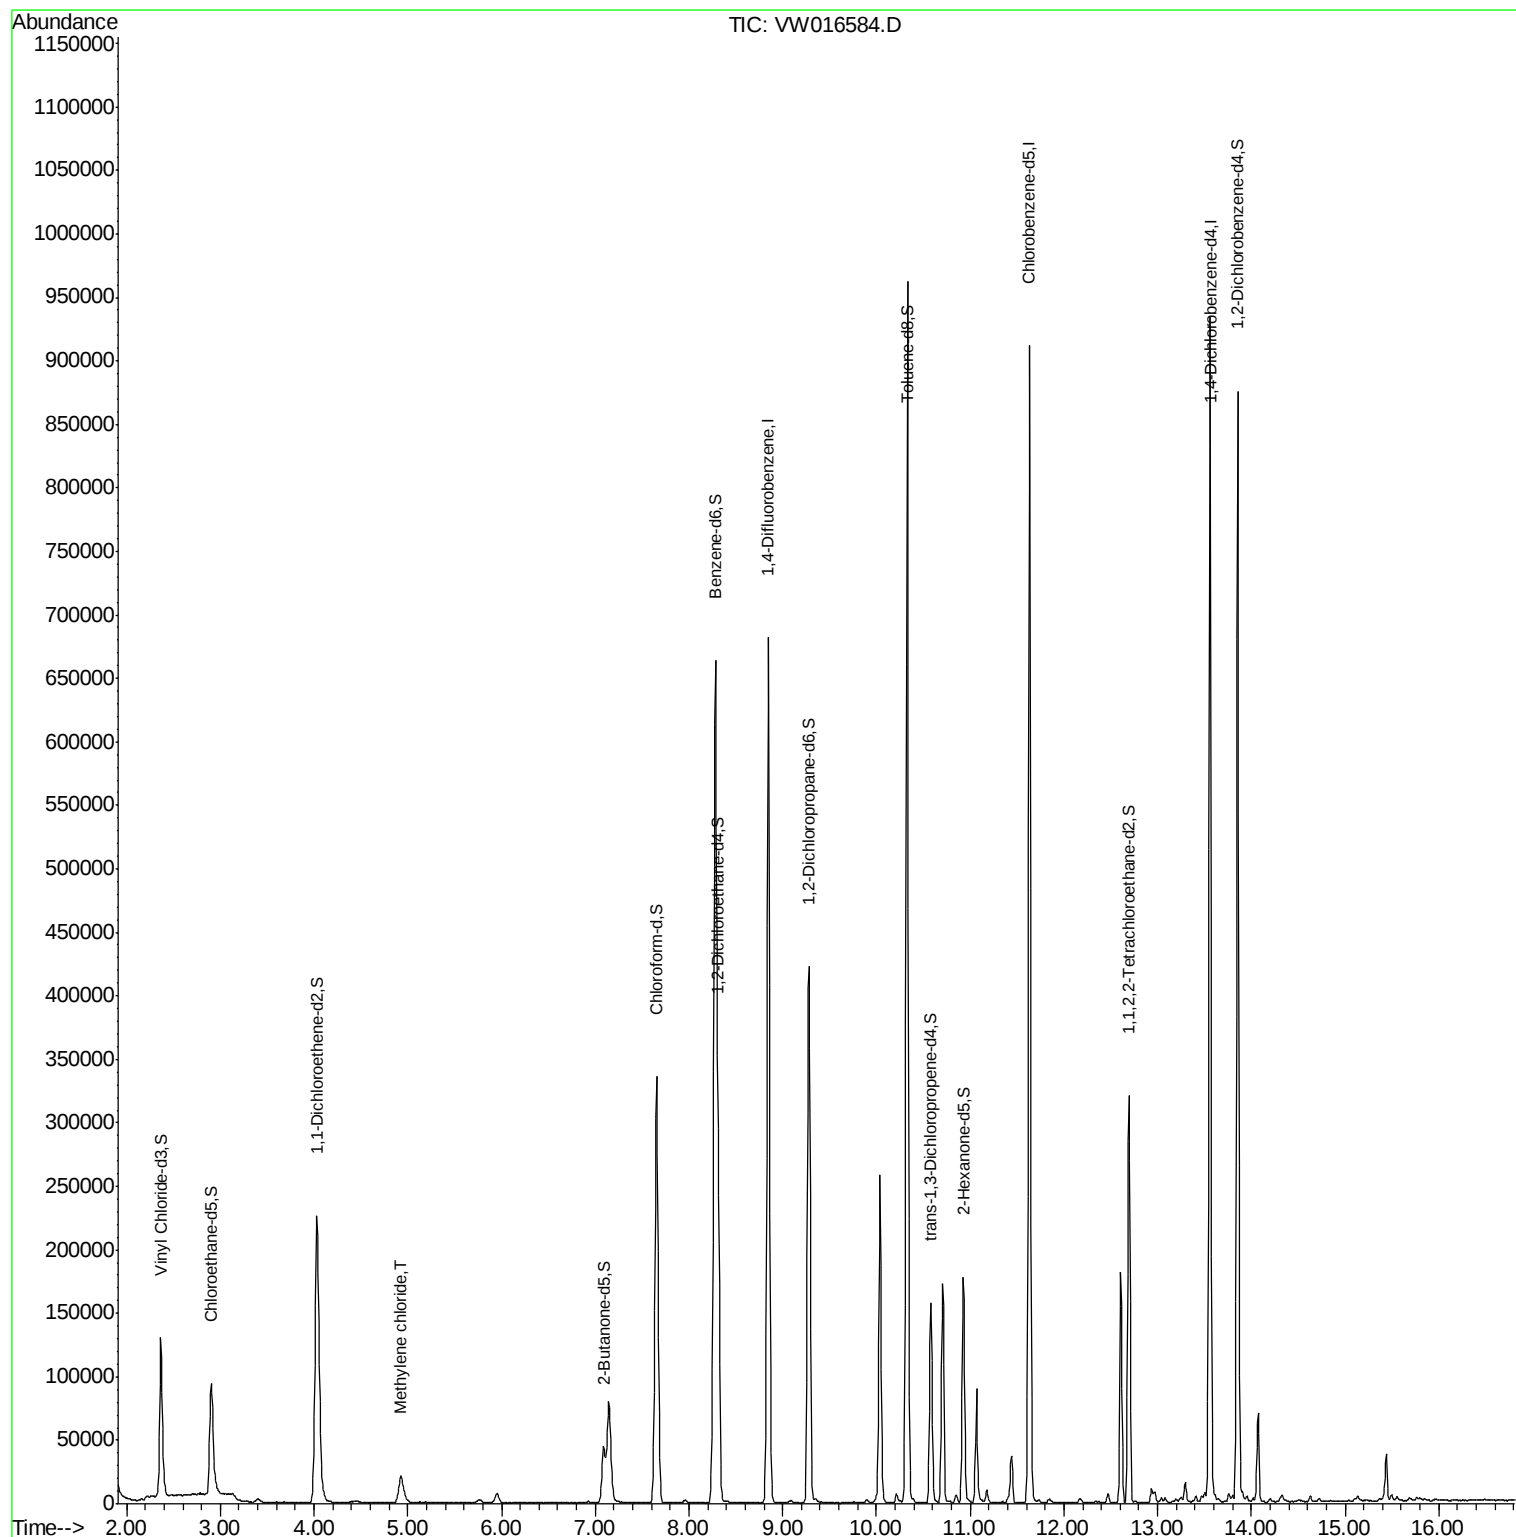

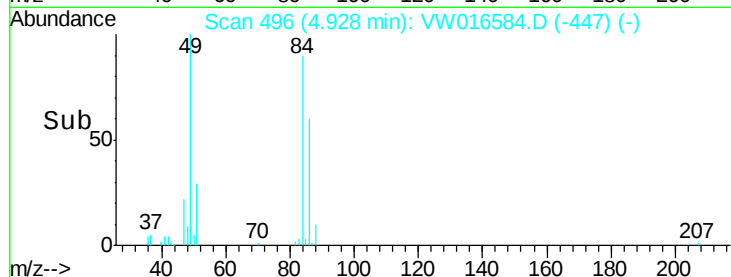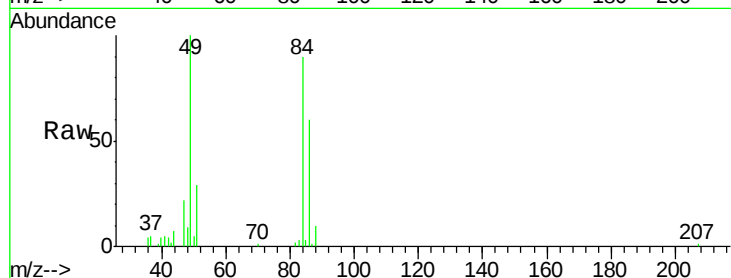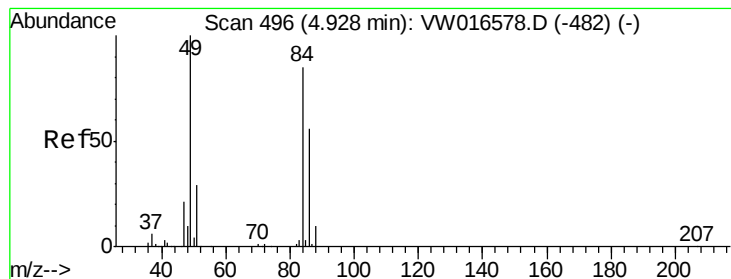

#16
Methylene chloride
Concen: 2.097 ug/L
RT: 4.93 min Scan# 496
Delta R.T. 0.00 min
Lab File: VW016584.D
Acq: 18 Sep 2020 14:30

Instrument :
MSVOA_W
ClientSampleId :
VBLK103

Tot Ion: 84 Resp: 18306

Ion	Ratio	Lower	Upper
84	100		
86	66.4	46.2	85.8
49	111.0	82.8	153.8

