

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091823\
 Data File : VW027129.D
 Acq On : 18 Sep 2023 16:03
 Operator : SY/MD
 Sample : 04472-04
 Misc : 4.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 18 22:38:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Sep 18 22:36:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	534602	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	358199	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	82051	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	121303	14.103	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	56.400%	
7) Chloroethane-d5	2.893	69	118572	17.851	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	71.400%	
11) 1,1-Dichloroethene-d2	4.015	65	57662	15.636	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	62.560%	
21) 2-Butanone-d5	7.081	46	79295	49.787	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	99.580%	
24) Chloroform-d	7.648	84	334782	20.844	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	83.360%	
26) 1,2-Dichloroethane-d4	8.051	65	97	0.012	ug/L	-0.26
Spiked Amount	25.000	Range 70 - 130	Recovery	=	0.040%#	
32) Benzene-d6	8.276	84	685557	29.636	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	118.560%	
36) 1,2-Dichloropropane-d6	9.276	67	212838	32.516	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	130.080%#	
41) Toluene-d8	10.325	98	502735	24.419	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	97.680%	
43) trans-1,3-Dichloroprop...	10.575	79	44964	16.999	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	68.000%	
47) 2-Hexanone-d5	10.922	63	37683	47.777	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	95.560%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	158901	30.298	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	121.200%#	
66) 1,2-Dichlorobenzene-d4	13.855	152	83662	28.552	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	114.200%	
Target Compounds					Qvalue	
48) 2-Hexanone	10.922	43	4829	2.541	ug/L #	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091823\
Data File : VW027129.D
Acq On : 18 Sep 2023 16:03
Operator : SY/MD
Sample : 04472-04
Misc : 4.82g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Sep 18 22:38:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Sep 18 22:36:33 2023
Response via : Initial Calibration

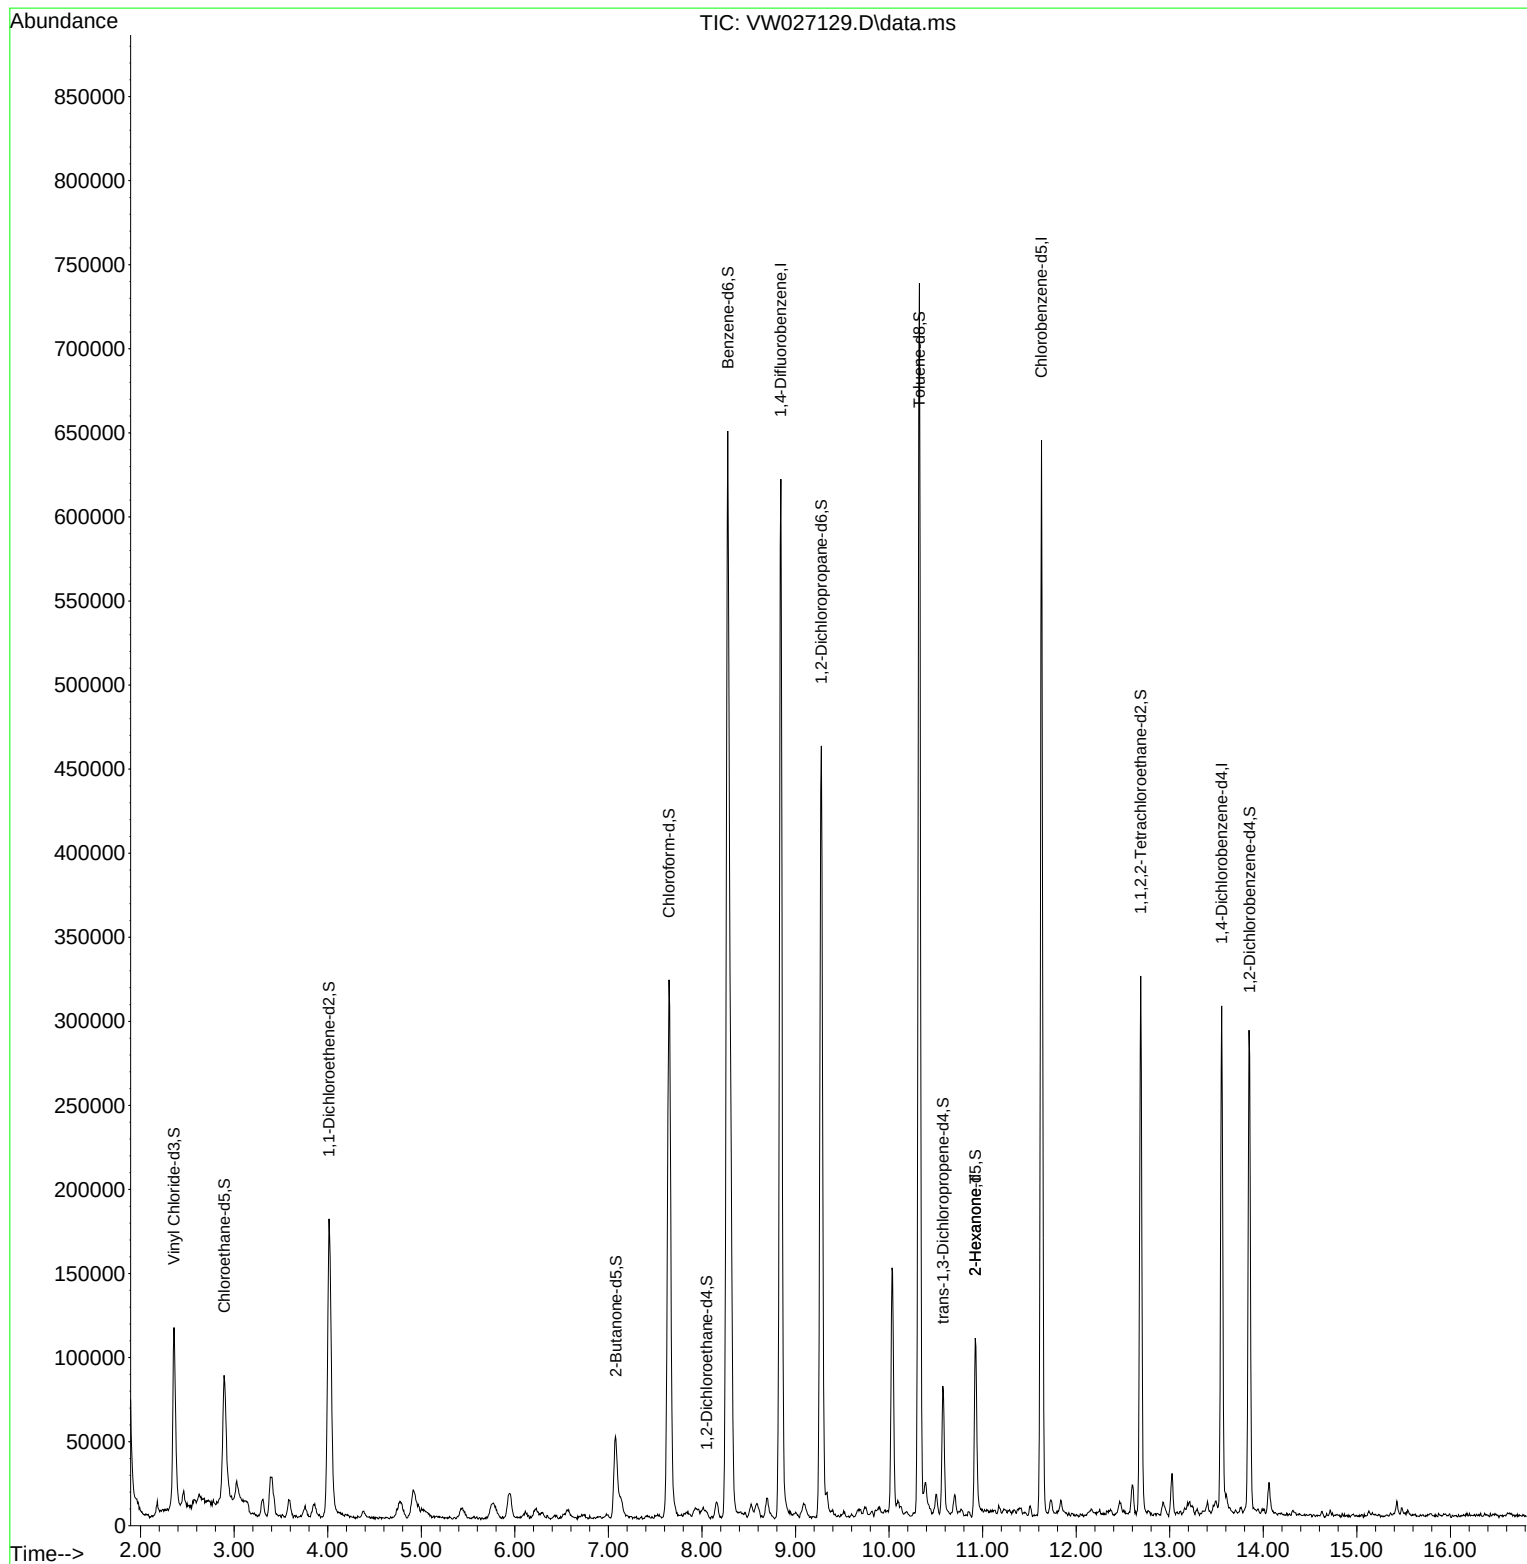

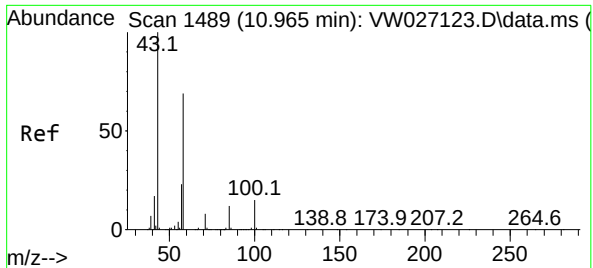

#48
 2-Hexanone
 Concen: 2.541 ug/L
 RT: 10.922 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW027129.D
 Acq: 18 Sep 2023 16:03

Instrument :
 MSVOA_W
 ClientSampleId :

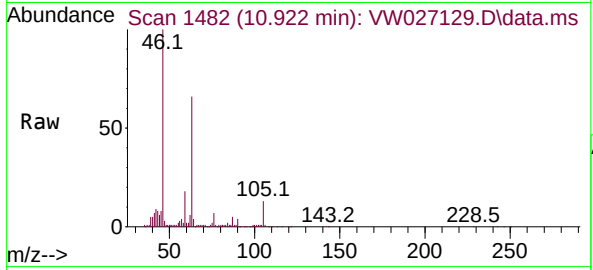

Tgt Ion: 43	Resp: 4829
Ion Ratio	Lower Upper
43 100	
58 35.8	51.4 77.0#
57 52.0	17.2 25.8#
100 6.8	12.2 18.2#

