
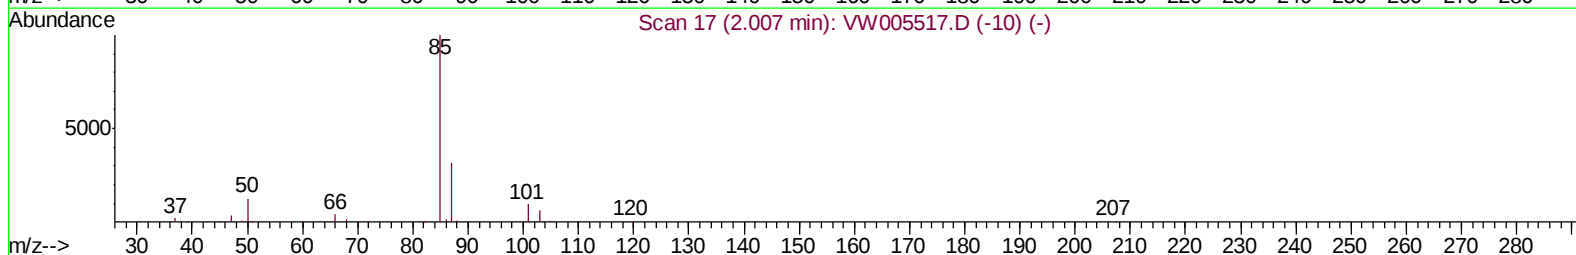
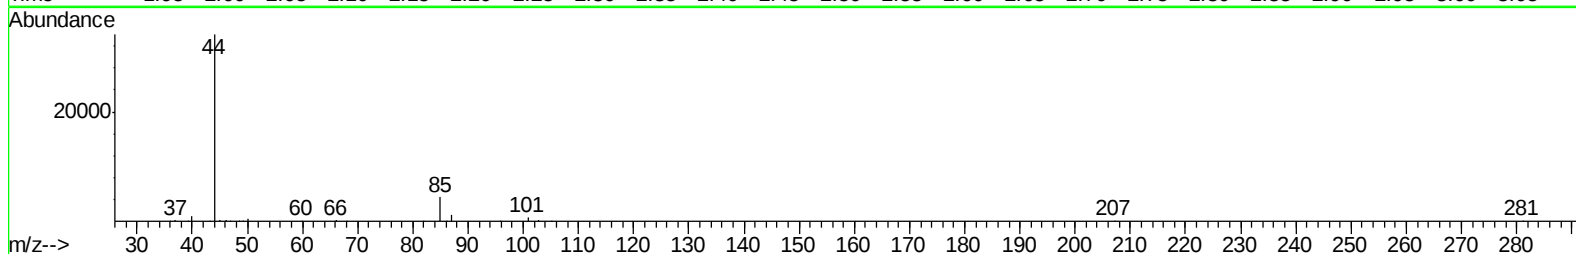


Data File : VW005521.D
Acq On : 19 Sep 2018 17:59
Operator : SY/AP
Sample : VSTD2.596
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 07:59:14 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091918S.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 19 17:31:20 2018
Response via : Initial Calibration

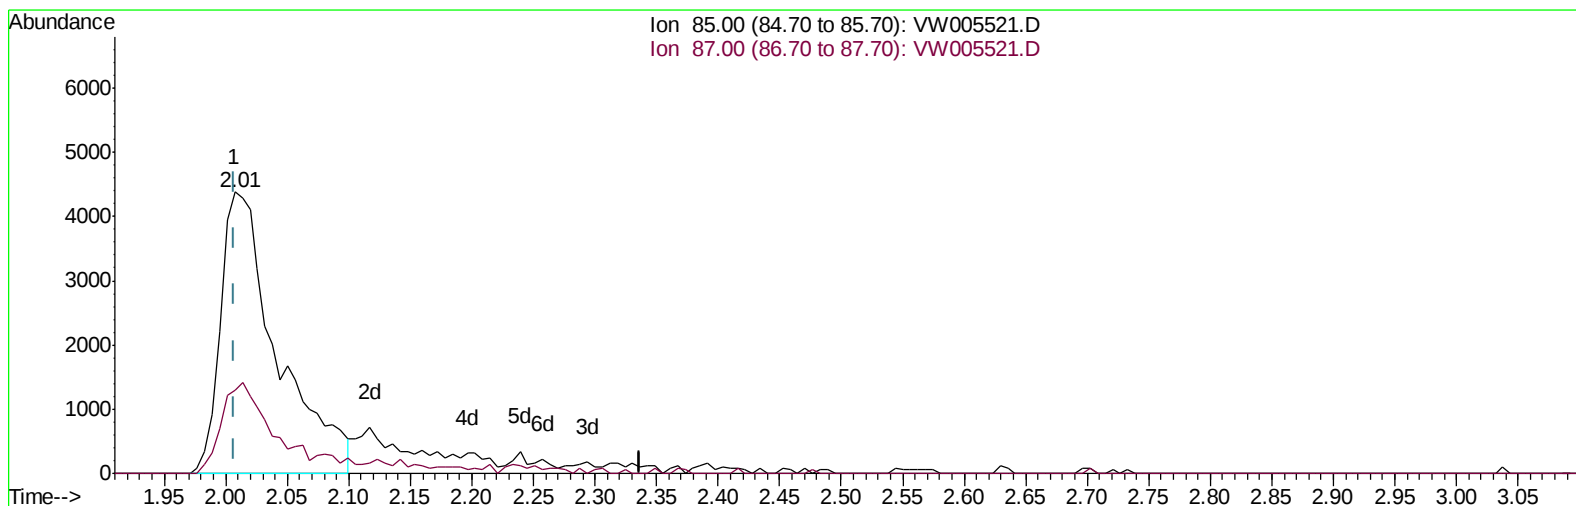

TIC: VW005521.D

(2) Dichlorodifluoromethane (T)

2.007min (+0.000) 2.87ug/L m

response 13927

Ion	Exp%	Act%
85.00	100	100
87.00	30.30	25.52
0.00	0.00	0.00
0.00	0.00	0.00