

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027143.D
 Acq On : 19 Sep 2023 11:57
 Operator : SY/MD
 Sample : 04472-02RE
 Misc : 5.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 20 01:35:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	651164	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	568713	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	191317	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	154666	14.763	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.040%
7) Chloroethane-d5	2.899	69	113526	14.032	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.120%
11) 1,1-Dichloroethene-d2	4.021	65	74679	16.626	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.520%
21) 2-Butanone-d5	7.081	46	87103	44.899	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.800%
24) Chloroform-d	7.648	84	421609	21.551	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.200%
26) 1,2-Dichloroethane-d4	8.307	65	211210	22.126	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.520%
32) Benzene-d6	8.276	84	844628	22.997	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.000%
36) 1,2-Dichloropropane-d6	9.276	67	258892	24.912	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.640%
41) Toluene-d8	10.325	98	685504	20.971	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.880%
43) trans-1,3-Dichloroprop...	10.575	79	80430	19.152	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.600%
47) 2-Hexanone-d5	10.922	63	58328	46.578	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.160%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	244524	29.365	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	117.480%
66) 1,2-Dichlorobenzene-d4	13.848	152	180072	26.356	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.440%
Target Compounds					Qvalue	
13) Acetone	4.124	43	10555	5.759	ug/L	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
Data File : VW027143.D
Acq On : 19 Sep 2023 11:57
Operator : SY/MD
Sample : 04472-02RE
Misc : 5.33g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 20 01:35:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 20 01:34:37 2023
Response via : Initial Calibration

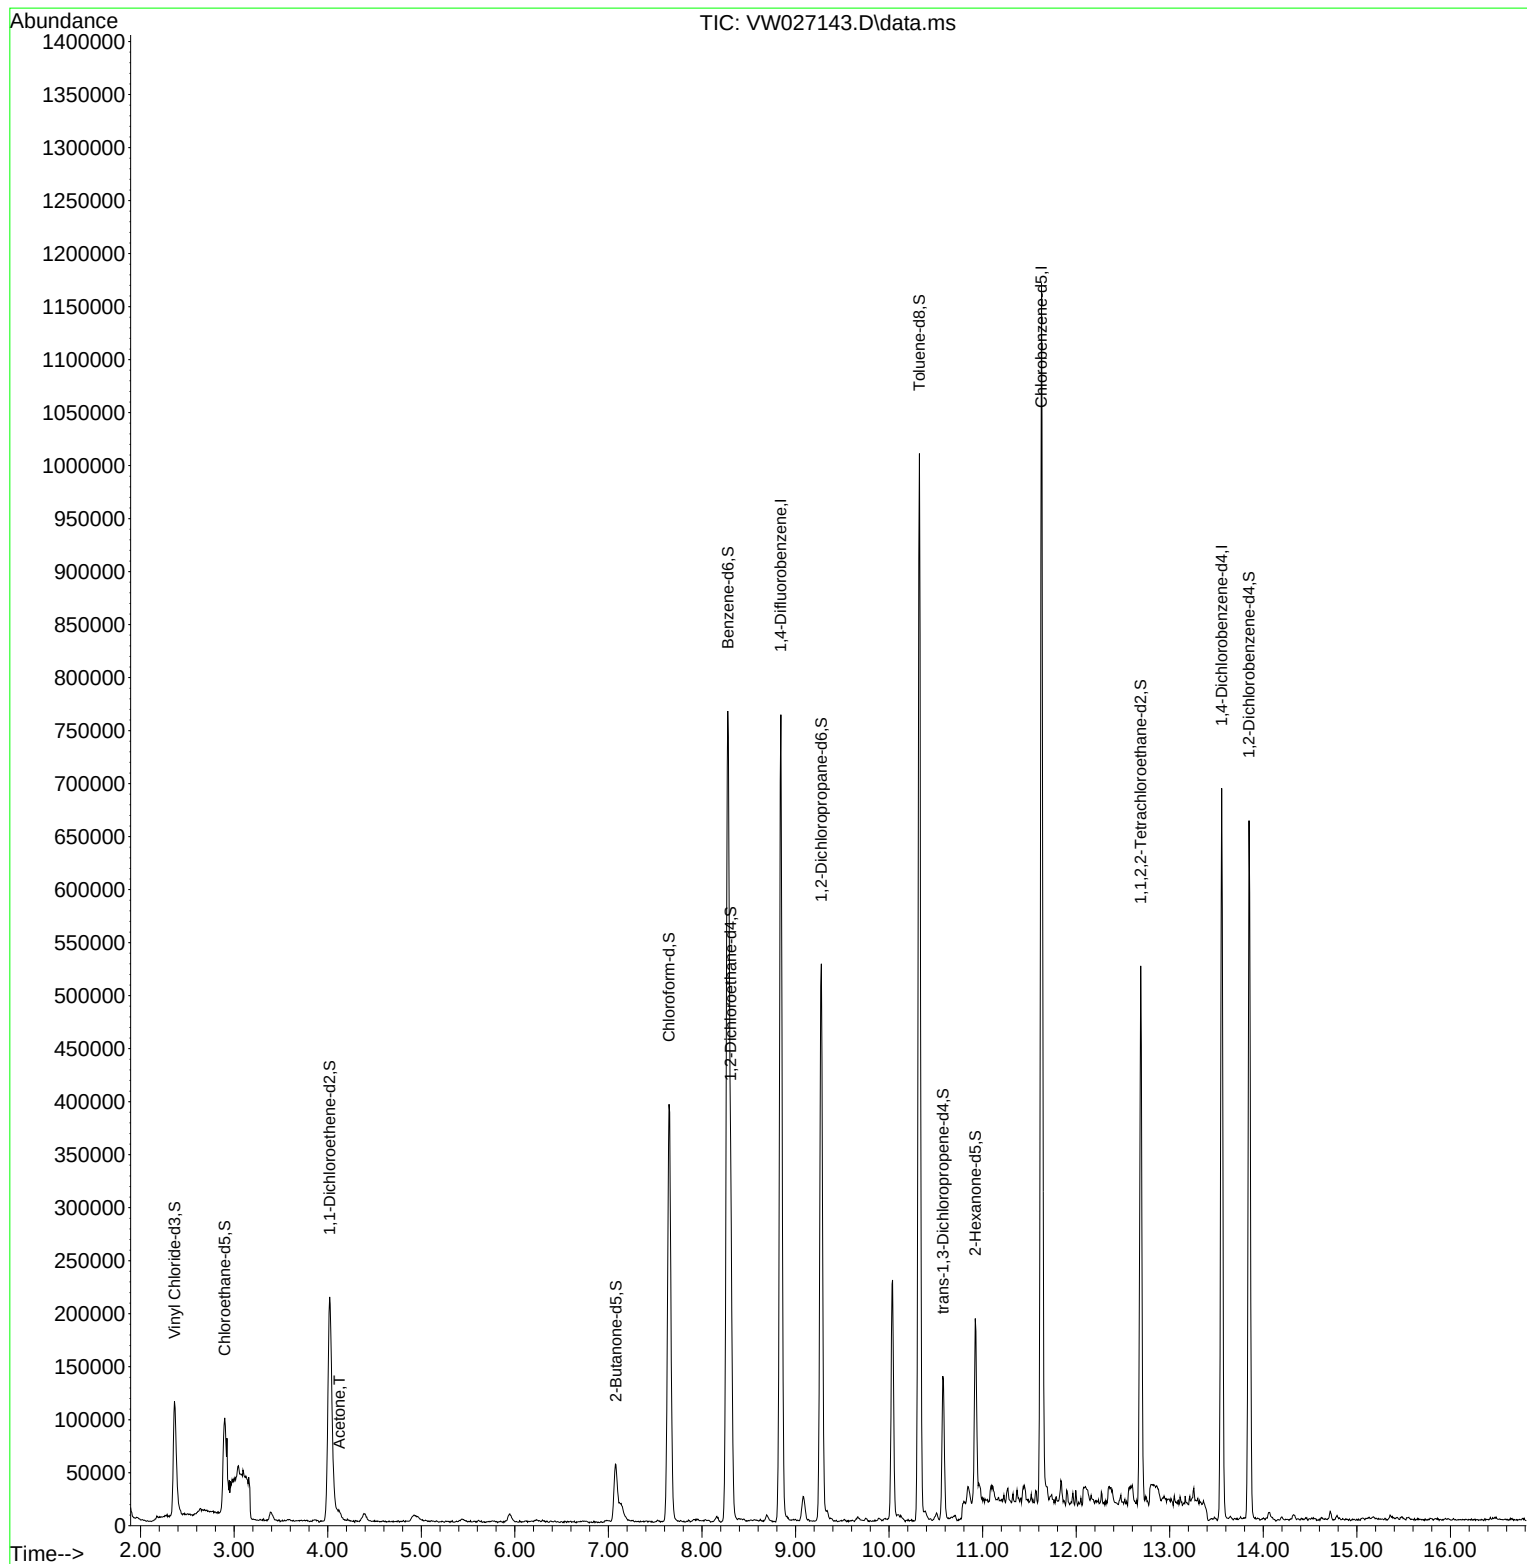

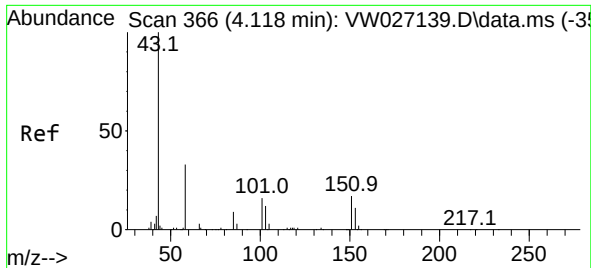

#13
 Acetone
 Concen: 5.759 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW027143.D
 Acq: 19 Sep 2023 11:57

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 43 Resp: 10555
 Ion Ratio Lower Upper
 43 100
 58 19.2 0.0 77.4

