

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027157.D
 Acq On : 19 Sep 2023 19:03
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 20 01:39:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	631948	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	636095	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	349086	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	233498	22.965	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.840%
7) Chloroethane-d5	2.899	69	178791	22.770	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.080%
11) 1,1-Dichloroethene-d2	4.021	65	77252	17.721	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.880%
21) 2-Butanone-d5	7.075	46	99957	53.092	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.180%
24) Chloroform-d	7.648	84	349797	18.424	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.680%
26) 1,2-Dichloroethane-d4	8.215	65	226	0.024	ug/L	-0.09
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#
32) Benzene-d6	8.276	84	798159	19.430	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.720%
36) 1,2-Dichloropropane-d6	9.270	67	223004	19.185	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.760%
41) Toluene-d8	10.319	98	841954	23.029	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.120%
43) trans-1,3-Dichloroprop...	10.575	79	104664	22.283	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.120%
47) 2-Hexanone-d5	10.922	63	73880	52.747	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.500%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	178108	19.124	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.480%
66) 1,2-Dichlorobenzene-d4	13.848	152	264396	21.208	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.840%
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	52361	4.355	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
Data File : VW027157.D
Acq On : 19 Sep 2023 19:03
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Sep 20 01:39:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 20 01:34:37 2023
Response via : Initial Calibration

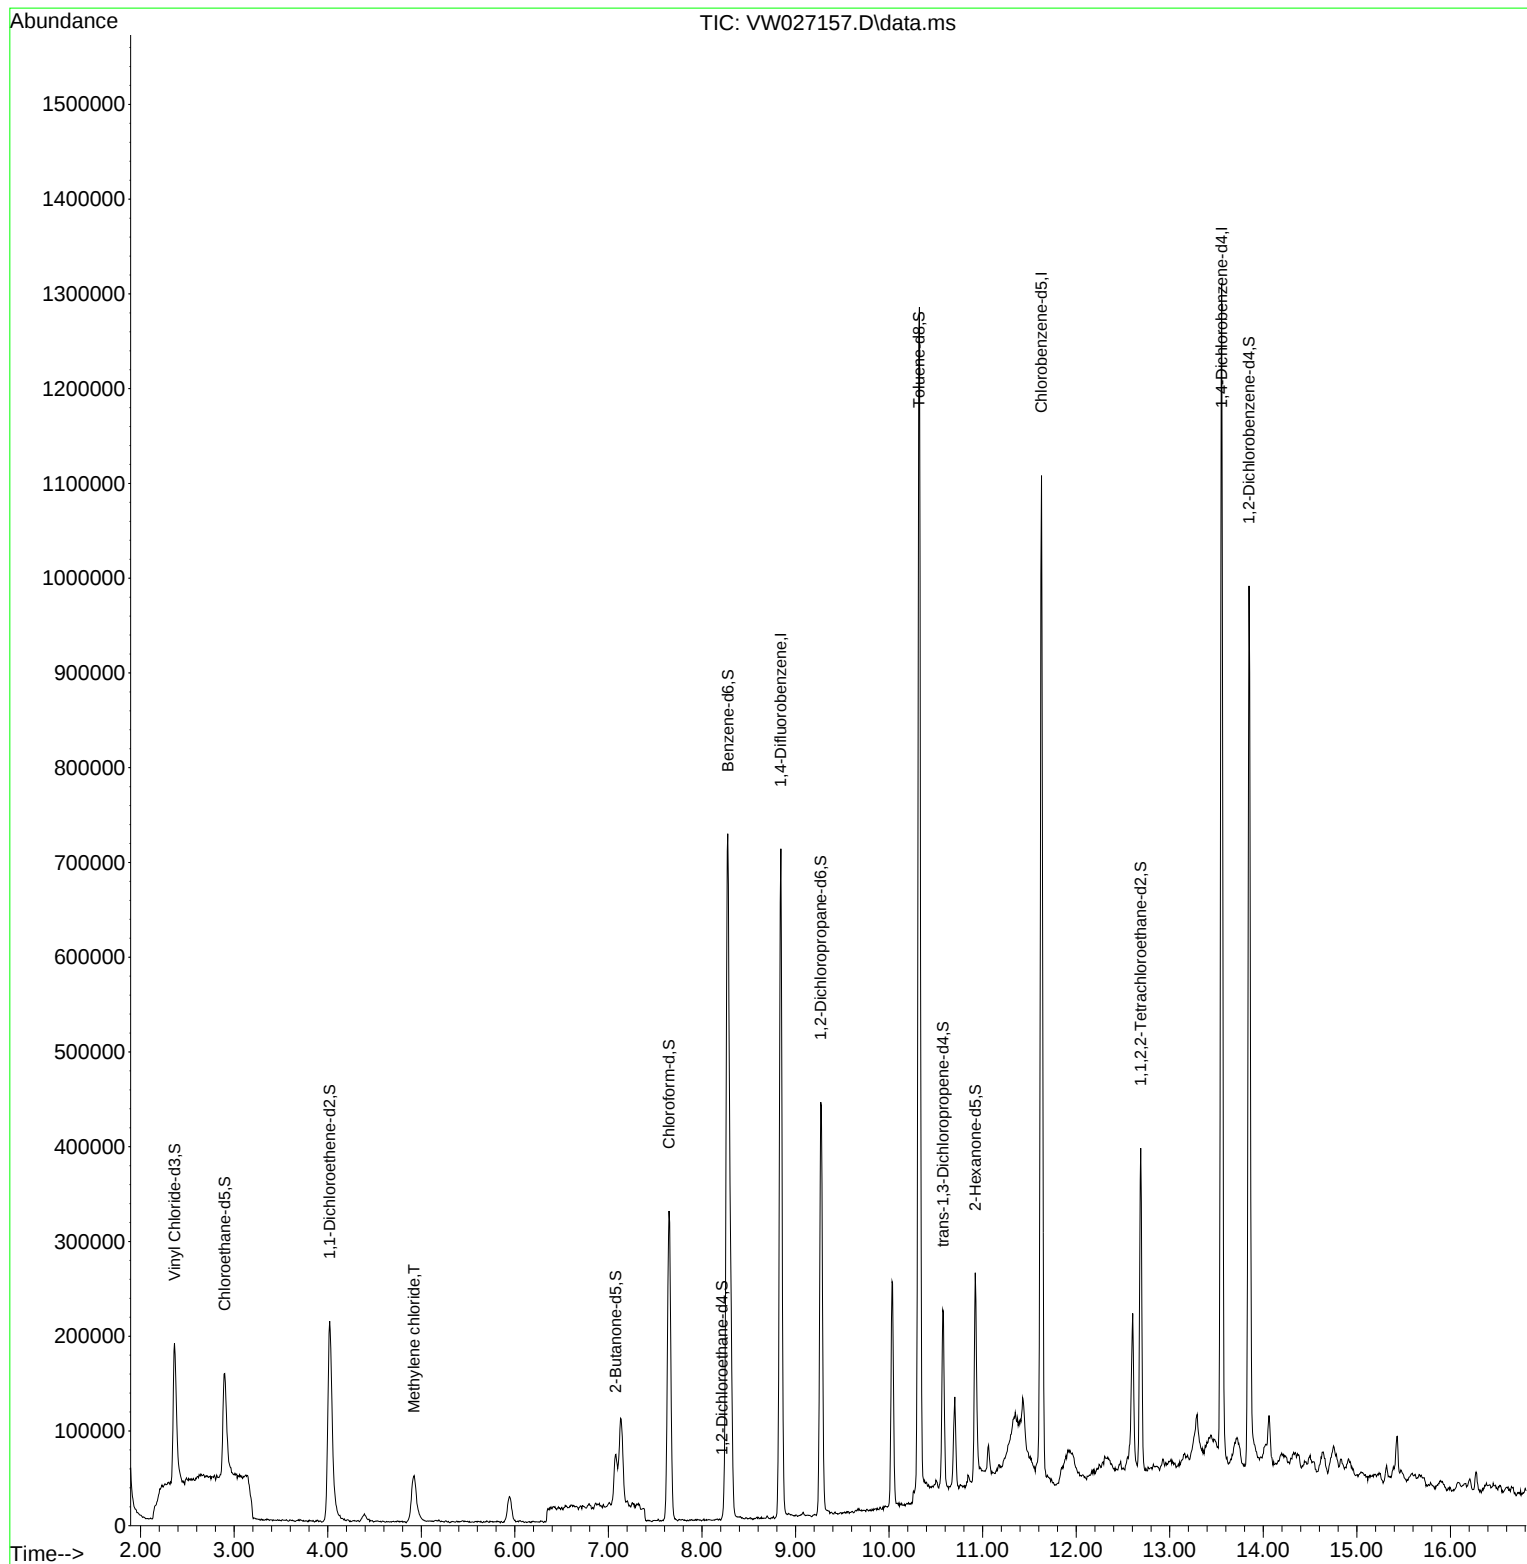

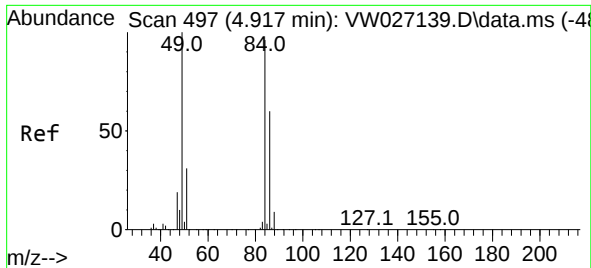

#16
Methylene chloride
Concen: 4.355 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW027157.D
Acq: 19 Sep 2023 19:03

Instrument :
MSVOA_W
ClientSampleId :

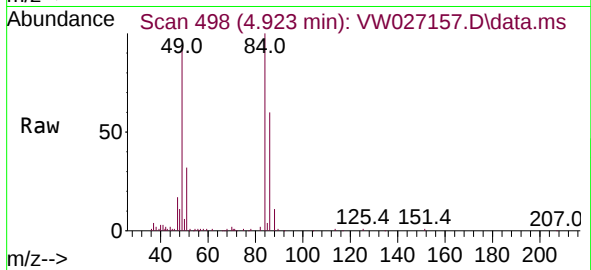

Tgt Ion: 84 Resp: 52361

Ion	Ratio	Lower	Upper
84	100		
86	59.6	46.7	86.7
49	92.6	77.1	143.1

