




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027143.D
 Acq On : 19 Sep 2023 11:57
 Operator : SY/MD
 Sample : 04472-02RE
 Misc : 5.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYE9

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:35:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

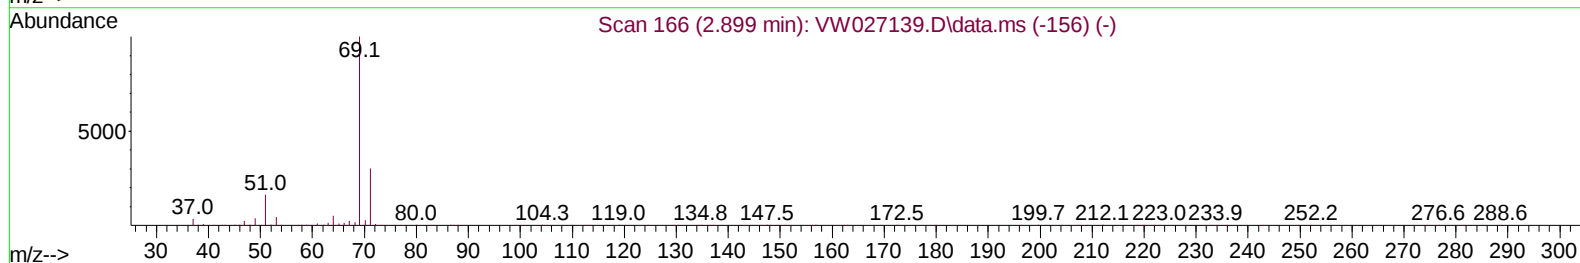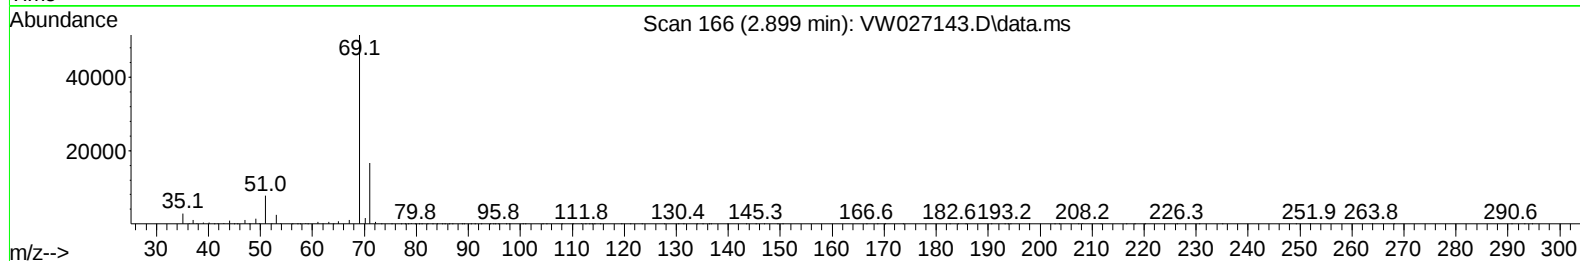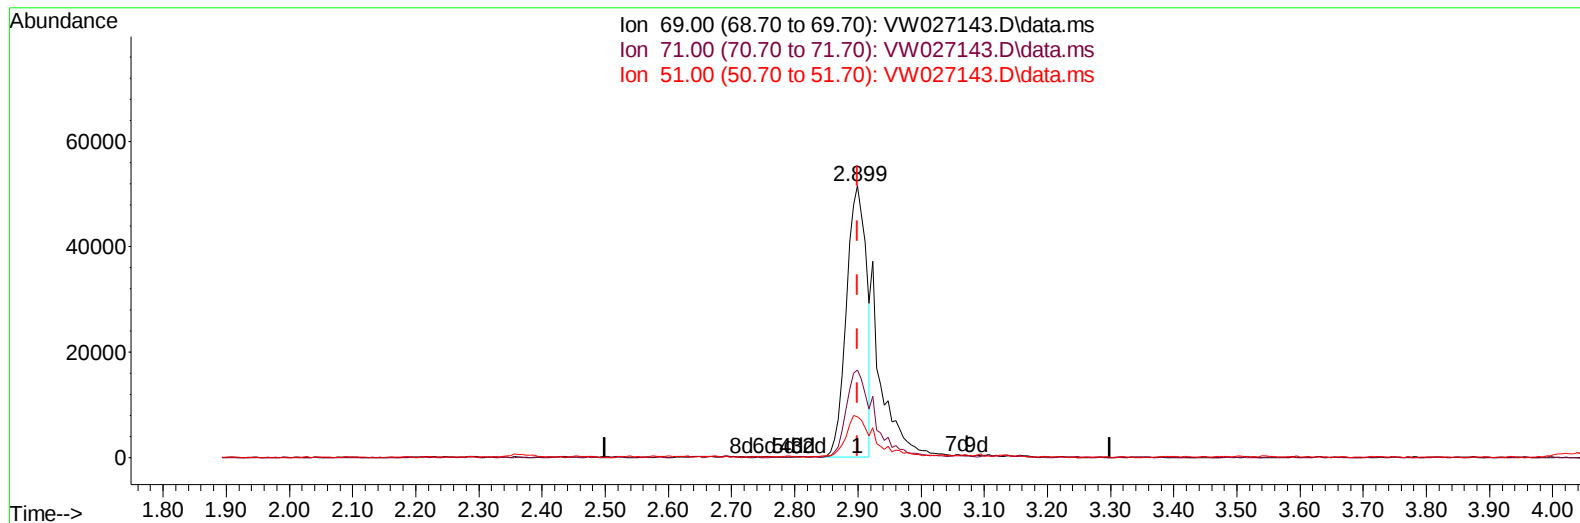

TIC: VW027143.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (0.000) 14.03 ug/L

response 113526

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.60	31.87
51.00	8.40	14.76#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027143.D
 Acq On : 19 Sep 2023 11:57
 Operator : SY/MD
 Sample : 04472-02RE
 Misc : 5.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYE9

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:35:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

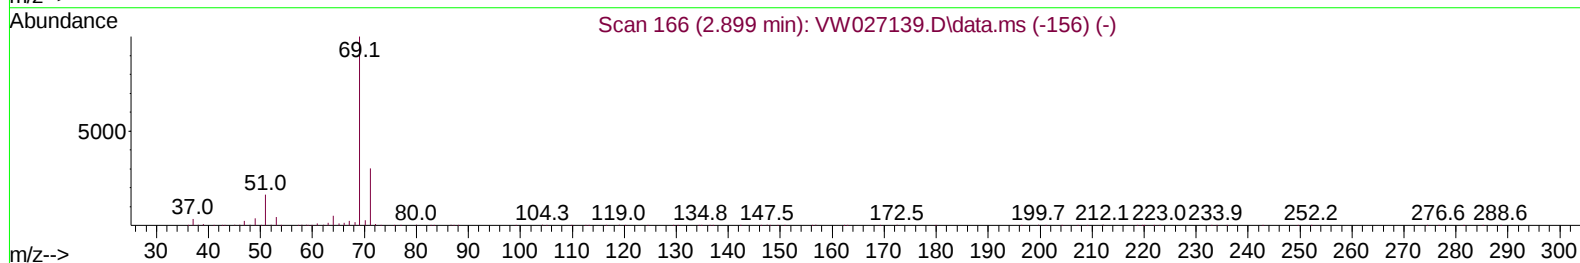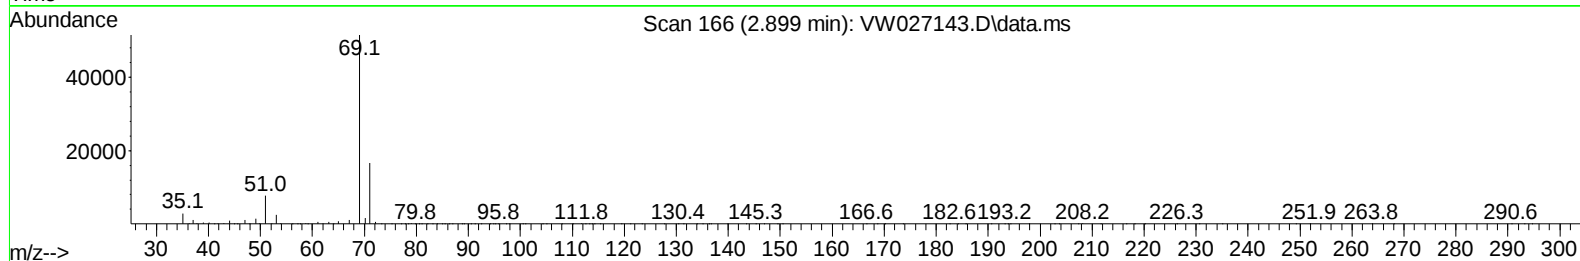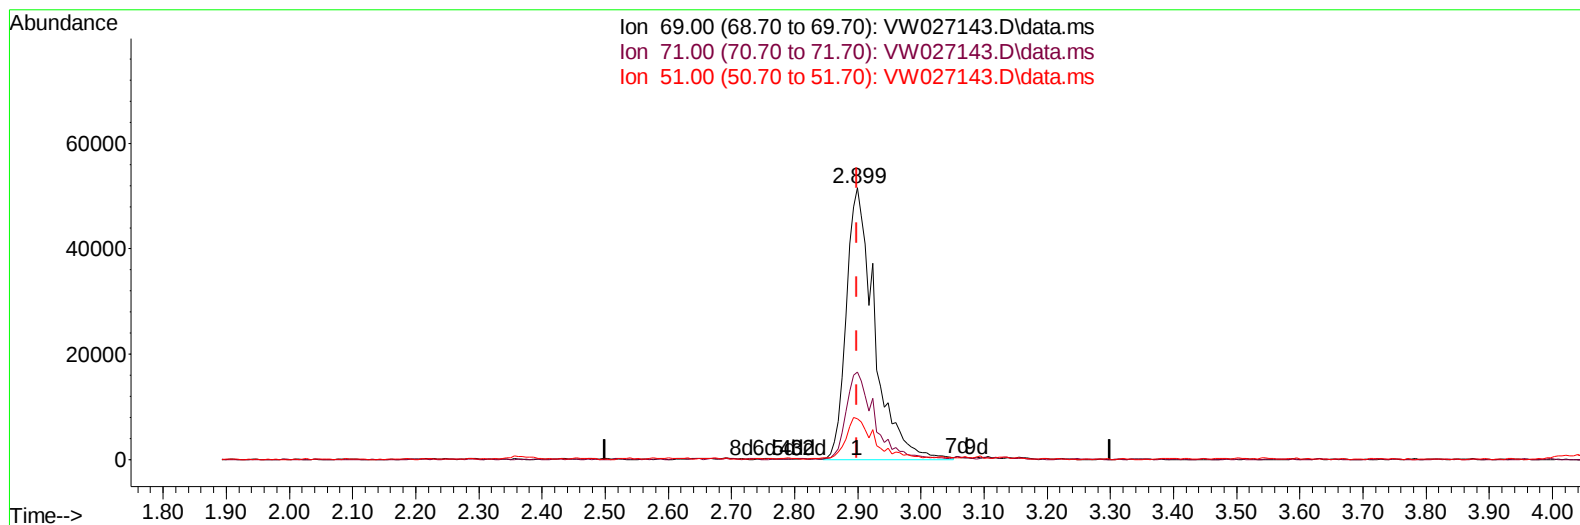

TIC: VW027143.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (0.000) 19.81 ug/L m

response 160312

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.60	22.57#
51.00	8.40	10.45
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
 Data File : VW027143.D
 Acq On : 19 Sep 2023 11:57
 Operator : SY/MD
 Sample : 04472-02RE
 Misc : 5.33g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYZE9

Manual IntegrationsAPPROVED

Quant Time: Sep 20 01:35:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 20 01:34:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/20/2023
 Supervised By :Mahesh Dadoda 09/20/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		651164	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		568713	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		191317	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		154666	14.763	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	59.040%		
7) Chloroethane-d5	2.899	69		160312m	19.814	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	79.240%		
11) 1,1-Dichloroethene-d2	4.021	65		74679	16.626	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	66.520%		
21) 2-Butanone-d5	7.081	46		87103	44.899	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	89.800%		
24) Chloroform-d	7.648	84		421609	21.551	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	86.200%		
26) 1,2-Dichloroethane-d4	8.307	65		211210	22.126	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	88.520%		
32) Benzene-d6	8.276	84		844628	22.997	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	92.000%		
36) 1,2-Dichloropropane-d6	9.276	67		258892	24.912	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	99.640%		
41) Toluene-d8	10.325	98		685504	20.971	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	83.880%		
43) trans-1,3-Dichloroprop...	10.575	79		80430	19.152	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	76.600%		
47) 2-Hexanone-d5	10.922	63		58328	46.578	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	93.160%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		244524	29.365	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	117.480%		
66) 1,2-Dichlorobenzene-d4	13.848	152		180072	26.356	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	105.440%		
Target Compounds							
13) Acetone	4.124	43		10555	5.759	ug/L	Qvalue 68

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091923\
Data File : VW027143.D
Acq On : 19 Sep 2023 11:57
Operator : SY/MD
Sample : 04472-02RE
Misc : 5.33g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZY9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/20/2023
Supervised By :Mahesh Dadoda 09/20/2023

Quant Time: Sep 20 01:35:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091823SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 20 01:34:37 2023
Response via : Initial Calibration

